




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
Data File : VW022960.D
Acq On : 10 May 2022 17:01
Operator : SY/VA
Sample : N2766-05
Misc : 7.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4F5

Manual IntegrationsAPPROVED

Quant Time: May 11 01:23:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 11 01:19:10 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/16/2022

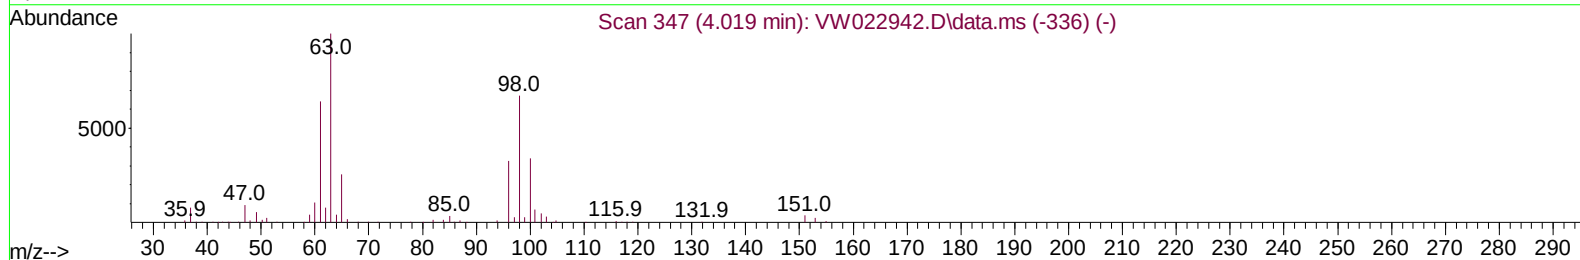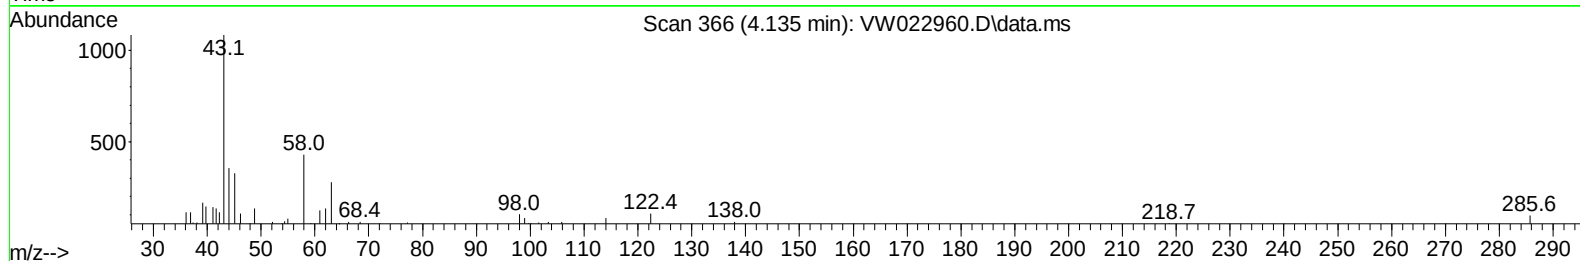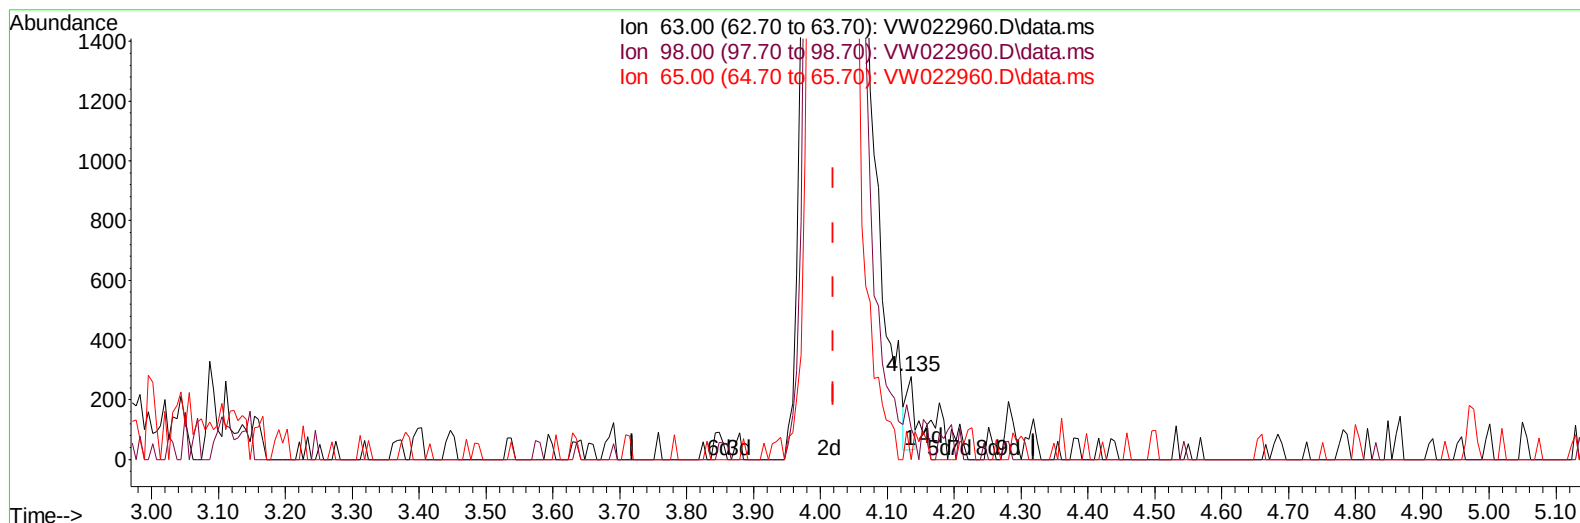

TIC: VW022960.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.135min (+ 0.116) 0.03 ug/L

response 182

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	71.43
65.00	23.30	19.23
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022960.D
 Acq On : 10 May 2022 17:01
 Operator : SY/VA
 Sample : N2766-05
 Misc : 7.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4F5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 11 01:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration

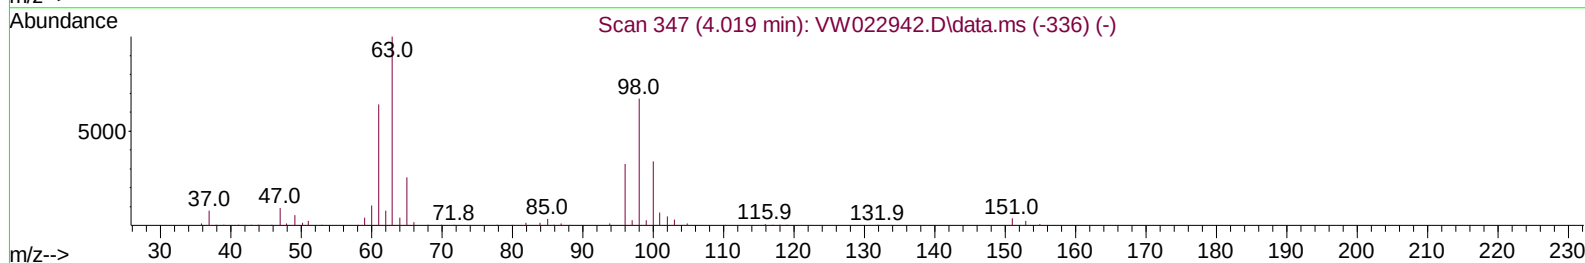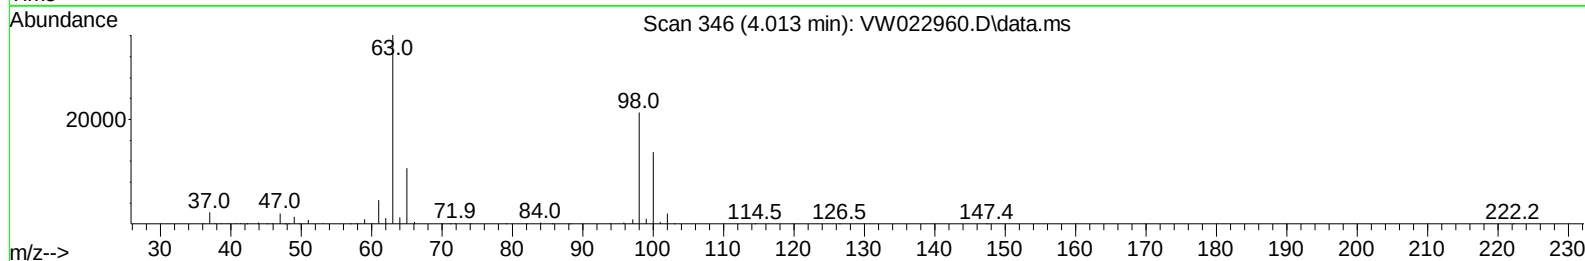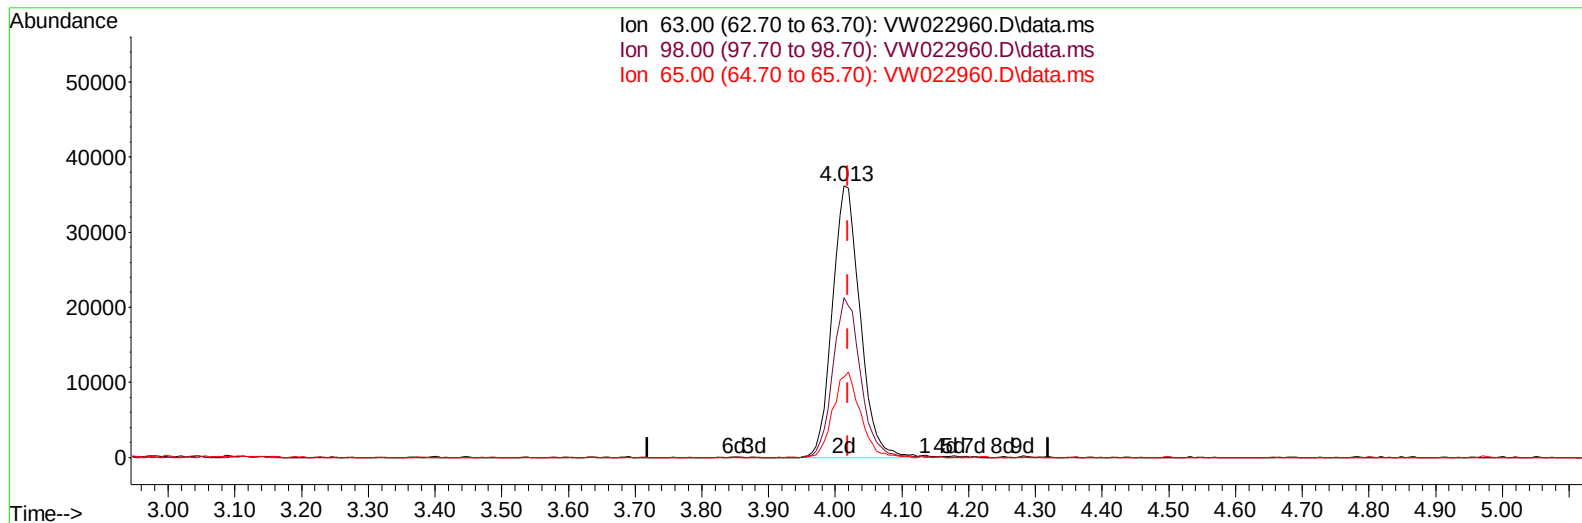

TIC: VW022960.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 18.21 ug/L m

response 104361

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.12#
65.00	23.30	0.03#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022960.D
 Acq On : 10 May 2022 17:01
 Operator : SY/VA
 Sample : N2766-05
 Misc : 7.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4F5

Manual IntegrationsAPPROVED

Quant Time: May 11 01:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/16/2022

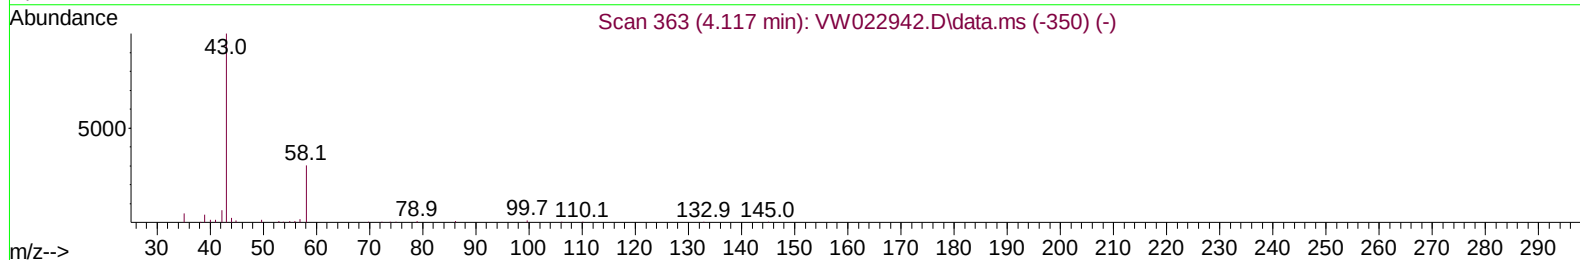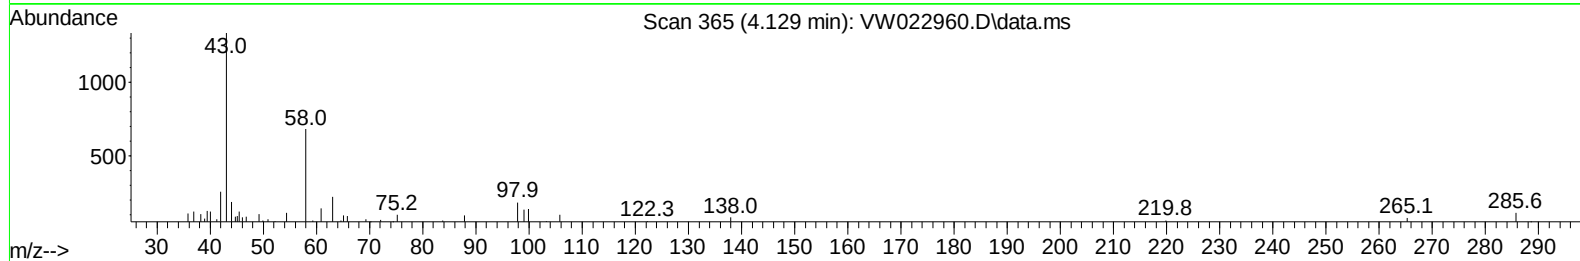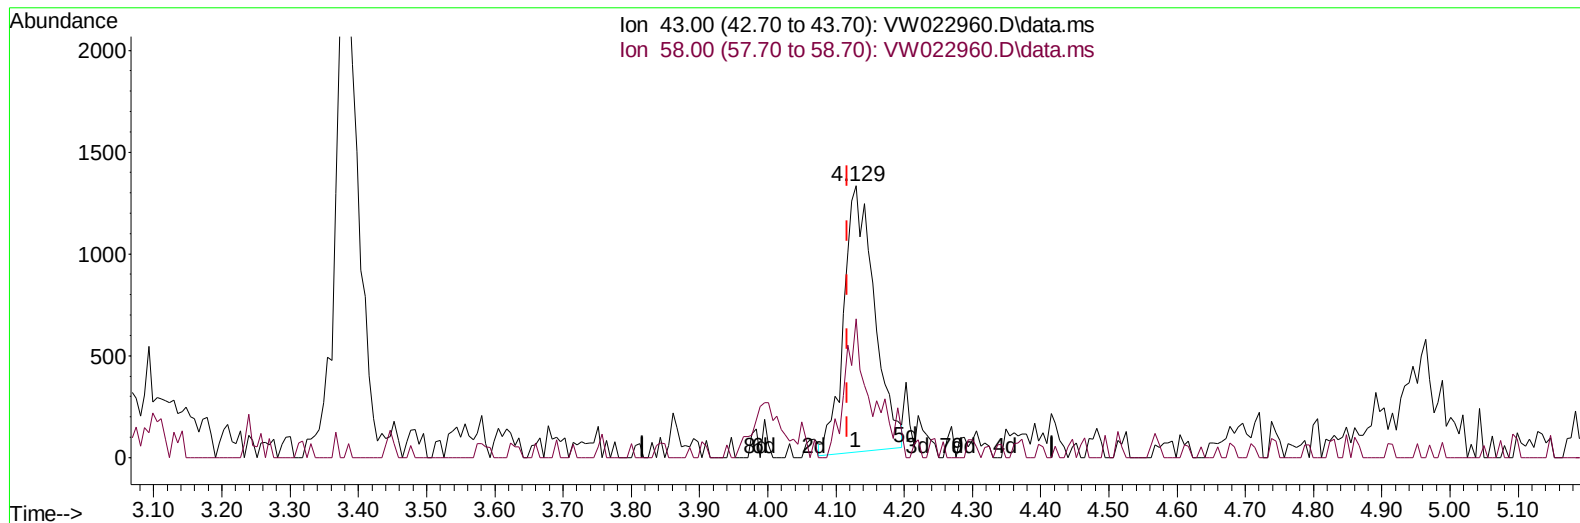

TIC: VW022960.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 6.47 ug/L

response 4083

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	21.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
Data File : VW022960.D
Acq On : 10 May 2022 17:01
Operator : SY/VA
Sample : N2766-05
Misc : 7.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4F5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 11 01:23:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 11 01:19:10 2022
Response via : Initial Calibration

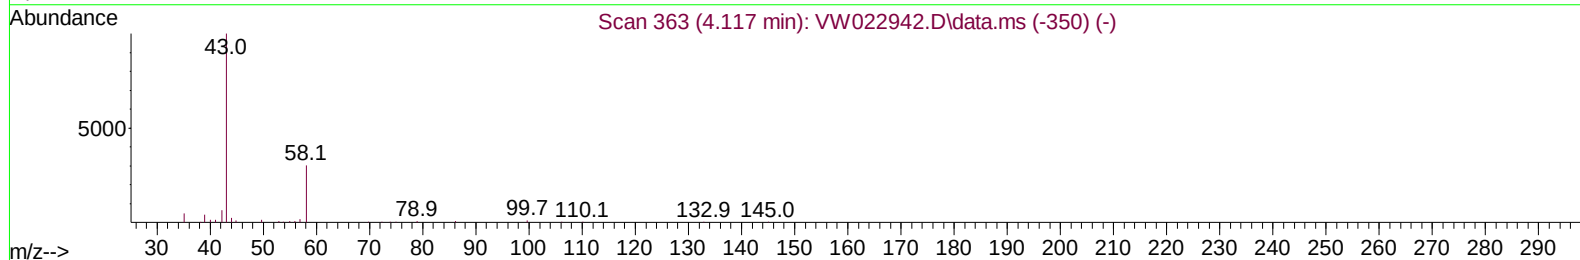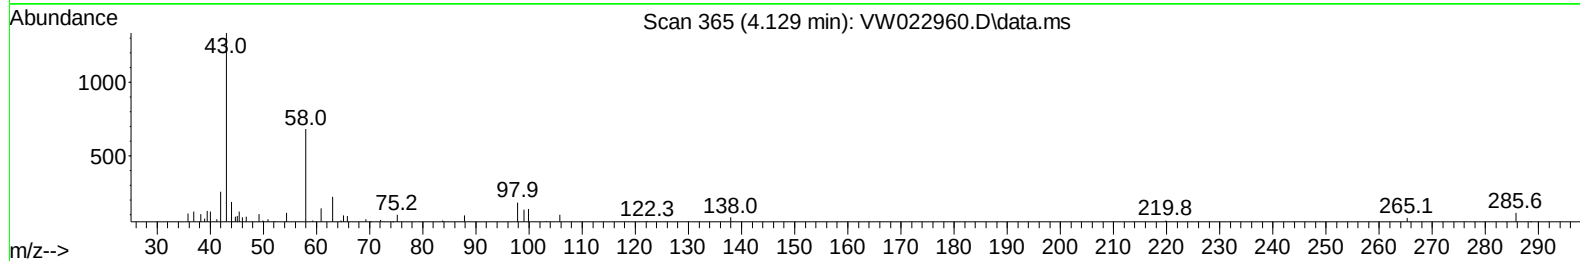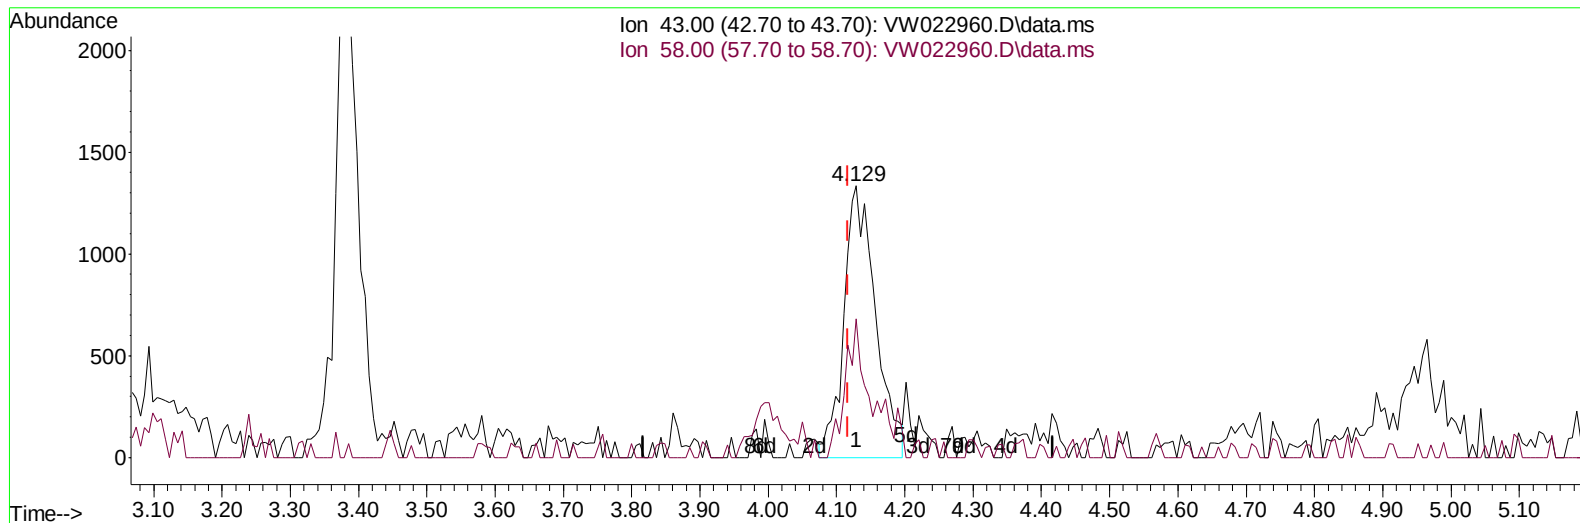

TIC: VW022960.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 6.80 ug/L m

response 4295

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	20.07
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022960.D
 Acq On : 10 May 2022 17:01
 Operator : SY/VA
 Sample : N2766-05
 Misc : 7.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4F5

Manual IntegrationsAPPROVED

Quant Time: May 11 01:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/16/2022

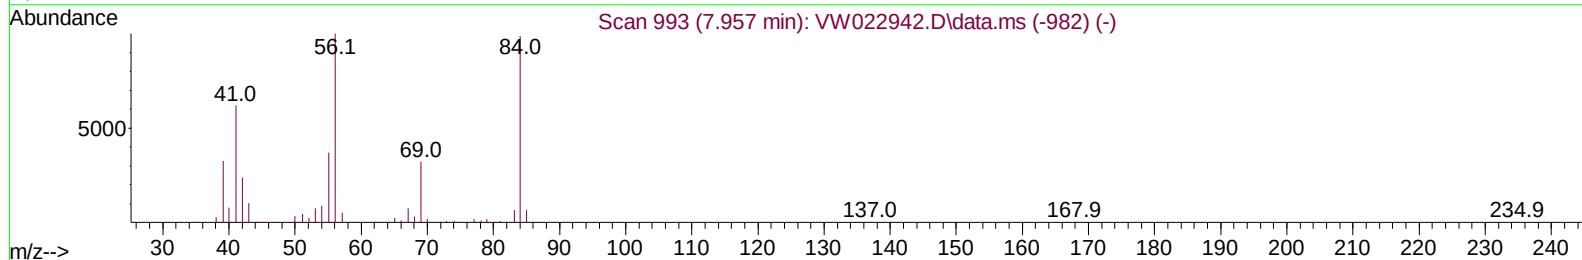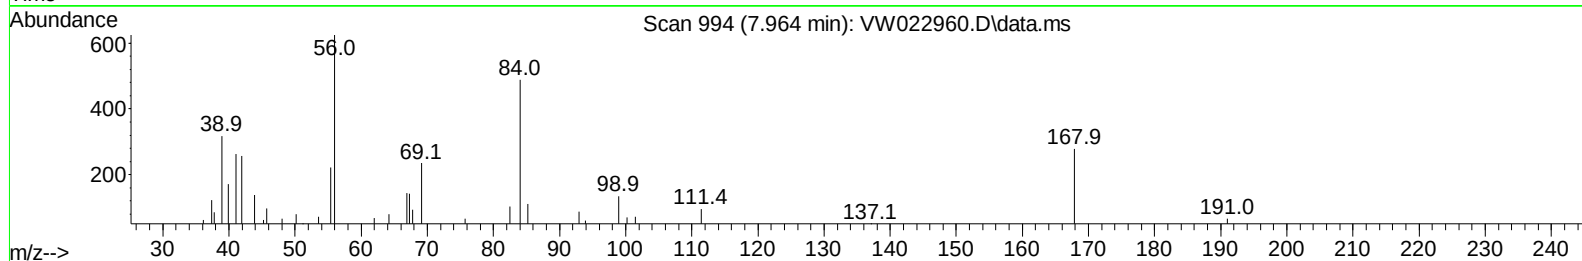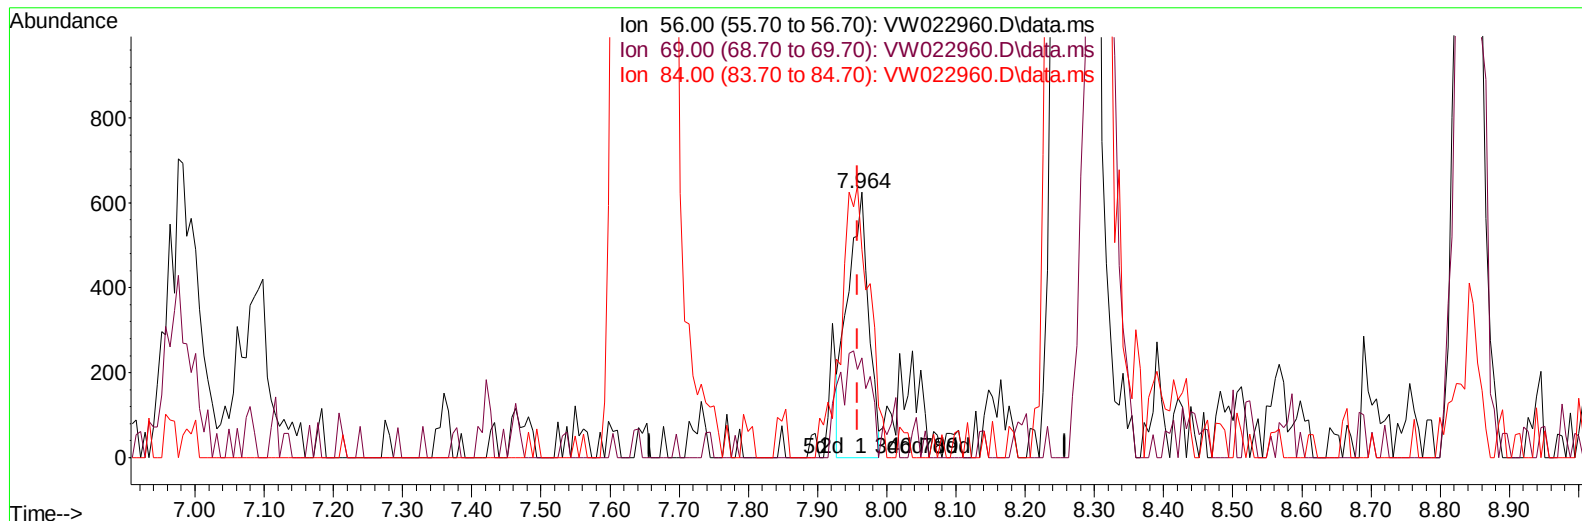

TIC: VW022960.D\data.ms

(29) Cyclohexane (T)

7.964min (+ 0.006) 0.61 ug/L

response 1325

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	32.00	39.25#
84.00	97.80	126.19#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
Data File : VW022960.D
Acq On : 10 May 2022 17:01
Operator : SY/VA
Sample : N2766-05
Misc : 7.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4F5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 11 01:23:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 11 01:19:10 2022
Response via : Initial Calibration

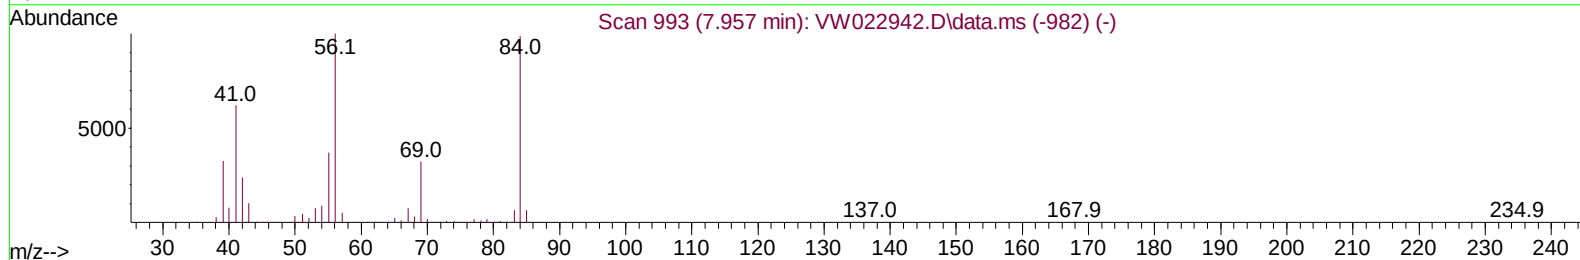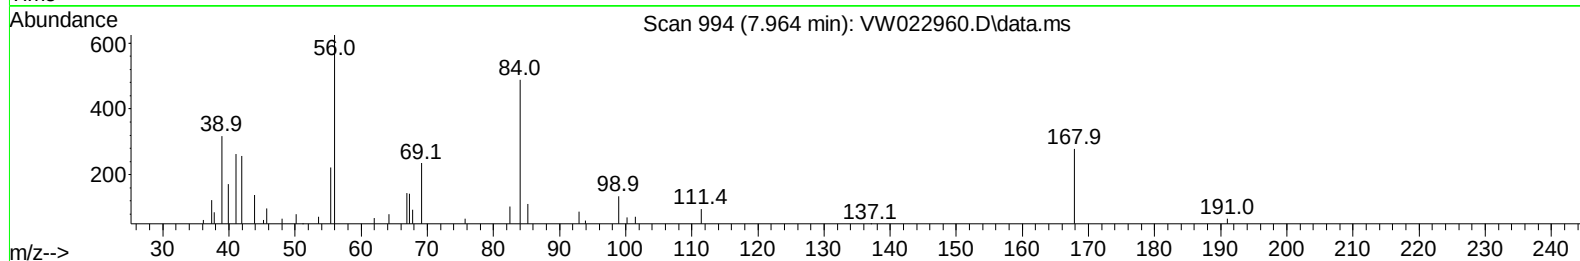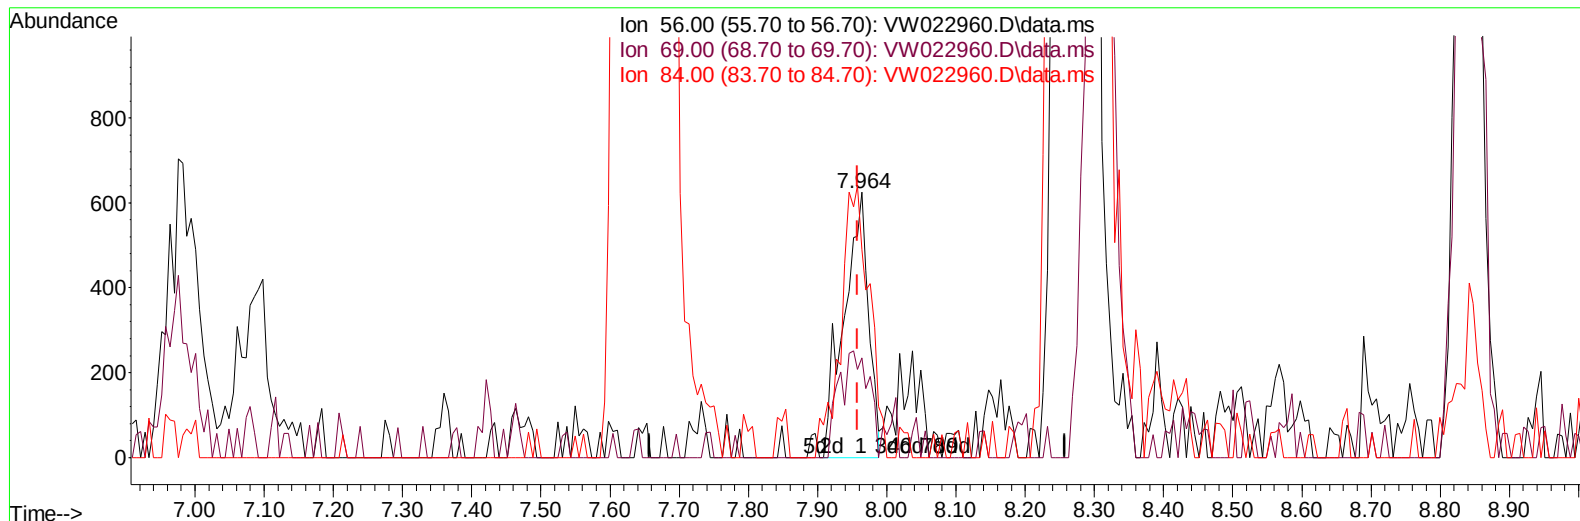

TIC: VW022960.D\data.ms

(29) Cyclohexane (T)

7.964min (+ 0.006) 0.72 ug/L m

response 1547

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	32.00	33.61
84.00	97.80	108.08
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022960.D
 Acq On : 10 May 2022 17:01
 Operator : SY/VA
 Sample : N2766-05
 Misc : 7.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4F5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
 Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 11 01:23:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		216236	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		99806	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		14763	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		115685	26.076	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery = 104.320%			
7) Chloroethane-d5	2.885	69		92272	31.970	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery = 127.880%			
11) 1,1-Dichloroethene-d2	4.013	63		104361m	18.206	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery = 72.840%			
21) 2-Butanone-d5	7.080	46		65463	77.609	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery = 155.220%#			
24) Chloroform-d	7.653	84		179327	28.306	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery = 113.240%			
26) 1,2-Dichloroethane-d4	8.305	65		100640	28.964	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery = 115.840%			
32) Benzene-d6	8.275	84		301288	52.373	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery = 209.480%#			
36) 1,2-Dichloropropane-d6	9.275	67		94725	58.618	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery = 234.480%#			
41) Toluene-d8	10.323	98		176809	31.816	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery = 127.280%			
43) trans-1,3-Dichloroprop...	10.579	79		20176	27.116	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery = 108.480%			
47) 2-Hexanone-d5	10.927	63		38640	125.257	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery = 250.520%#			
56) 1,1,2,2-Tetrachloroeth...	12.689	84		73019	48.479	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery = 193.920%#			
66) 1,2-Dichlorobenzene-d4	13.853	152		15542	30.116	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery = 120.480%#			
Target Compounds							
13) Acetone	4.129	43		4295m	6.801	ug/L	
14) Carbon disulfide	4.379	76		7280	0.959	ug/L	98
29) Cyclohexane	7.964	56		1547m	0.717	ug/L	
42) Toluene	10.384	91		16815	2.552	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
Data File : VW022960.D
Acq On : 10 May 2022 17:01
Operator : SY/VA
Sample : N2766-05
Misc : 7.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4F5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/11/2022
Supervised By :Mahesh Dadoda 05/16/2022

Quant Time: May 11 01:23:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Wed May 11 01:19:10 2022
Response via : Initial Calibration

