

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022953.D
 Acq On : 10 May 2022 13:54
 Operator : SY/VA
 Sample : N2746-04
 Misc : 6.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSL0

Quant Time: May 11 01:22:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration


| Compound | R.T. | QIon | Response | Conc | Units | Dev(Min) |
|-------------------------------|--------|----------------|------------|---------|-------|----------|
| ----- | | | | | | |
| Internal Standards | | | | | | |
| 1) 1,4-Difluorobenzene | 8.842 | 114 | 369555 | 25.000 | ug/L | 0.00 |
| 28) Chlorobenzene-d5 | 11.628 | 117 | 345222 | 25.000 | ug/L | 0.00 |
| 58) 1,4-Dichlorobenzene-d4 | 13.554 | 152 | 157122 | 25.000 | ug/L | 0.00 |
| System Monitoring Compounds | | | | | | |
| 4) Vinyl Chloride-d3 | 2.349 | 65 | 115499 | 15.233 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 30 - 150 | Recovery = | 60.920% | | |
| 7) Chloroethane-d5 | 2.885 | 69 | 92143 | 18.680 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 30 - 150 | Recovery = | 74.720% | | |
| 11) 1,1-Dichloroethene-d2 | 4.013 | 63 | 126510 | 12.913 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 45 - 110 | Recovery = | 51.640% | | |
| 21) 2-Butanone-d5 | 7.080 | 46 | 66876 | 46.391 | ug/L | 0.00 |
| Spiked Amount | 50.000 | Range 20 - 135 | Recovery = | 92.780% | | |
| 24) Chloroform-d | 7.647 | 84 | 223868 | 20.677 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 40 - 150 | Recovery = | 82.720% | | |
| 26) 1,2-Dichloroethane-d4 | 8.305 | 65 | 126440 | 21.293 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 70 - 130 | Recovery = | 85.160% | | |
| 32) Benzene-d6 | 8.275 | 84 | 420835 | 21.149 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 20 - 135 | Recovery = | 84.600% | | |
| 36) 1,2-Dichloropropane-d6 | 9.275 | 67 | 128243 | 22.944 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 70 - 120 | Recovery = | 91.760% | | |
| 41) Toluene-d8 | 10.323 | 98 | 379421 | 19.739 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 30 - 130 | Recovery = | 78.960% | | |
| 43) trans-1,3-Dichloroprop... | 10.579 | 79 | 49476 | 19.224 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 30 - 135 | Recovery = | 76.880% | | |
| 47) 2-Hexanone-d5 | 10.927 | 63 | 52131 | 48.856 | ug/L | 0.00 |
| Spiked Amount | 50.000 | Range 20 - 135 | Recovery = | 97.720% | | |
| 56) 1,1,2,2-Tetrachloroeth... | 12.689 | 84 | 116512 | 22.364 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 45 - 120 | Recovery = | 89.440% | | |
| 66) 1,2-Dichlorobenzene-d4 | 13.853 | 152 | 127628 | 23.237 | ug/L | 0.00 |
| Spiked Amount | 25.000 | Range 75 - 120 | Recovery = | 92.960% | | |
| Target Compounds | | | | | | |
| 13) Acetone | 4.129 | 43 | 14341 | 13.287 | ug/L | 99 |
| ----- | | | | | | |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051022\
 Data File : VW022953.D
 Acq On : 10 May 2022 13:54
 Operator : SY/VA
 Sample : N2746-04
 Misc : 6.51g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 DBSL0


Quant Time: May 11 01:22:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed May 11 01:19:10 2022
 Response via : Initial Calibration

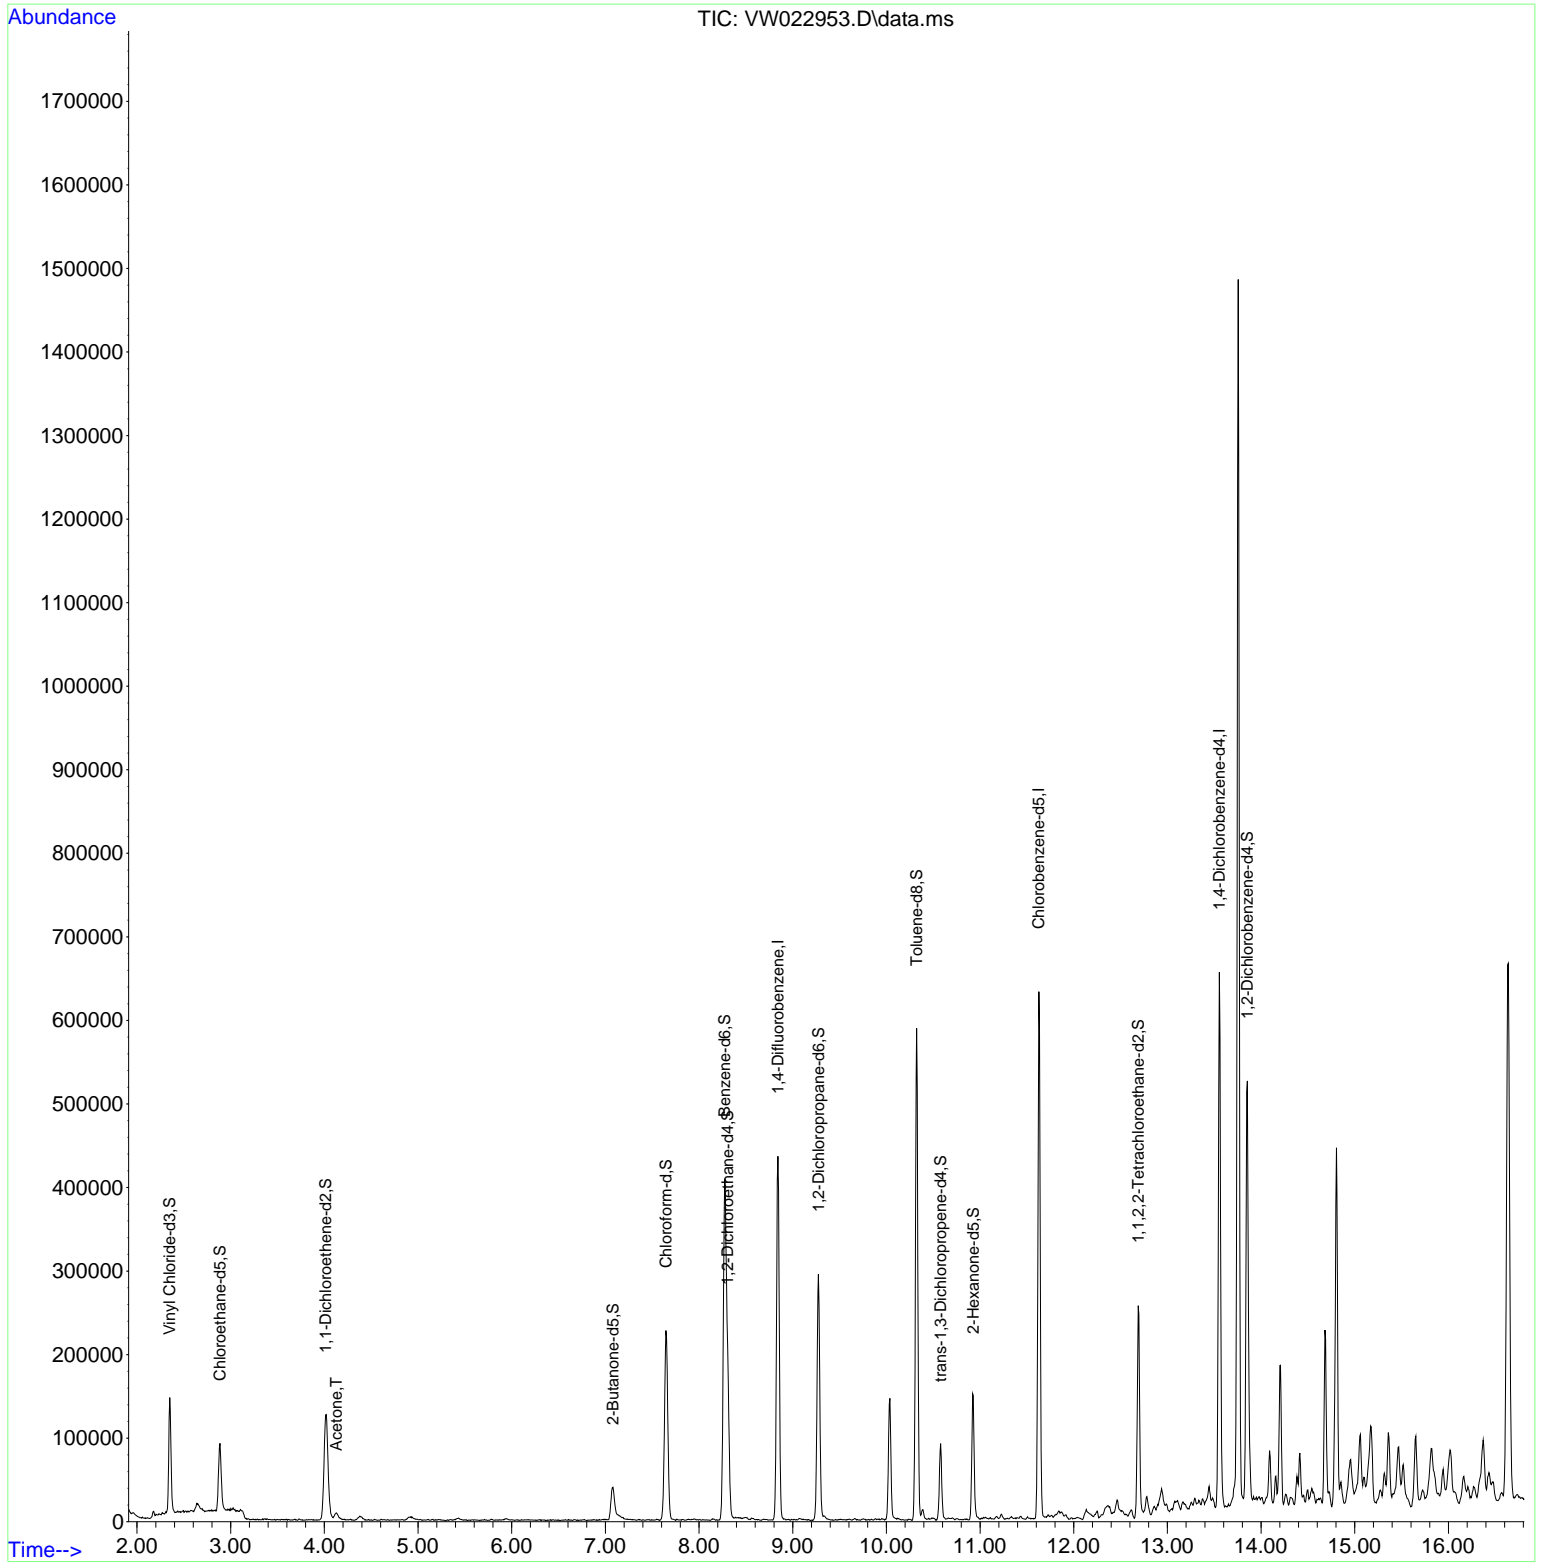

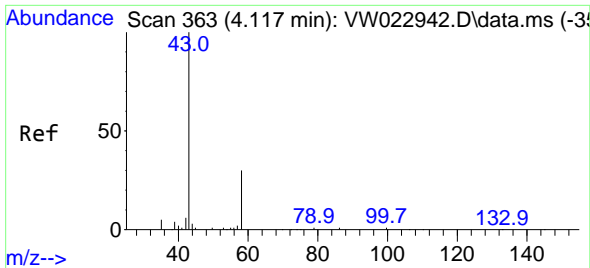

#13
 Acetone
 Concen: 13.287 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW022953.D
 Acq: 10 May 2022 13:54

Instrument :
 MSVOA_W
 ClientSampleId :
 DBSL0

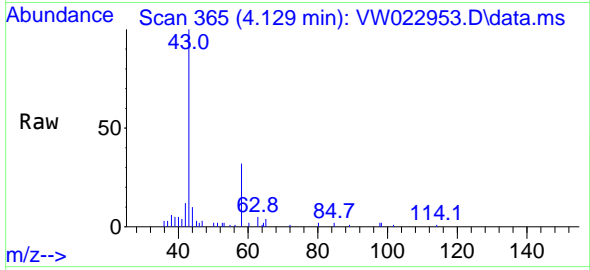

Tgt Ion: 43 Resp: 14341
 Ion Ratio Lower Upper
 43 100
 58 32.8 0.0 64.0

