


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW051119\
Data File : VW010375.D
Acq On : 11 May 2019 12:02
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W050919S.M
Title : SW846 8260
Last Update : Fri May 10 03:41:21 2019

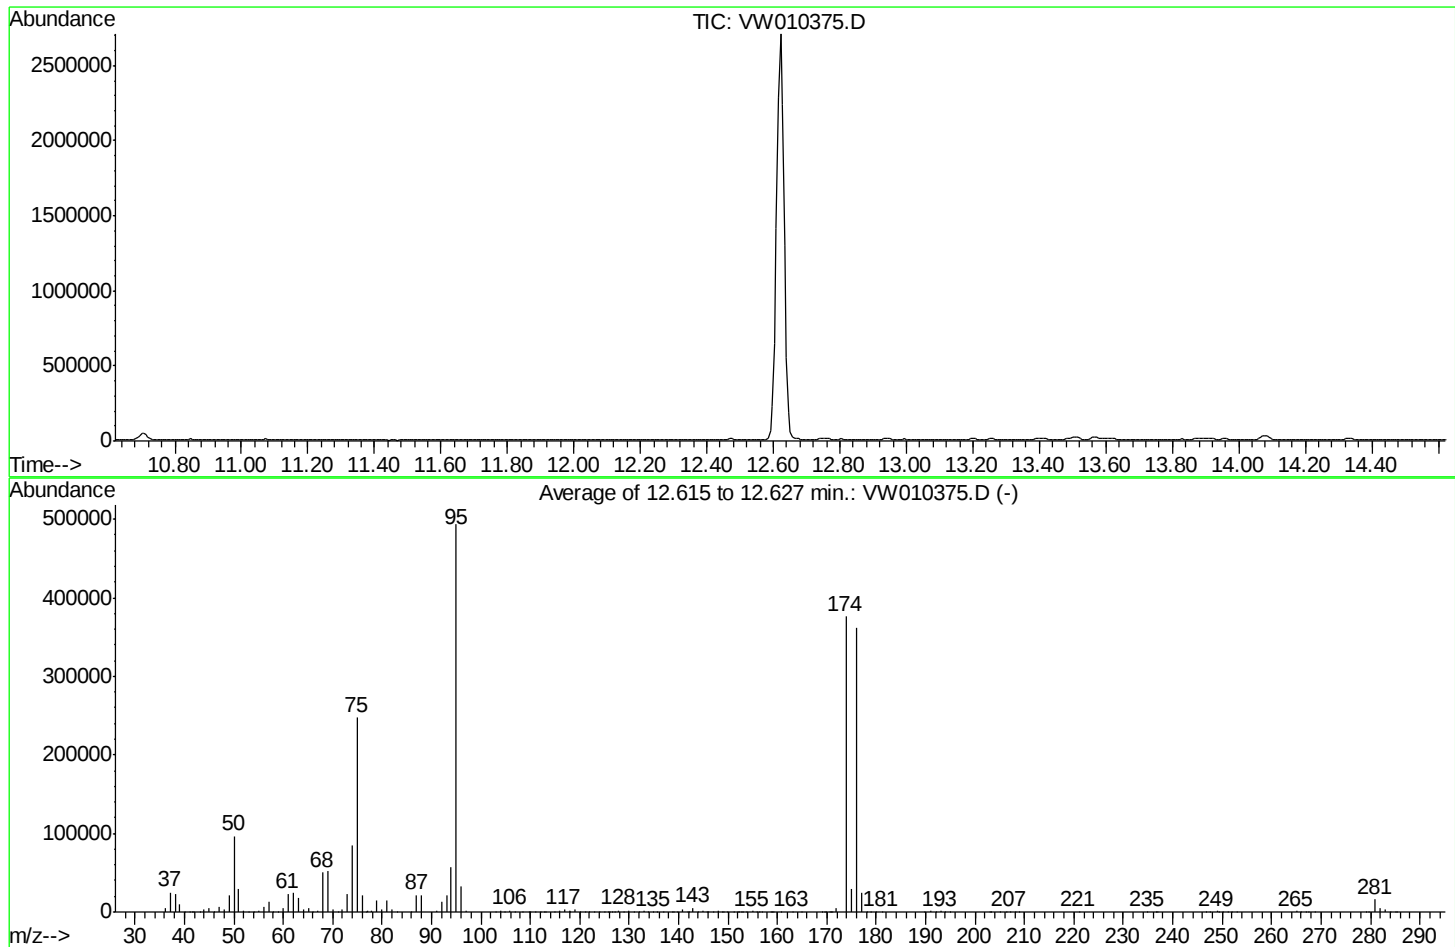

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	96861	PASS
75	95	30	60	50.1	247360	PASS
95	95	100	100	100.0	493482	PASS
96	95	5	9	6.6	32656	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	76.2	375808	PASS
175	174	5	9	8.0	29906	PASS
176	174	95	101	96.1	361002	PASS
177	176	5	9	6.7	24210	PASS