




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051123\
 Data File : VW025957.D
 Acq On : 11 May 2023 15:47
 Operator : SY/MD
 Sample : 02689-03
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/12/2023
 Supervised By :Mahesh Dadoda 05/12/2023

Quant Time: May 12 05:39:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

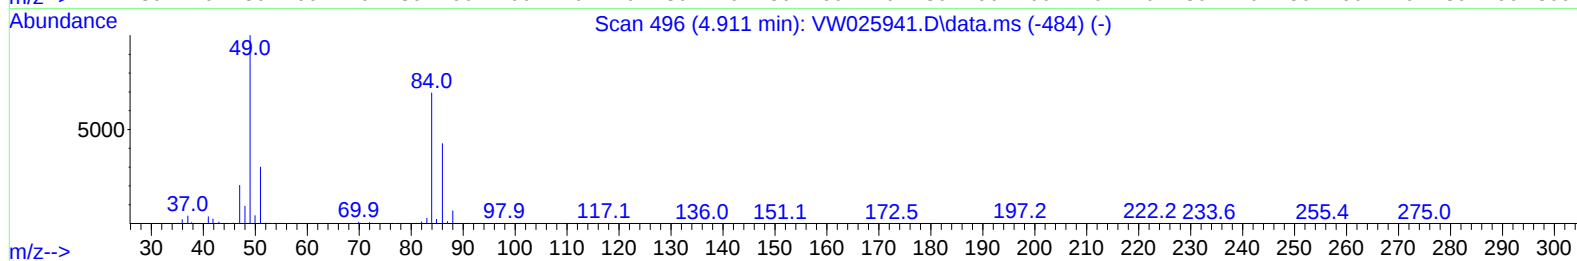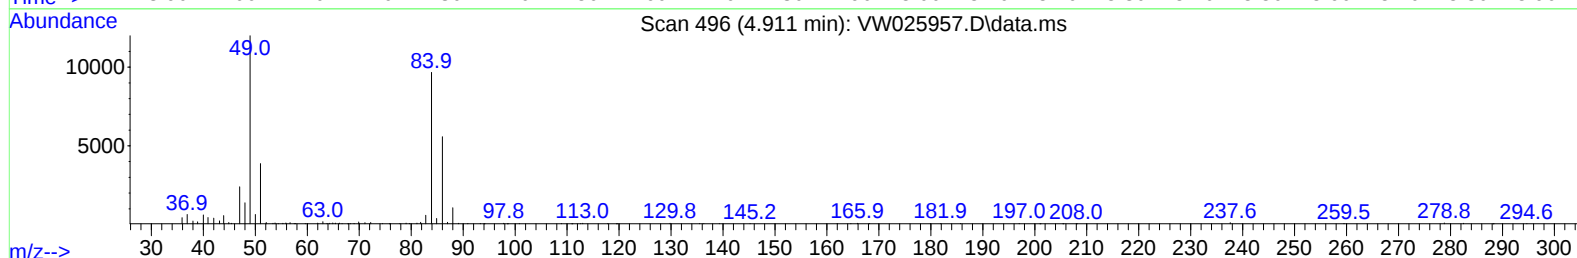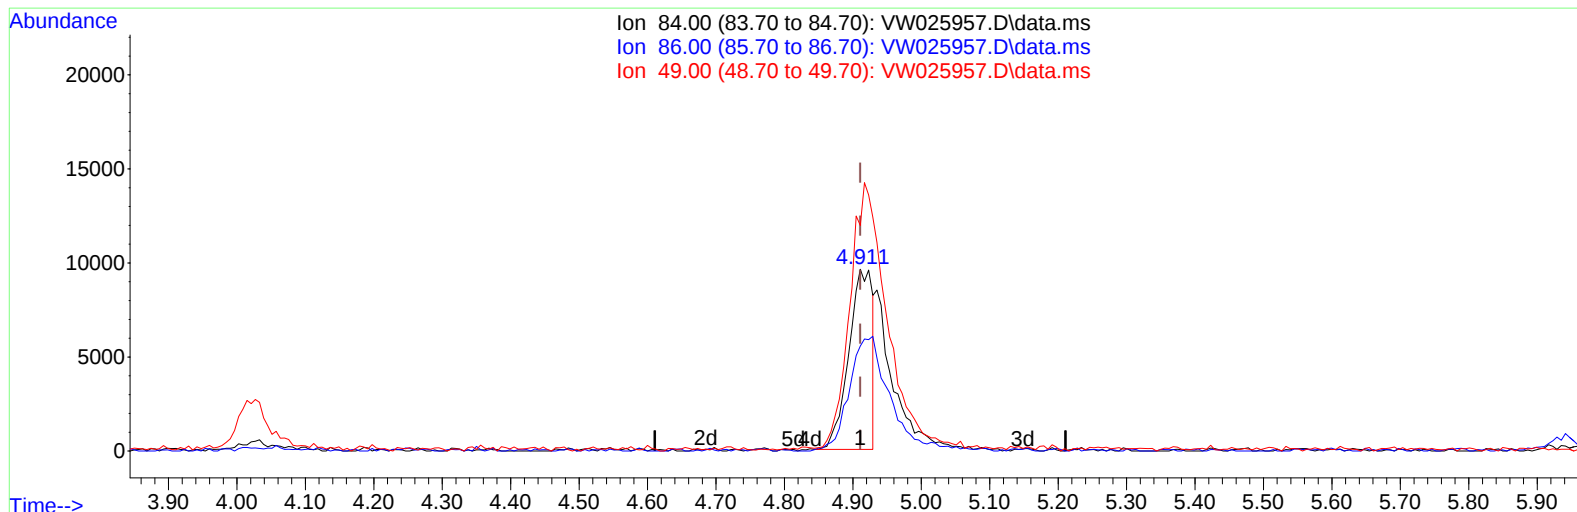

TIC: VW025957.D\data.ms

(16) Methylene chloride (T)

4.911min (-0.000) 1.79 ug/L

response 23093

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	59.60	57.78
49.00	136.20	124.10
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051123\
 Data File : VW025957.D
 Acq On : 11 May 2023 15:47
 Operator : SY/MD
 Sample : 02689-03
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/12/2023
 Supervised By :Mahesh Dadoda 05/12/2023

Quant Time: May 12 05:39:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

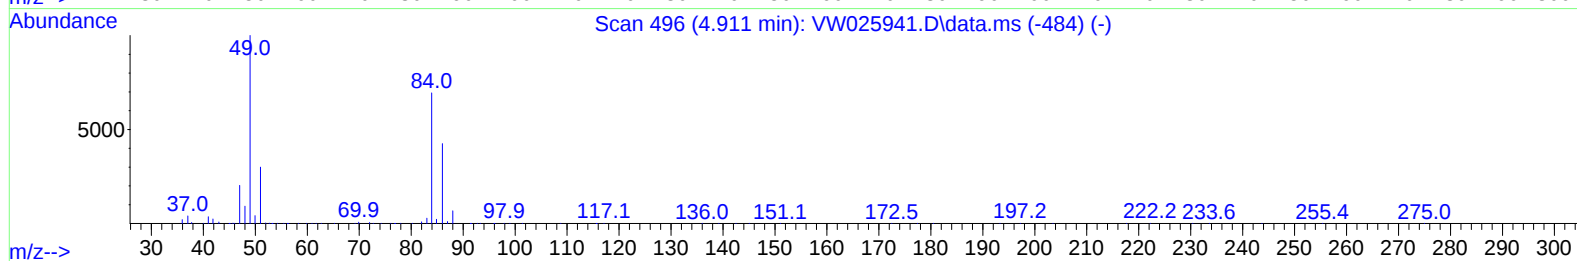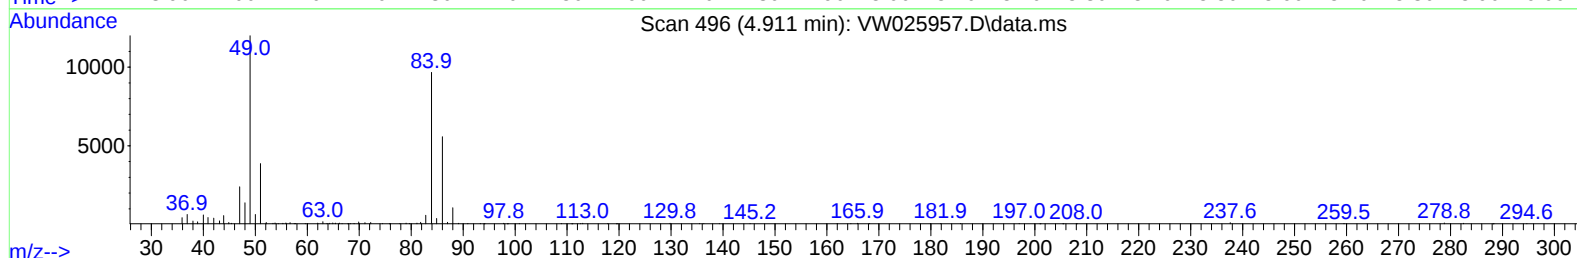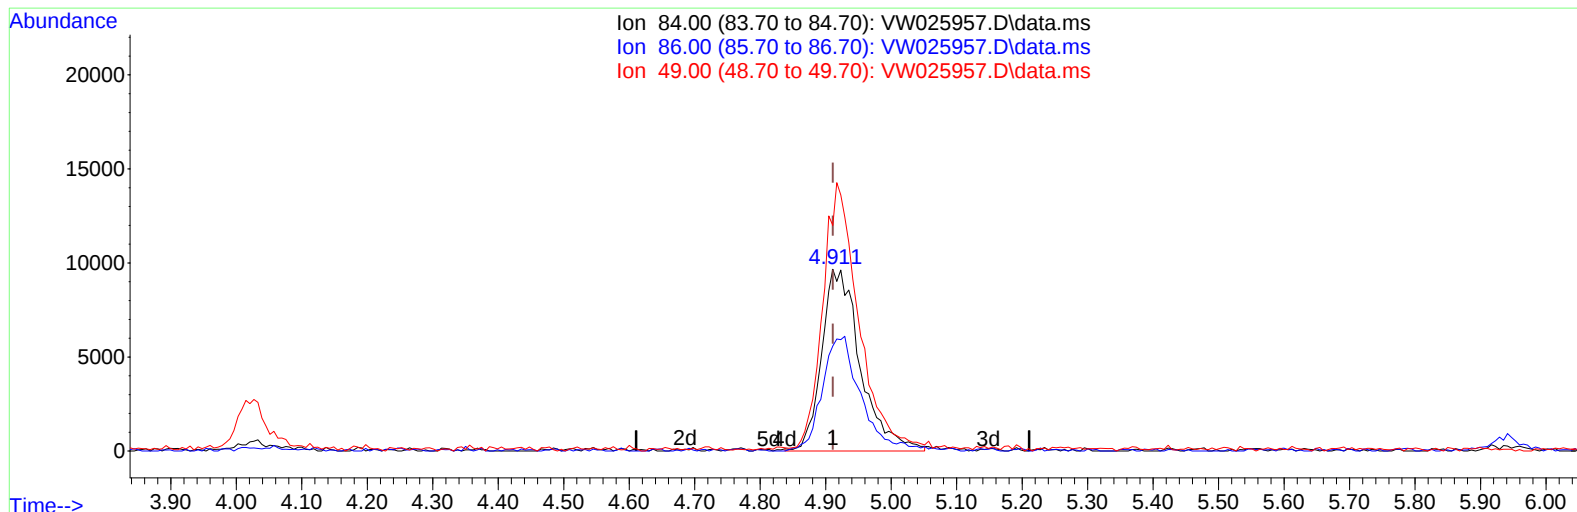

TIC: VW025957.D\data.ms

(16) Methylene chloride (T)

4.911min (-0.000) 3.08 ug/L m

response 39699

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	59.60	57.78
49.00	136.20	124.10
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051123\
 Data File : VW025957.D
 Acq On : 11 May 2023 15:47
 Operator : SY/MD
 Sample : 02689-03
 Misc : 5.05g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/12/2023
 Supervised By :Mahesh Dadoda 05/12/2023

Quant Time: May 12 05:39:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 05 23:47:36 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	625576	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	571991	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	264442	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	194975	21.994	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	87.960%		
7) Chloroethane-d5	2.893	69	137813	20.969	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.880%		
11) 1,1-Dichloroethene-d2	4.021	65	95127	21.430	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	85.720%		
21) 2-Butanone-d5	7.081	46	142211	48.526	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.060%		
24) Chloroform-d	7.648	84	425300	23.577	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.320%		
26) 1,2-Dichloroethane-d4	8.300	65	245253	24.044	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	96.160%		
32) Benzene-d6	8.276	84	861611	23.053	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.200%		
36) 1,2-Dichloropropane-d6	9.270	67	281057	23.503	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.000%		
41) Toluene-d8	10.325	98	734204	22.030	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	88.120%		
43) trans-1,3-Dichloroprop...	10.574	79	105056	21.673	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	86.680%		
47) 2-Hexanone-d5	10.922	63	99363	48.728	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.460%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	222214	24.380	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	97.520%		
66) 1,2-Dichlorobenzene-d4	13.848	152	232245	24.092	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.360%		
Target Compounds						Qvalue
16) Methylene chloride	4.911	84	39699m	3.077	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051123\
Data File : VW025957.D
Acq On : 11 May 2023 15:47
Operator : SY/MD
Sample : 02689-03
Misc : 5.05g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/12/2023
Supervised By :Mahesh Dadoda 05/12/2023

Quant Time: May 12 05:39:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 05 23:47:36 2023
Response via : Initial Calibration

