


Data Path : W:\HPCHEM1\MSVOA W\DATA\VW051518\
Data File : VW002523.D
Acq On : 14 May 2018 20:01
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W051518S.M
Title : SW846 8260
Last Update : Tue May 15 03:32:11 2018

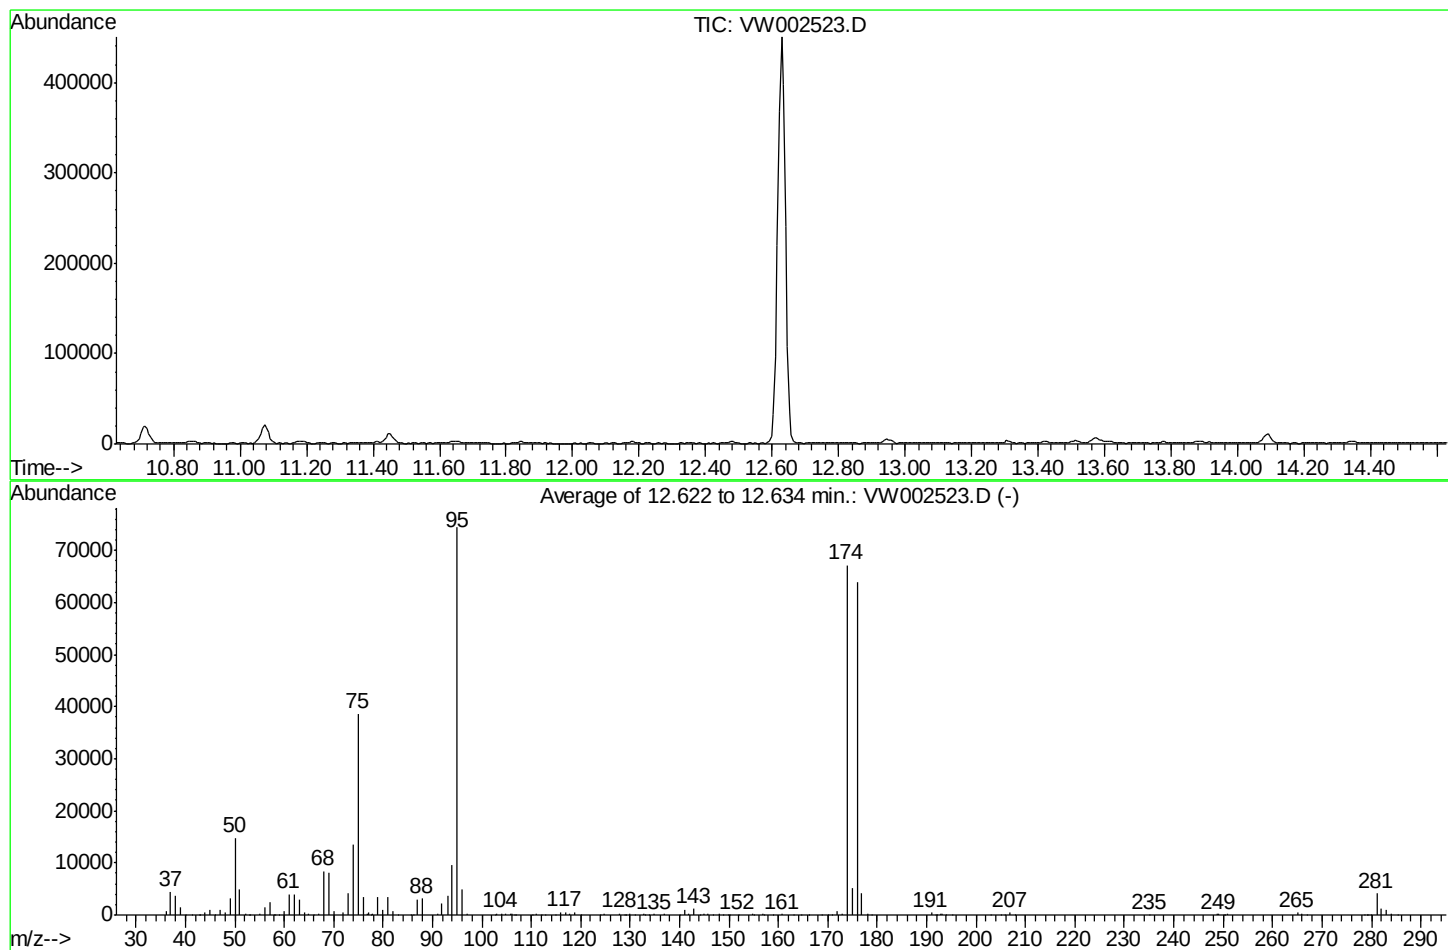

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	14785	PASS
75	95	30	60	51.9	38616	PASS
95	95	100	100	100.0	74416	PASS
96	95	5	9	6.8	5029	PASS
173	174	0.00	2	0.4	289	PASS
174	95	50	100	90.2	67120	PASS
175	174	5	9	7.9	5274	PASS
176	174	95	101	95.2	63877	PASS
177	176	5	9	6.7	4273	PASS