


Data Path : W:\HPCHEM1\MSVOA W\DATA\VW051518\  
 Data File : VW002546.D  
 Acq On : 15 May 2018 09:23  
 Operator : JC/SY  
 Sample : BFB  
 Misc : 5.00G/5ML/MSVOA W/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_W  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA\_W\METHOD\82W051518S.M  
 Title : SW846 8260  
 Last Update : Tue May 15 03:32:11 2018

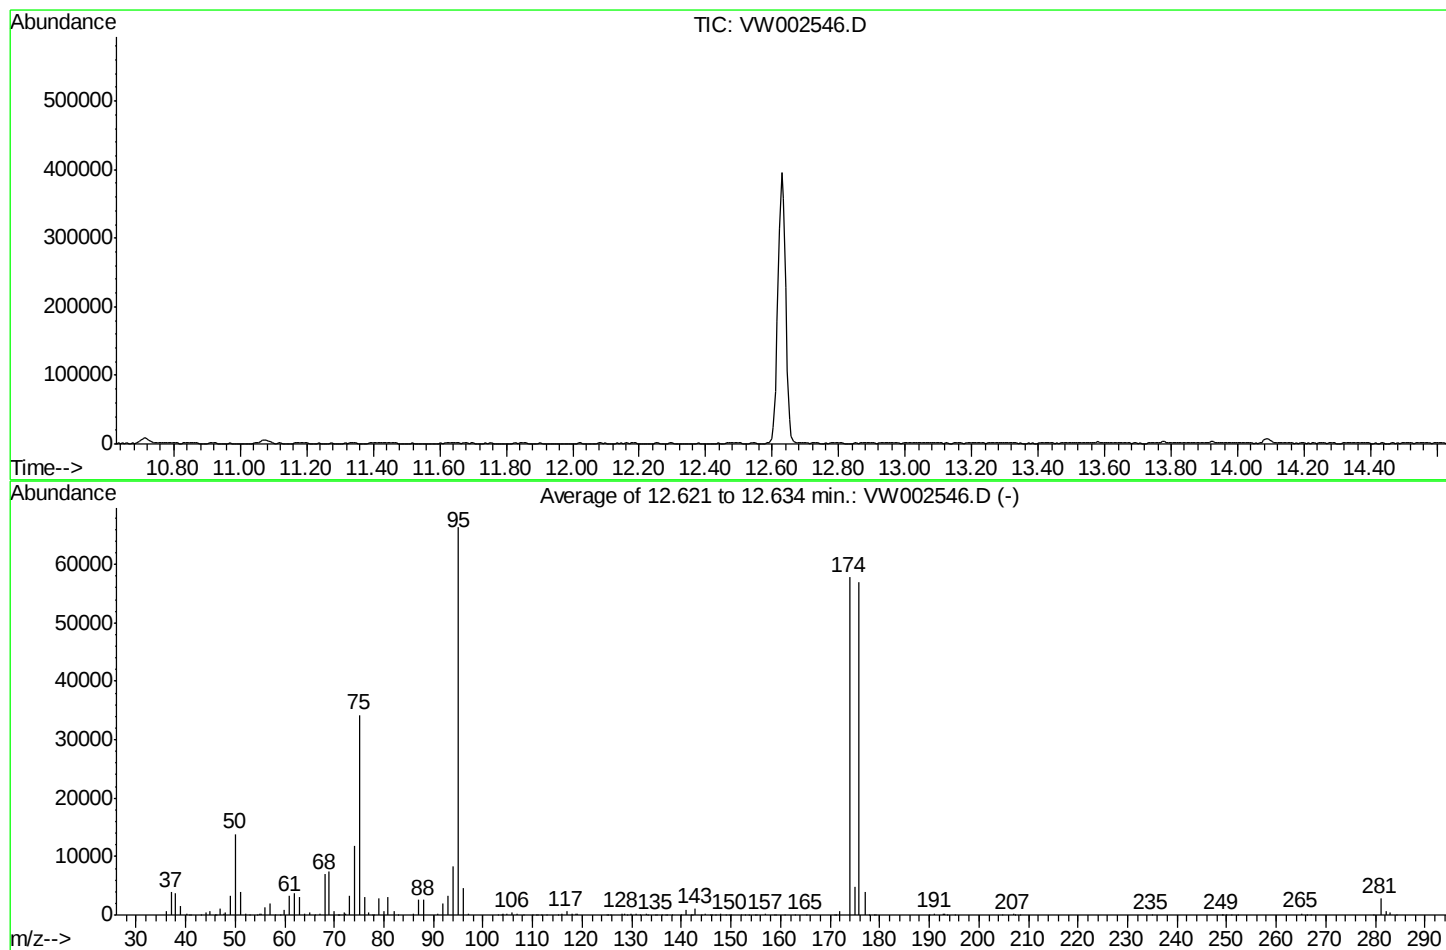

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1802

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 20.9      | 13850   | PASS             |
| 75          | 95           | 30           | 60           | 51.6      | 34245   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 66349   | PASS             |
| 96          | 95           | 5            | 9            | 6.8       | 4523    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 87.2      | 57832   | PASS             |
| 175         | 174          | 5            | 9            | 8.2       | 4741    | PASS             |
| 176         | 174          | 95           | 101          | 98.4      | 56893   | PASS             |
| 177         | 176          | 5            | 9            | 6.8       | 3852    | PASS             |