


Data Path : W:\HPCHEM1\MSVOA W\DATA\VW051518\
Data File : VW002565.D
Acq On : 15 May 2018 22:26
Operator : JC/SY
Sample : BFB
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W051518S.M
Title : SW846 8260
Last Update : Tue May 15 03:32:11 2018

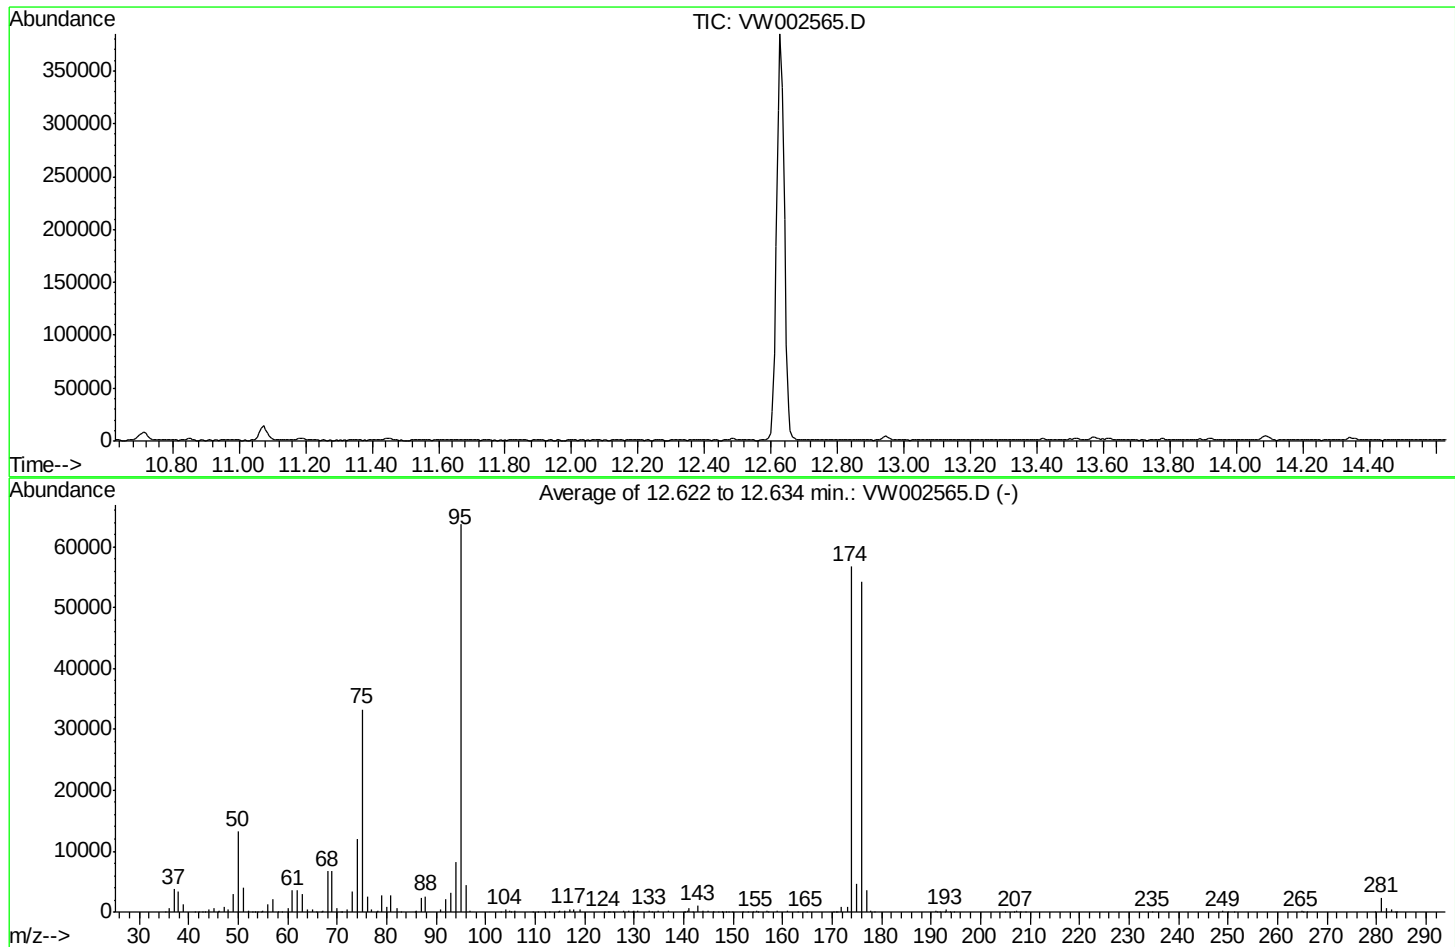

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	13183	PASS
75	95	30	60	52.2	33272	PASS
95	95	100	100	100.0	63728	PASS
96	95	5	9	7.0	4476	PASS
173	174	0.00	2	1.4	772	PASS
174	95	50	100	89.0	56733	PASS
175	174	5	9	8.1	4582	PASS
176	174	95	101	95.8	54362	PASS
177	176	5	9	6.8	3679	PASS