



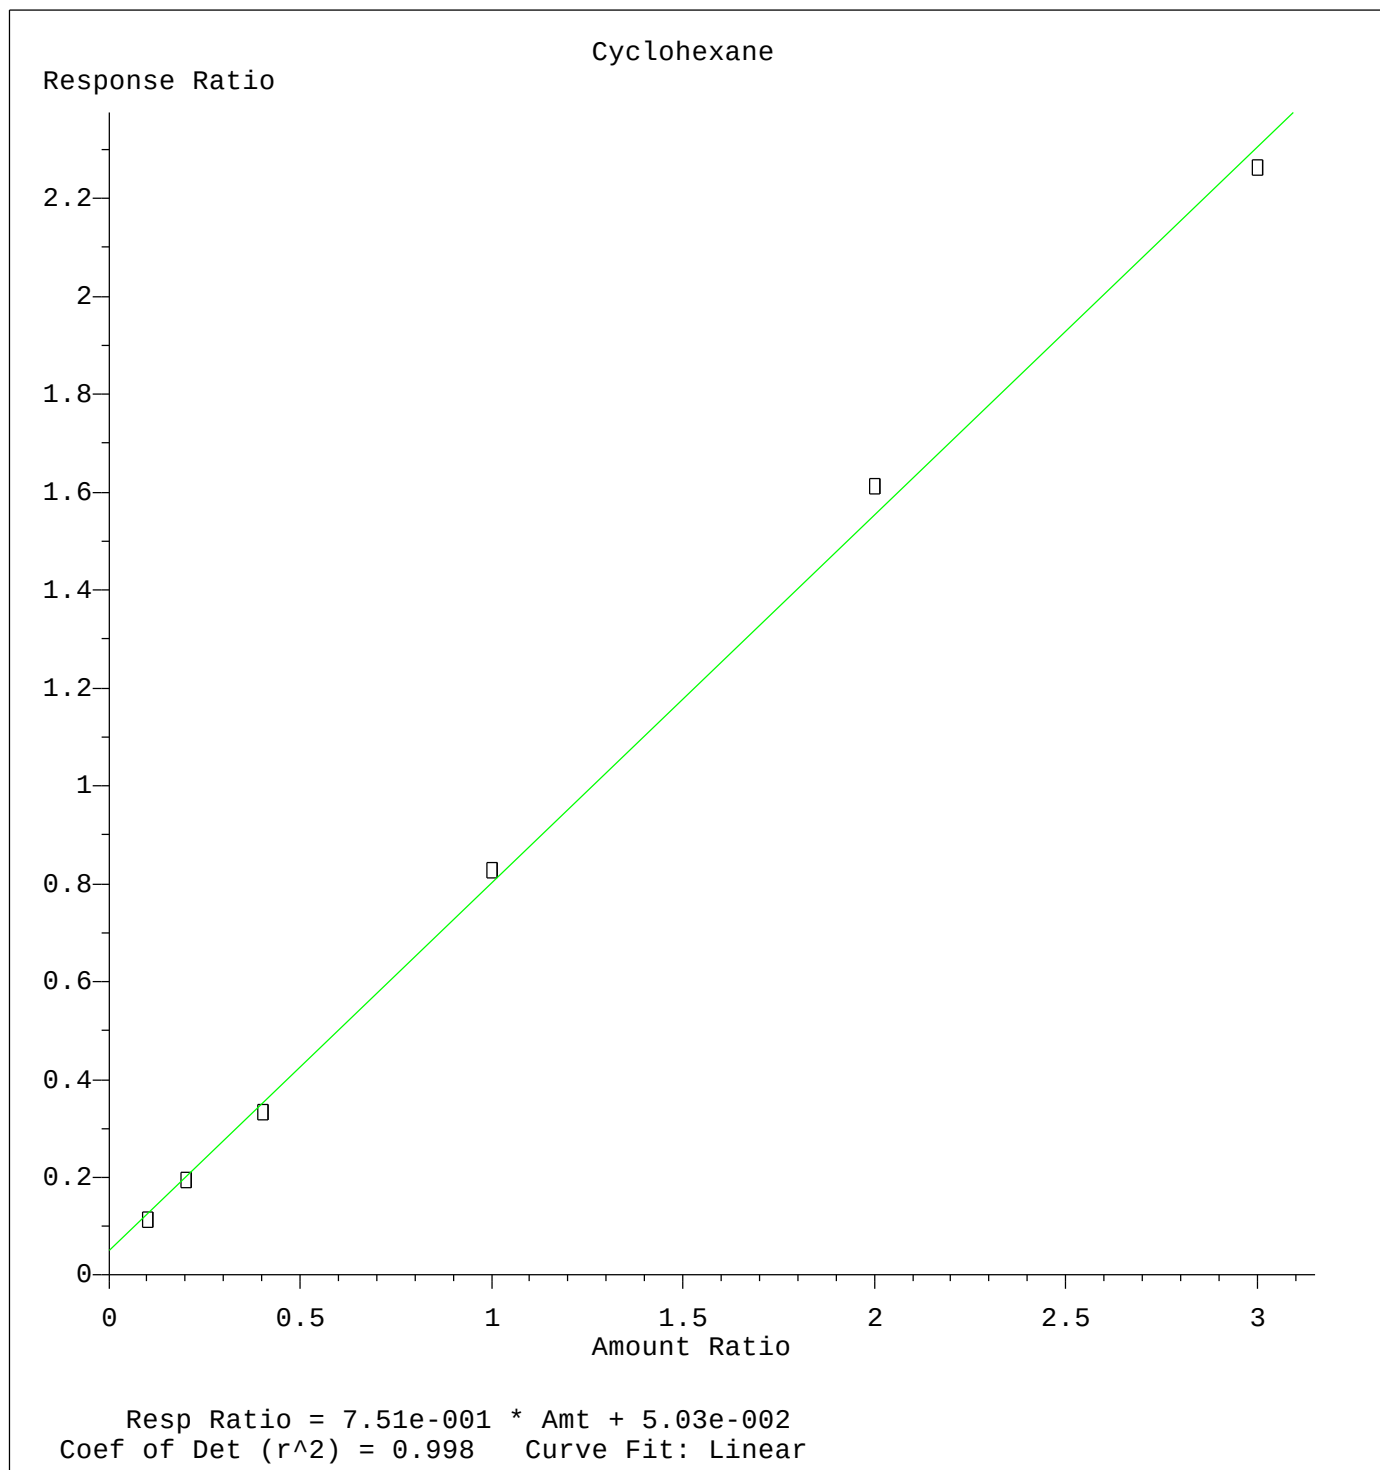

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051619S.M
Calibration Table Last Updated: Fri May 17 09:10:13 2019

Dichlorodifluoromethane

Response Ratio

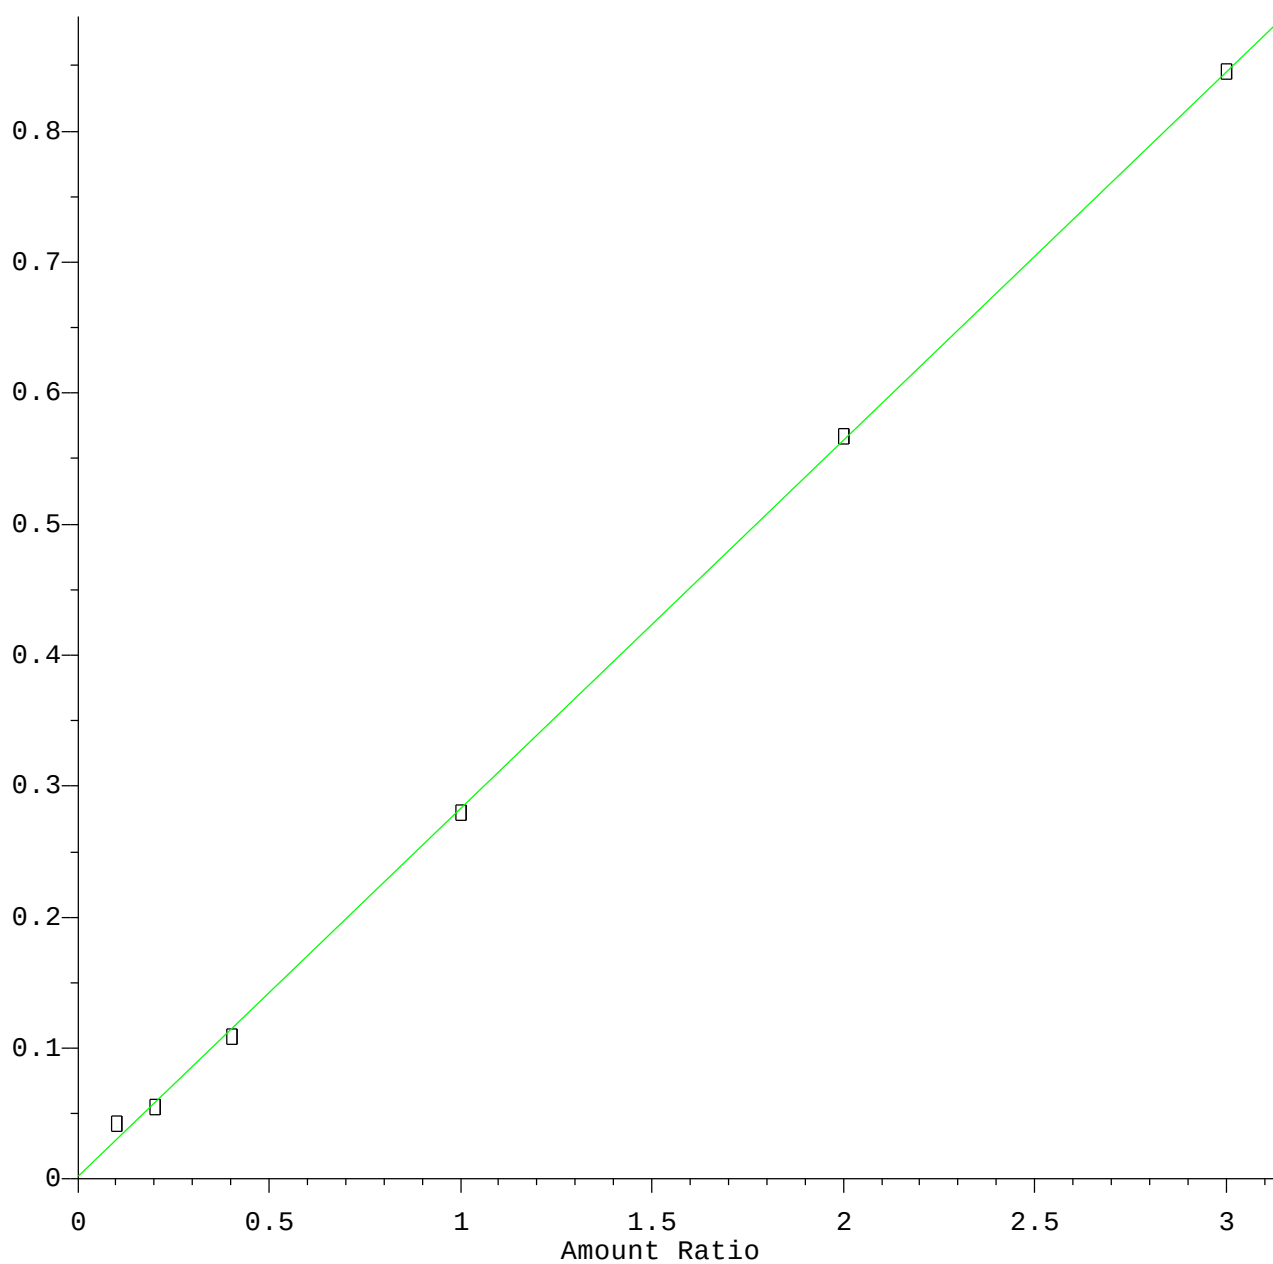

Resp Ratio = $2.81 \times 10^{-1} \times \text{Amt} + 2.46 \times 10^{-3}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051619S.M
Calibration Table Last Updated: Fri May 17 09:10:13 2019