


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW051619\
Data File : VW010408.D
Acq On : 16 May 2019 17:50
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051619S.M
Title : SW846 8260
Last Update : Fri May 17 09:10:13 2019

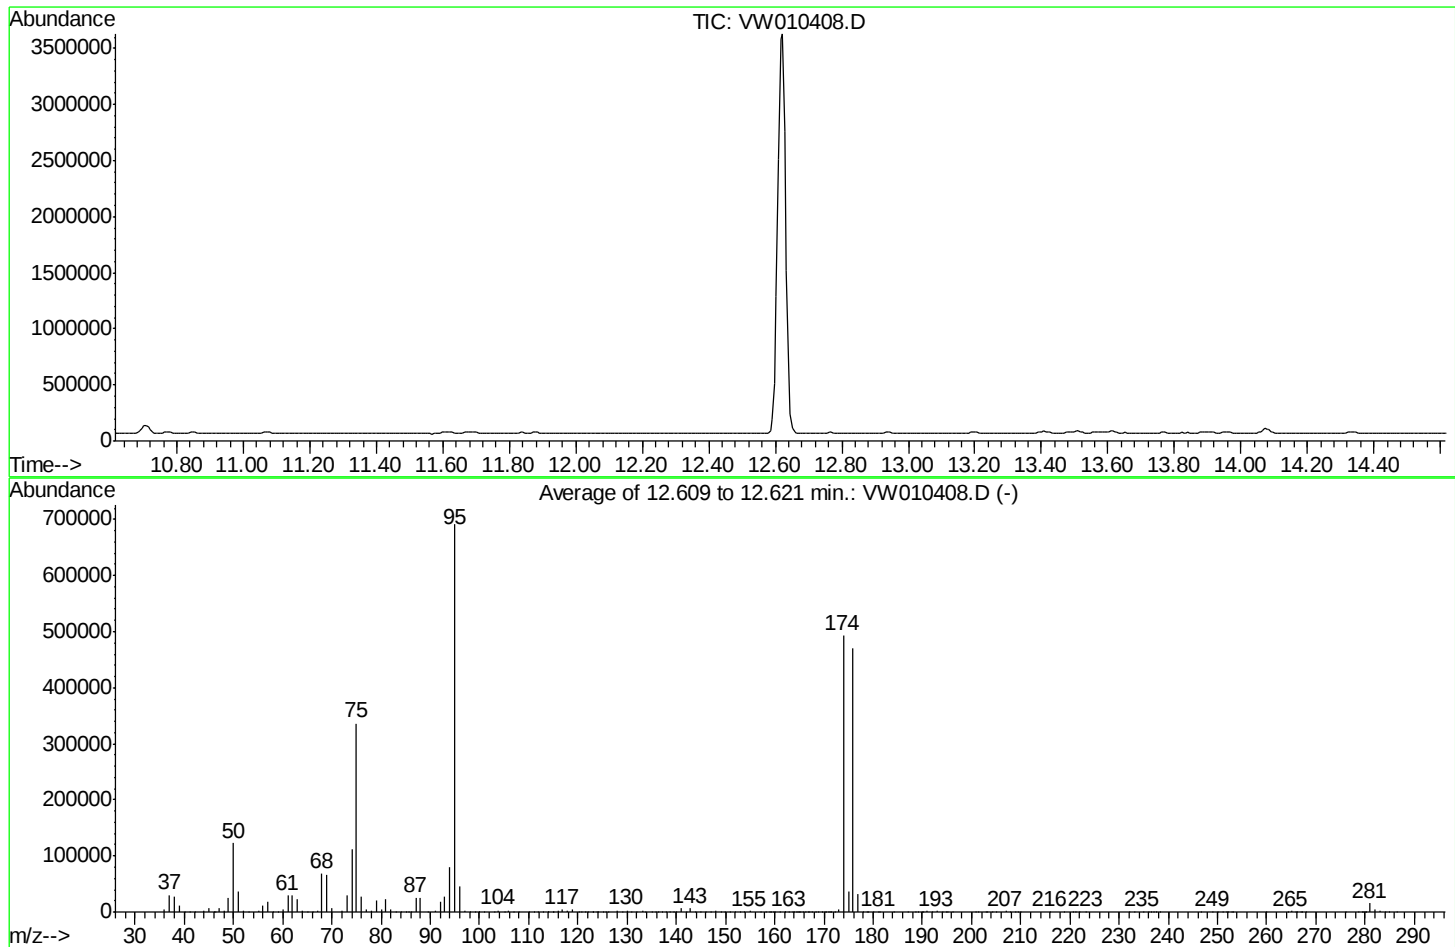

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	122888	PASS
75	95	30	60	48.6	336112	PASS
95	95	100	100	100.0	691319	PASS
96	95	5	9	6.8	46827	PASS
173	174	0.00	2	1.0	5030	PASS
174	95	50	100	71.3	492906	PASS
175	174	5	9	7.3	36216	PASS
176	174	95	101	95.4	470165	PASS
177	176	5	9	6.7	31696	PASS