

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
 Data File : VW023043.D
 Acq On : 16 May 2022 10:42
 Operator : SY/VA
 Sample : N2815-07
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 X3A86

Quant Time: May 17 01:25:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 17 01:24:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	339891	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	323087	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	183780	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	171599	24.608	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.440%
7) Chloroethane-d5	2.886	69	121359	26.750	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.000%
11) 1,1-Dichloroethene-d2	4.019	63	205748	22.835	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	91.320%
21) 2-Butanone-d5	7.080	46	61698	46.534	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.060%
24) Chloroform-d	7.647	84	258459	25.955	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.800%
26) 1,2-Dichloroethane-d4	8.098	65	51	0.009	ug/L	-0.21
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.040%#
32) Benzene-d6	8.269	84	505950	27.169	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.680%
36) 1,2-Dichloropropane-d6	9.275	67	143013	27.339	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	109.360%
41) Toluene-d8	10.323	98	490092	27.243	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	108.960%
43) trans-1,3-Dichloroprop...	10.579	79	64181	26.646	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	106.600%
47) 2-Hexanone-d5	10.921	63	48587	48.655	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.300%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	125051	25.647	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.600%
66) 1,2-Dichlorobenzene-d4	13.853	152	177417	27.616	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.480%
Target Compounds						Qvalue
2) Dichlorodifluoromethane	2.008	85	23677	12.779	ug/L	92
3) Chloromethane	2.215	50	56635	15.818	ug/L	97
5) Vinyl chloride	2.361	62	188849	26.282	ug/L	99
6) Bromomethane	2.776	94	61592	13.350	ug/L	91
8) Chloroethane	2.922	64	34137	9.850	ug/L	96
9) Trichlorofluoromethane	3.257	101	35043	10.670	ug/L	96
10) 1,1,2-Trichloro-1,2,2-...	4.062	101	112162	22.840	ug/L	98
12) 1,1-Dichloroethene	4.038	96	75231	17.282	ug/L #	80
15) Methyl Acetate	4.666	43	47151	23.644	ug/L	100
16) Methylene chloride	4.916	84	105920	21.297	ug/L	98
18) Methyl tert-butyl Ether	5.428	73	309605	41.400	ug/L	99
22) 2-Butanone	7.171	43	71707	51.654	ug/L	99
25) Chloroform	7.677	83	192451	20.962	ug/L	99
29) Cyclohexane	7.952	56	160646	22.991	ug/L	99
33) Benzene	8.324	78	856857	45.019	ug/L	100
34) Trichloroethene	9.092	95	295791	56.509	ug/L	99
42) Toluene	10.384	91	1210558	56.753	ug/L	97
45) 1,1,2-Trichloroethane	10.787	97	79767	20.716	ug/L	97
46) Tetrachloroethene	10.860	164	45896	11.667	ug/L	93

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
 Data File : VW023043.D
 Acq On : 16 May 2022 10:42
 Operator : SY/VA
 Sample : N2815-07
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 X3A86

Quant Time: May 17 01:25:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 17 01:24:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


51) Chlorobenzene	11.652	112	192748	13.707	ug/L	97
52) Ethylbenzene	11.725	91	669112	28.196	ug/L	100
53) m,p-Xylene	11.841	106	317439	33.949	ug/L	98
54) o-Xylene	12.164	106	253072	28.204	ug/L	99
55) Styrene	12.177	104	161905	10.619	ug/L	94
57) 1,1,2,2-Tetrachloroethane	12.713	83	56719	11.794	ug/L	97
59) Bromoform	12.347	173	27417	10.527	ug/L	99
60) Isopropylbenzene	12.463	105	555876	22.079	ug/L	100
61) 1,2,3-Trichloropropane	12.743	75	22322	6.079	ug/L #	1
63) 1,2,4-Trimethylbenzene	13.249	105	556146	26.443	ug/L	97
64) 1,3-Dichlorobenzene	13.493	146	240346	21.382	ug/L	91
65) 1,4-Dichlorobenzene	13.579	146	121576	10.471	ug/L	97
69) 1,3,5-Trichlorobenzene	15.127	180	122774	16.454	ug/L	98
70) 1,2,4-trichlorobenzene	15.127	180	122774	20.455	ug/L	98
72) 1,2,3-Trichlorobenzene	15.554	180	165350	31.083	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
Data File : VW023043.D
Acq On : 16 May 2022 10:42
Operator : SY/VA
Sample : N2815-07
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
X3A86

Quant Time: May 17 01:25:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 17 01:24:30 2022
Response via : Initial Calibration




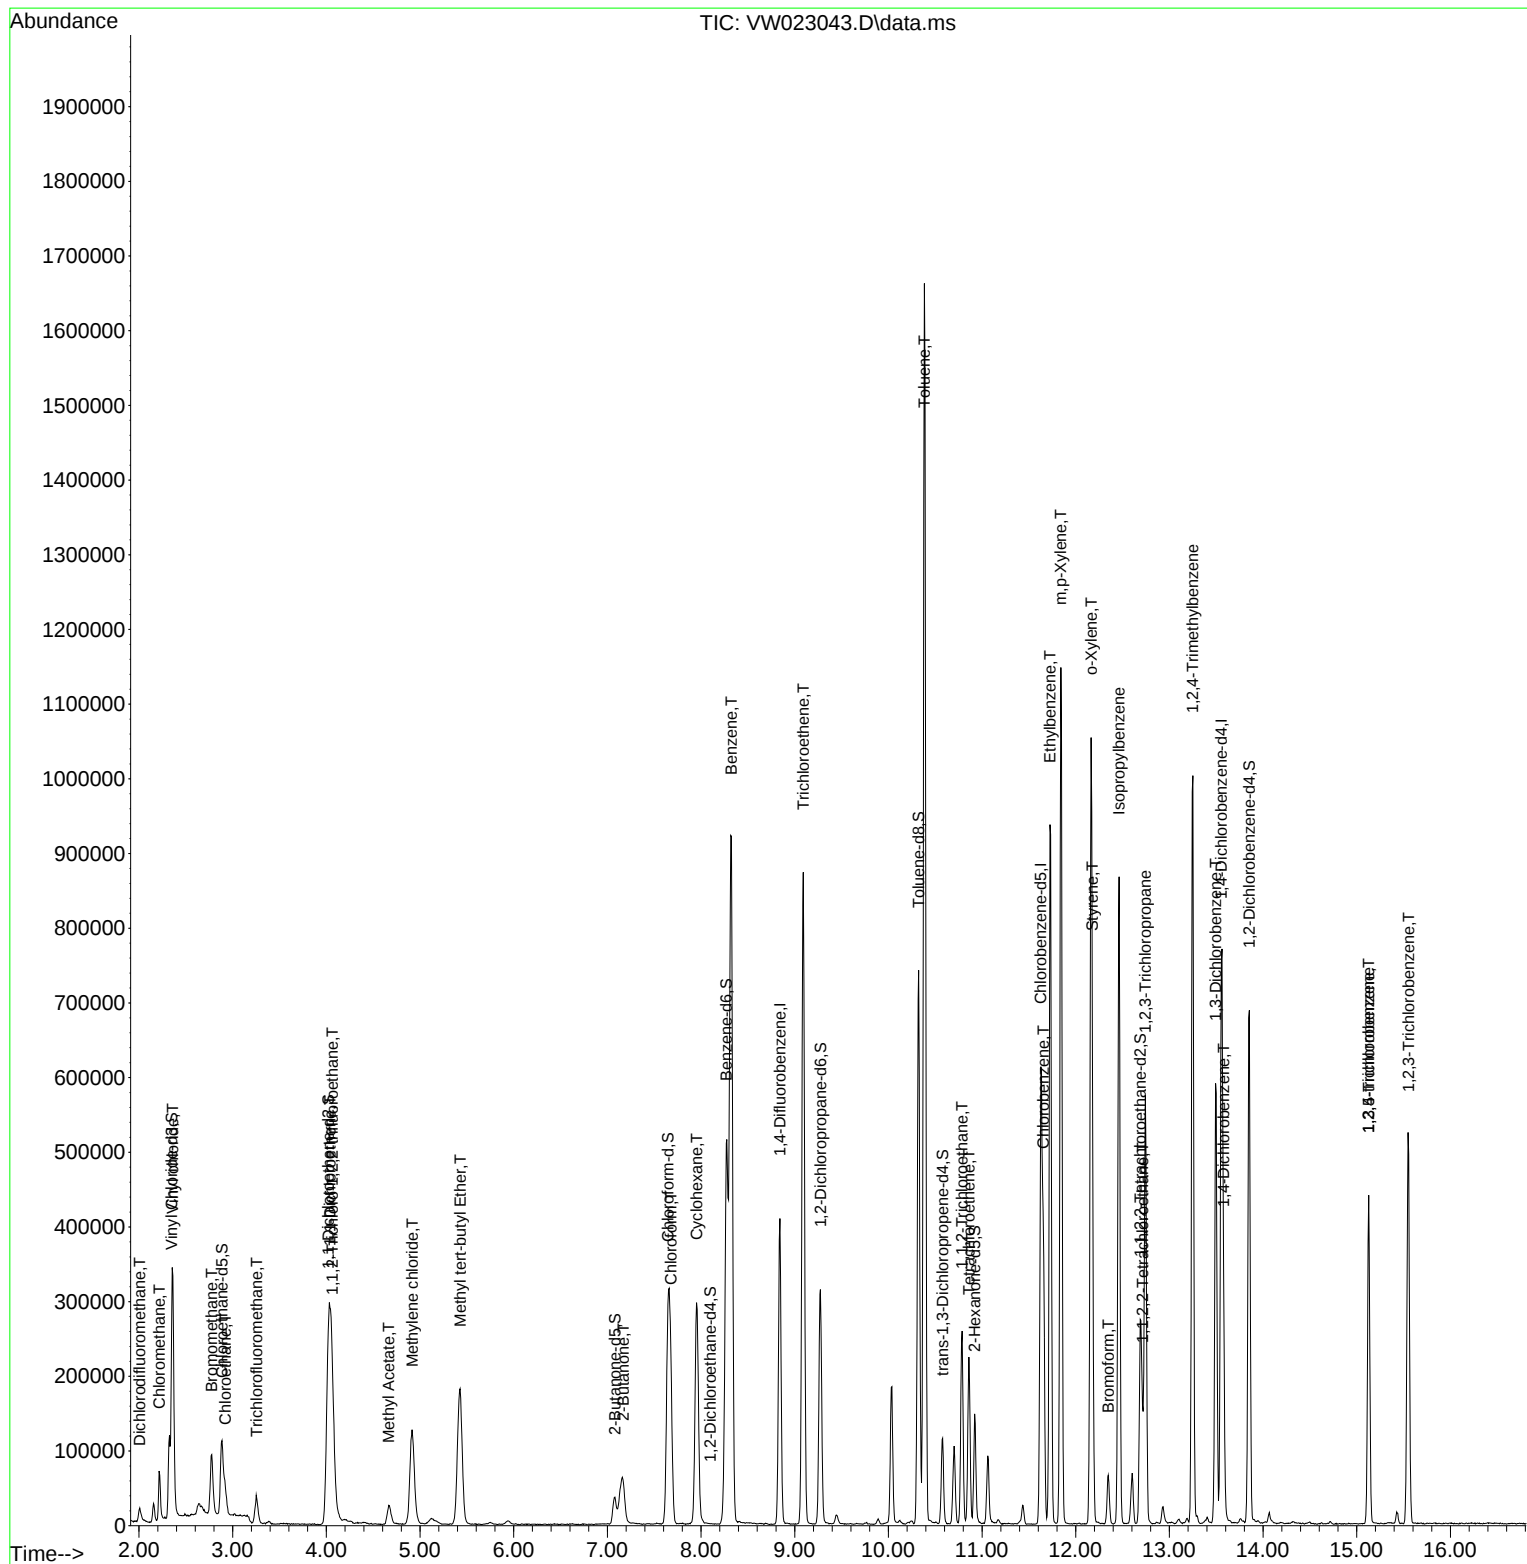




#2
 Dichlorodifluoromethane
 Concen: 12.779 ug/L
 RT: 2.008 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: VW023043.D
 Acq: 16 May 2022 10:42




Instrument :
 MSVOA_W
 ClientSampleId :
 X3A86


Tgt Ion: 85 Resp: 23677
 Ion Ratio Lower Upper
 85 100
 87 30.2 27.8 41.8

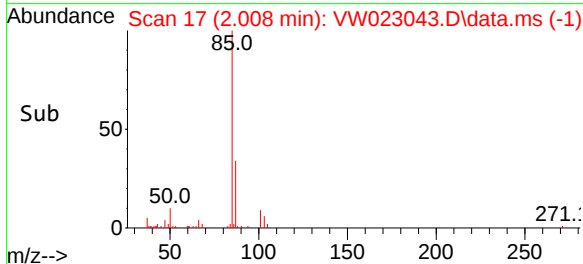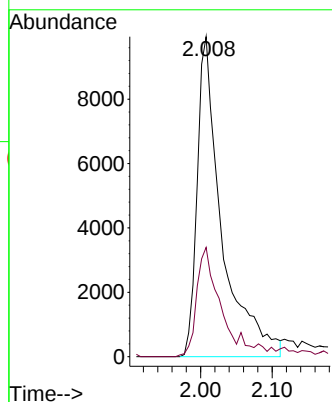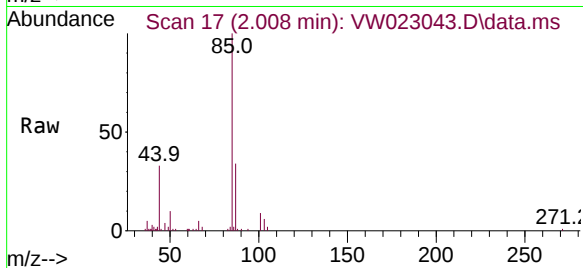

#3
 Chloromethane
 Concen: 15.818 ug/L
 RT: 2.215 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: VW023043.D
 Acq: 16 May 2022 10:42

Tgt Ion: 50 Resp: 56635
 Ion Ratio Lower Upper
 50 100
 52 34.5 23.1 42.9


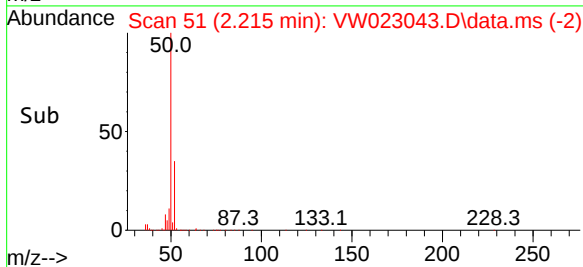
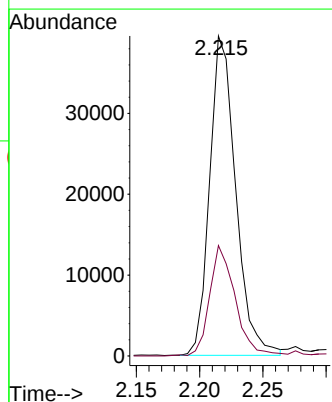
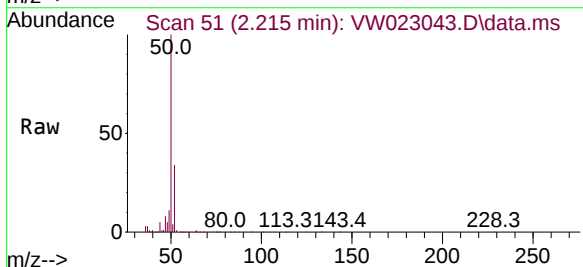




#5
 Vinyl chloride
 Concen: 26.282 ug/L
 RT: 2.361 min Scan# 75
 Delta R.T. 0.000 min
 Lab File: VW023043.D
 Acq: 16 May 2022 10:42




Instrument :
 MSVOA_W
 ClientSampleId :
 X3A86


Tgt Ion: 62 Resp: 188849
 Ion Ratio Lower Upper
 62 100
 64 36.4 24.9 46.3

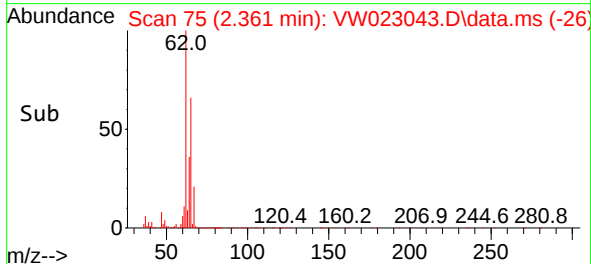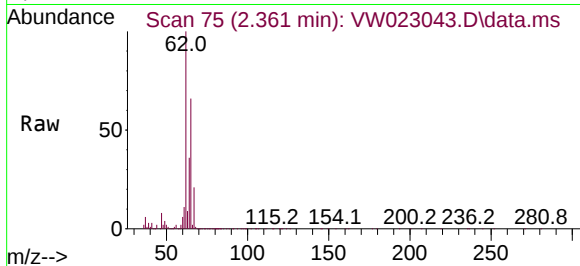

#6
 Bromomethane
 Concen: 13.350 ug/L
 RT: 2.776 min Scan# 143
 Delta R.T. 0.000 min
 Lab File: VW023043.D
 Acq: 16 May 2022 10:42

Tgt Ion: 94 Resp: 61592
 Ion Ratio Lower Upper
 94 100
 96 96.0 61.7 114.5


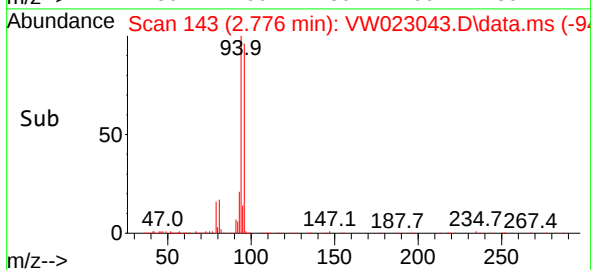

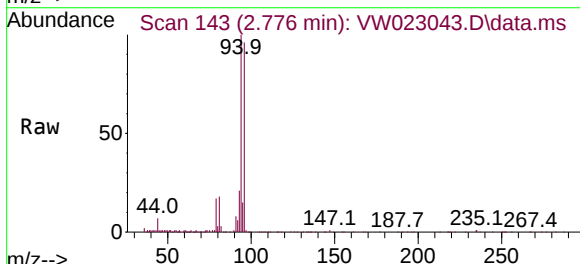




#8
Chloroethane
Concen: 9.850 ug/L
RT: 2.922 min Scan# 167
Delta R.T. 0.006 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion: 64 Resp: 34137
Ion Ratio Lower Upper
64 100
66 31.0 23.4 43.6

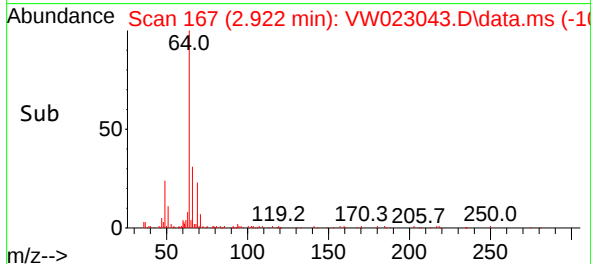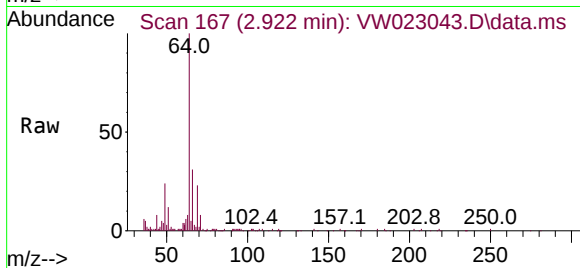

#9
Trichlorofluoromethane
Concen: 10.670 ug/L
RT: 3.257 min Scan# 222
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion: 101 Resp: 35043
Ion Ratio Lower Upper
101 100
103 64.0 53.9 80.9




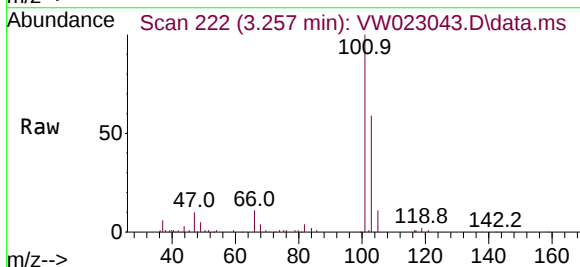


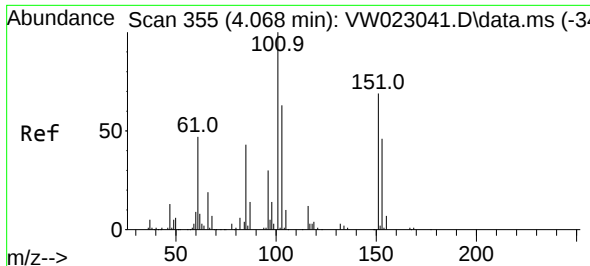

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 22.840 ug/L
 RT: 4.062 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VW023043.D
 Acq: 16 May 2022 10:42




Instrument :
 MSVOA_W
 ClientSampleId :
 X3A86


Tgt Ion:101 Resp: 112162
 Ion Ratio Lower Upper
 101 100
 85 43.4 34.3 51.5
 151 69.3 54.2 81.2

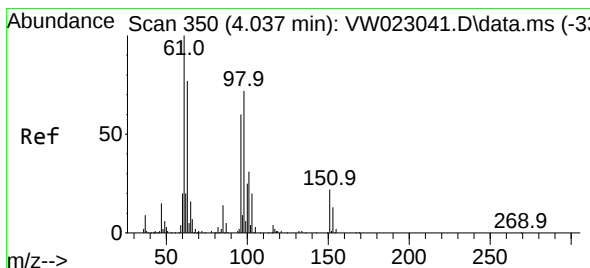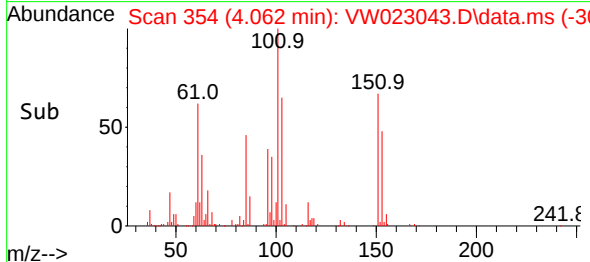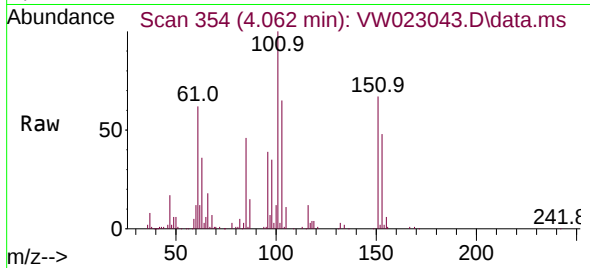

#12
 1,1-Dichloroethene
 Concen: 17.282 ug/L
 RT: 4.038 min Scan# 350
 Delta R.T. 0.000 min
 Lab File: VW023043.D
 Acq: 16 May 2022 10:42

Tgt Ion: 96 Resp: 75231
 Ion Ratio Lower Upper
 96 100
 61 170.8 125.7 233.5
 63 165.1 83.4 155.0#


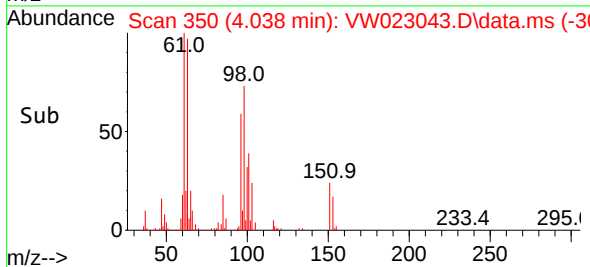

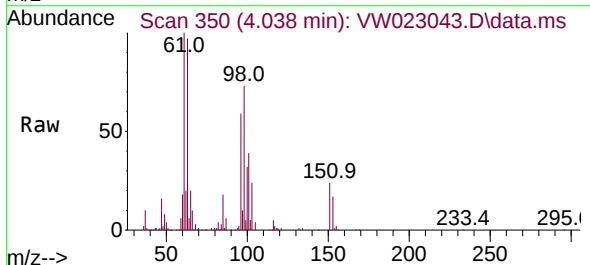


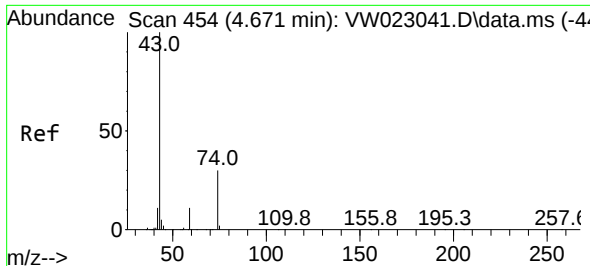

#15
Methyl Acetate
Concen: 23.644 ug/L
RT: 4.666 min Scan# 41
Delta R.T. -0.006 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion: 43 Resp: 47151
Ion Ratio Lower Upper
43 100
74 27.6 21.9 32.9

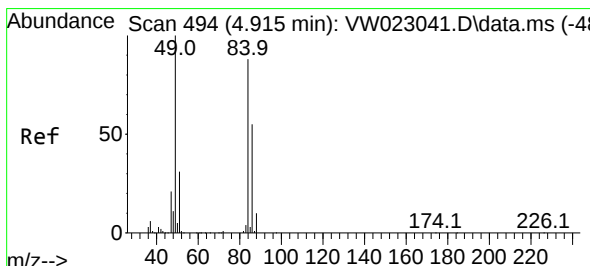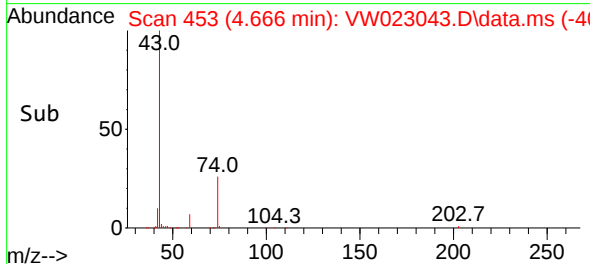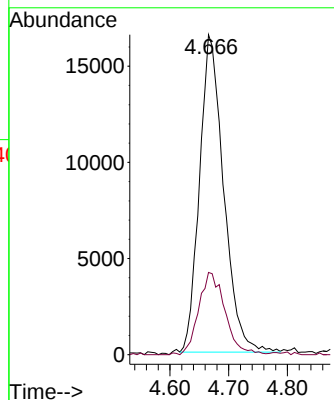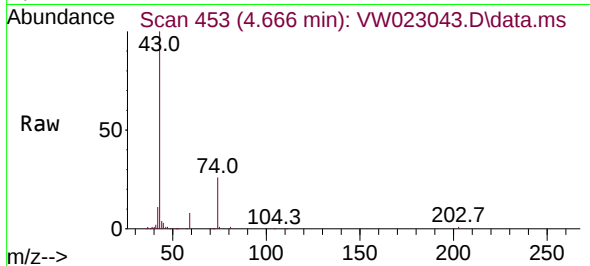

#16
Methylene chloride
Concen: 21.297 ug/L
RT: 4.916 min Scan# 494
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion: 84 Resp: 105920
Ion Ratio Lower Upper
84 100
86 66.4 45.4 84.4
49 119.3 82.5 153.1


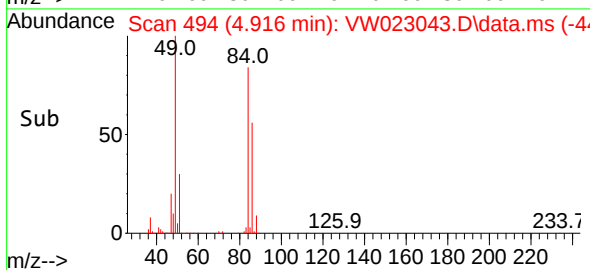
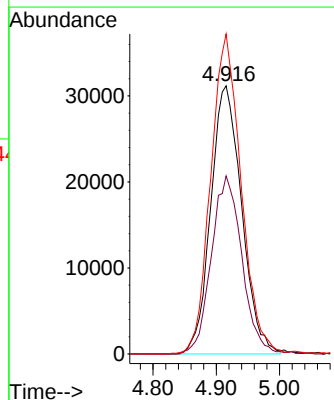
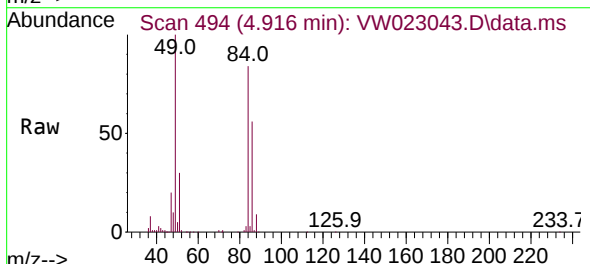




#18
Methyl tert-butyl Ether
Concen: 41.400 ug/L
RT: 5.428 min Scan# 51
Delta R.T. 0.006 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion: 73 Resp: 309605
Ion Ratio Lower Upper
73 100
43 19.5 15.9 23.9
57 20.7 16.5 24.7

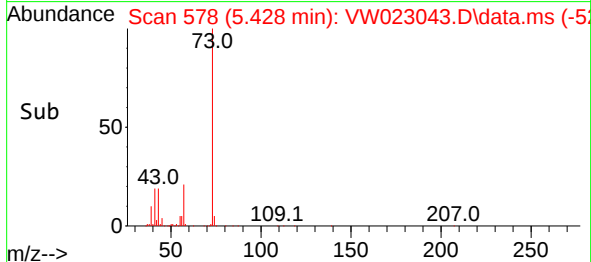

#22
2-Butanone
Concen: 51.654 ug/L
RT: 7.171 min Scan# 864
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion: 43 Resp: 71707
Ion Ratio Lower Upper
43 100
72 29.7 15.1 45.3


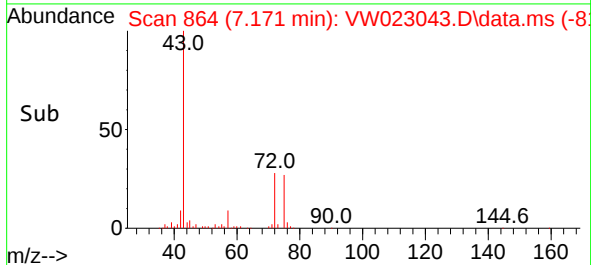






#25
Chloroform
Concen: 20.962 ug/L
RT: 7.677 min Scan# 946
Delta R.T. 0.006 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion: 83 Resp: 192451
Ion Ratio Lower Upper
83 100
85 66.0 46.6 86.6

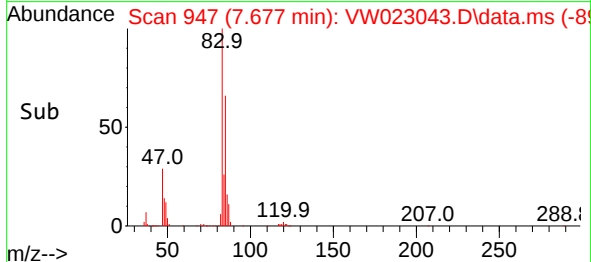

#29
Cyclohexane
Concen: 22.991 ug/L
RT: 7.952 min Scan# 992
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion: 56 Resp: 160646
Ion Ratio Lower Upper
56 100
69 32.3 25.6 38.4
84 98.3 78.2 117.4

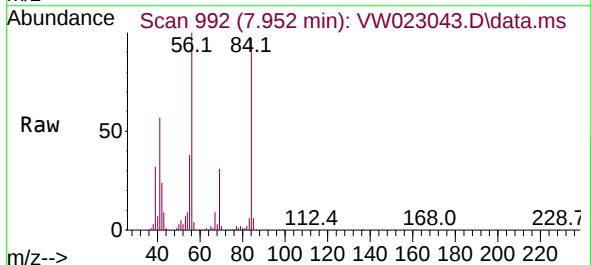

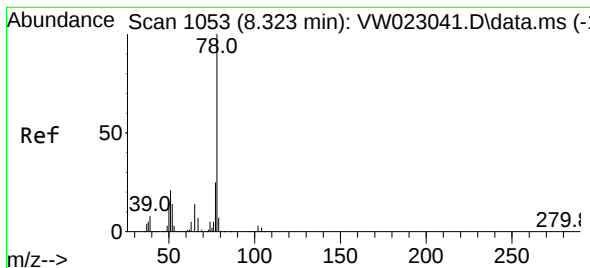

#33

Benzene

Concen: 45.019 ug/L

RT: 8.324 min Scan# 1053

Delta R.T. 0.000 min

Lab File: VW023043.D

Acq: 16 May 2022 10:42





Instrument :

MSVOA_W

ClientSampleId :

X3A86

Tgt Ion: 78 Resp: 856857

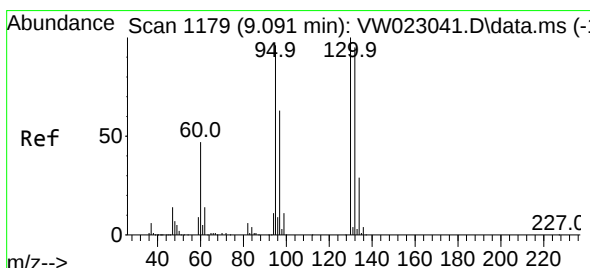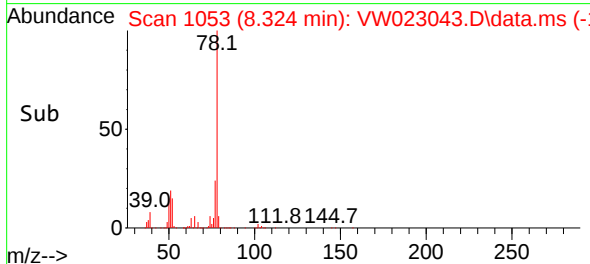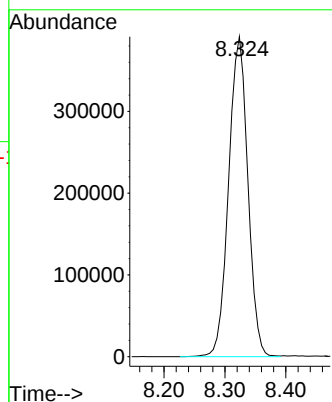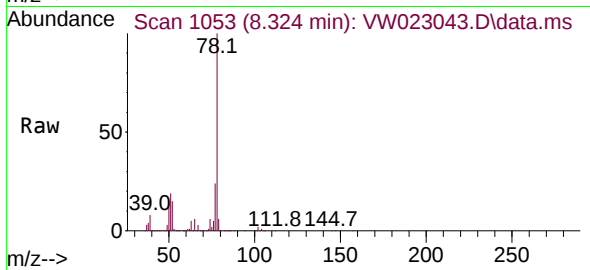

#34

Trichloroethene

Concen: 56.509 ug/L

RT: 9.092 min Scan# 1179

Delta R.T. 0.000 min

Lab File: VW023043.D

Acq: 16 May 2022 10:42

Tgt Ion: 95 Resp: 295791




Ion Ratio Lower Upper


95 100

97 65.6 46.1 85.7

132 97.1 66.9 124.3

130 98.4 69.5 129.1


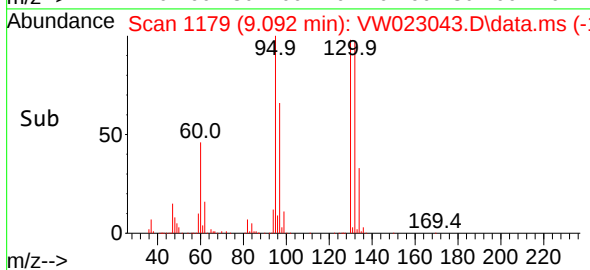

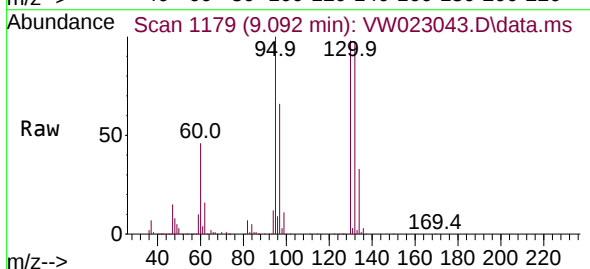




#42
Toluene
Concen: 56.753 ug/L
RT: 10.384 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion: 91 Resp: 1210558
Ion Ratio Lower Upper
91 100
92 57.3 41.6 77.2

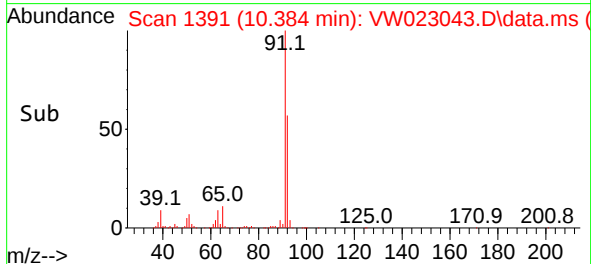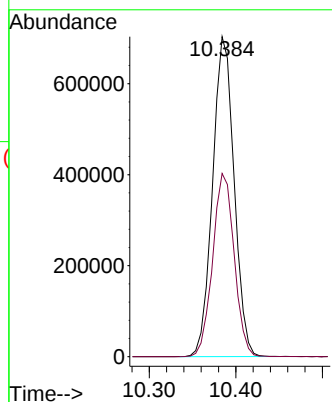

#45
1,1,2-Trichloroethane
Concen: 20.716 ug/L
RT: 10.787 min Scan# 1457
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion: 97 Resp: 79767
Ion Ratio Lower Upper
97 100
99 64.6 44.7 82.9
83 87.5 58.4 108.4
85 53.9 38.7 71.9









#46
Tetrachloroethene
Concen: 11.667 ug/L
RT: 10.860 min Scan# 1469
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion:	164	Resp:	45896
Ion Ratio	Lower	Upper	
164	100		
129	107.8	76.9	142.7
131	94.9	75.1	139.5
166	128.7	96.0	178.2

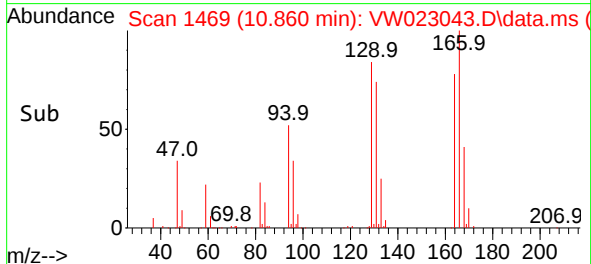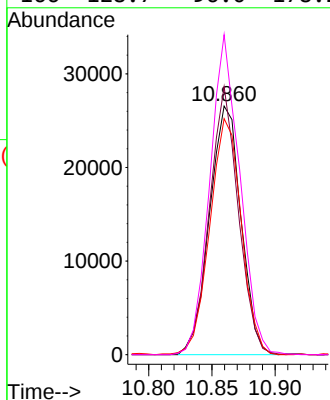

#51
Chlorobenzene
Concen: 13.707 ug/L
RT: 11.652 min Scan# 1599
Delta R.T. -0.006 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion:	112	Resp:	192748
Ion Ratio	Lower	Upper	
112	100		
114	28.6	22.0	41.0
77	54.4	42.6	63.8


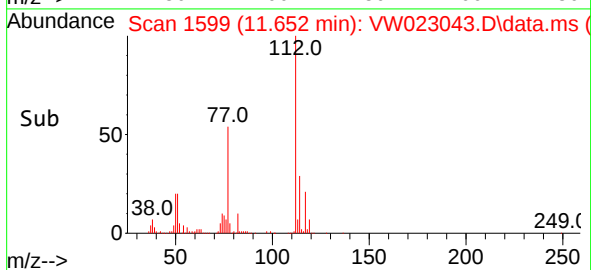
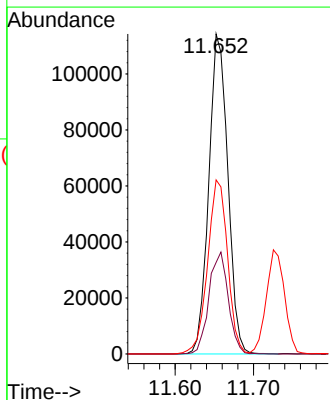
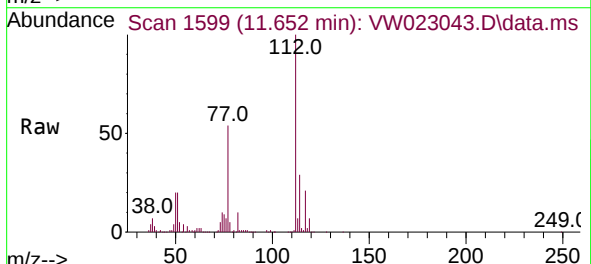




#52
Ethylbenzene
Concen: 28.196 ug/L
RT: 11.725 min Scan# 1611
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion: 91 Resp: 669112
Ion Ratio Lower Upper
91 100
106 31.9 22.3 41.3

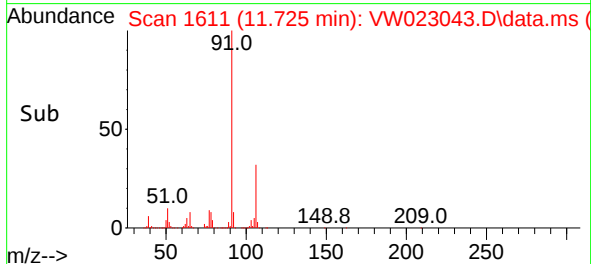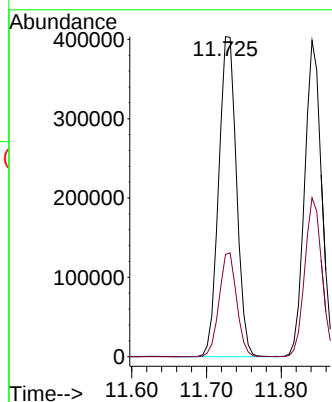

#53
m,p-Xylene
Concen: 33.949 ug/L
RT: 11.841 min Scan# 1630
Delta R.T. 0.006 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion:106 Resp: 317439
Ion Ratio Lower Upper
106 100
91 198.9 136.8 254.0


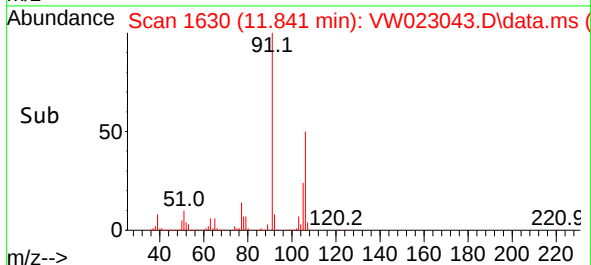






#54
o-Xylene
Concen: 28.204 ug/L
RT: 12.164 min Scan# 1
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion:106 Resp: 253072
Ion Ratio Lower Upper
106 100
91 208.0 147.2 273.4

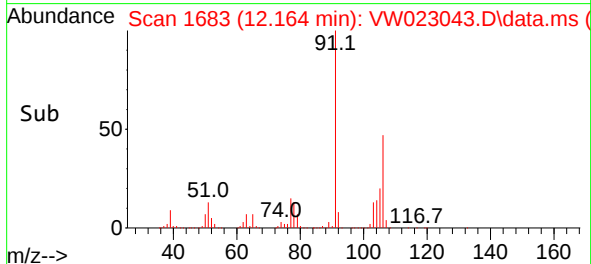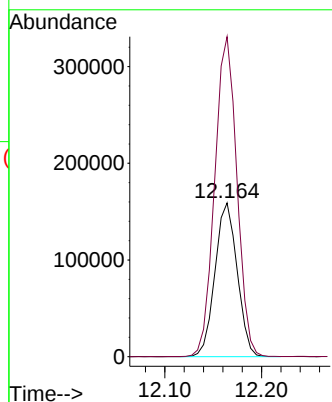

#55
Styrene
Concen: 10.619 ug/L
RT: 12.177 min Scan# 1685
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion:104 Resp: 161905
Ion Ratio Lower Upper
104 100
78 49.9 32.3 59.9

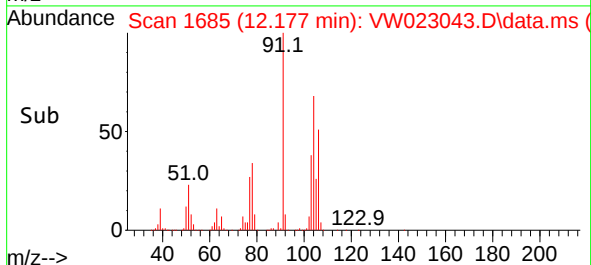



#57

1,1,2,2-Tetrachloroethane

Concen: 11.794 ug/L

RT: 12.713 min Scan# 1

Delta R.T. 0.000 min

Lab File: VW023043.D

Acq: 16 May 2022 10:42

Instrument :

MSVOA_W

ClientSampleId :

X3A86





Tgt Ion: 83 Resp: 56719

Ion Ratio Lower Upper

83 100

85 70.4 47.5 88.1

131 12.0 8.7 13.1

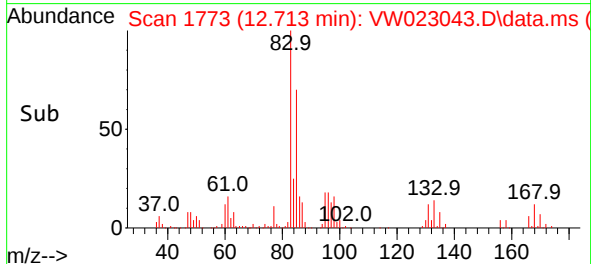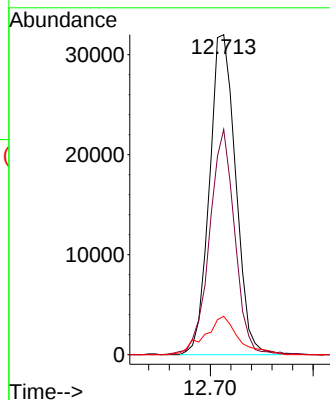

#59

Bromoform

Concen: 10.527 ug/L

RT: 12.347 min Scan# 1713

Delta R.T. 0.000 min

Lab File: VW023043.D

Acq: 16 May 2022 10:42




Tgt Ion: 173 Resp: 27417


Ion Ratio Lower Upper

173 100

175 47.9 38.1 57.1

254 8.8 6.5 9.7



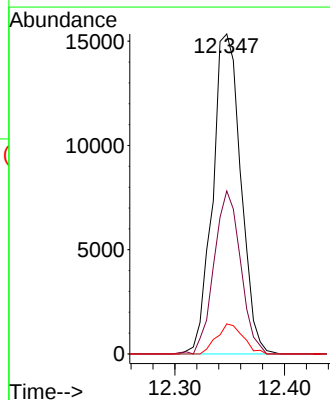





#60
Isopropylbenzene
Concen: 22.079 ug/L
RT: 12.463 min Scan# 11
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion:105 Resp: 555876
Ion Ratio Lower Upper
105 100
120 26.6 21.3 31.9
77 15.7 12.6 19.0

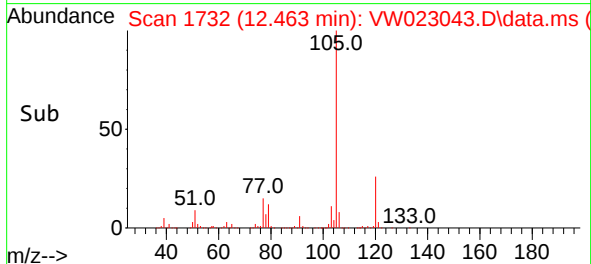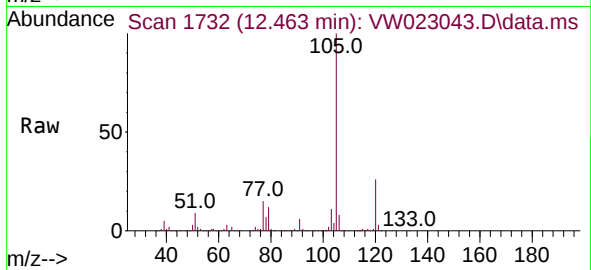

#61
1,2,3-Trichloropropane
Concen: 6.079 ug/L
RT: 12.743 min Scan# 1778
Delta R.T. -0.024 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion: 75 Resp: 22322
Ion Ratio Lower Upper
75 100
77 1064.4 26.2 39.2#
110 0.0 34.1 51.1#



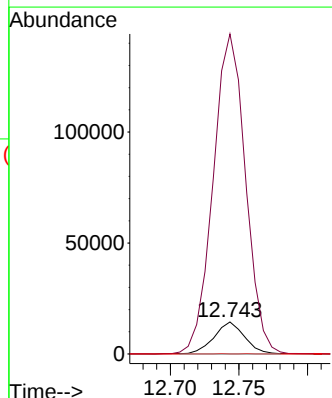





#63
1,2,4-Trimethylbenzene
Concen: 26.443 ug/L
RT: 13.249 min Scan# 1861
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42




Instrument :
MSVOA_W
ClientSampleId :
X3A86


Tgt Ion:105 Resp: 556146
Ion Ratio Lower Upper
105 100
120 44.8 37.4 56.2

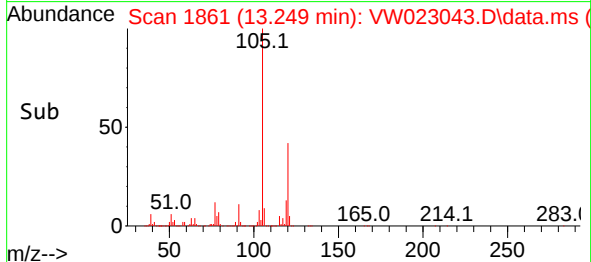

#64
1,3-Dichlorobenzene
Concen: 21.382 ug/L
RT: 13.493 min Scan# 1901
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion:146 Resp: 240346
Ion Ratio Lower Upper
146 100
111 40.2 29.5 54.9
148 59.0 48.6 90.2

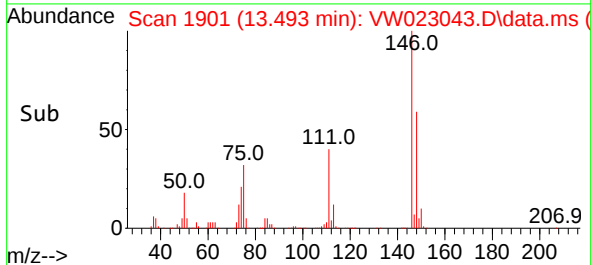



#65

1,4-Dichlorobenzene

Concen: 10.471 ug/L

RT: 13.579 min Scan# 1914

Delta R.T. 0.006 min

Lab File: VW023043.D

Acq: 16 May 2022 10:42

Instrument :

MSVOA_W

ClientSampleId :

X3A86





Tgt Ion:146 Resp: 121576

Ion Ratio Lower Upper

146 100

111 41.4 27.2 50.4

148 60.8 44.0 81.6

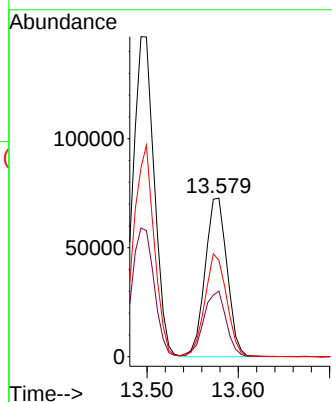

#69

1,3,5-Trichlorobenzene

Concen: 16.454 ug/L

RT: 15.127 min Scan# 2169

Delta R.T. 0.500 min

Lab File: VW023043.D

Acq: 16 May 2022 10:42

Tgt Ion:180 Resp: 122774




Ion Ratio Lower Upper


180 100

182 96.2 74.8 112.2

184 30.4 23.4 35.2

145 33.9 26.5 39.7


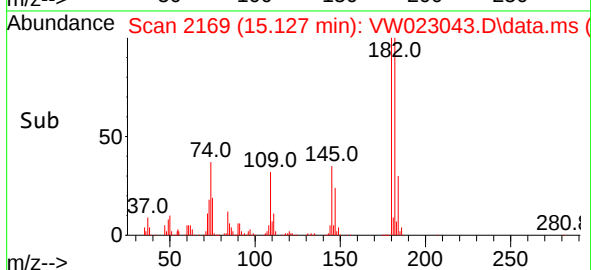






#70
1,2,4-trichlorobenzene
Concen: 20.455 ug/L
RT: 15.127 min Scan# 2169
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Instrument :
MSVOA_W
ClientSampleId :
X3A86

Tgt Ion:180 Resp: 122774
Ion Ratio Lower Upper
180 100
182 96.2 74.9 112.3
145 33.9 26.6 39.8

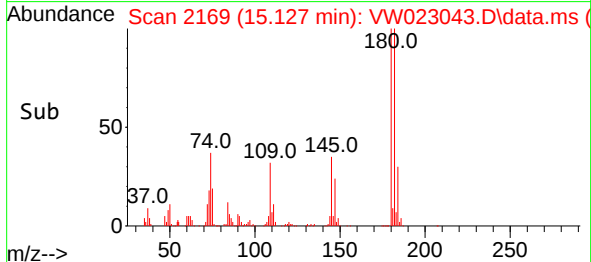

#72
1,2,3-Trichlorobenzene
Concen: 31.083 ug/L
RT: 15.554 min Scan# 2239
Delta R.T. 0.000 min
Lab File: VW023043.D
Acq: 16 May 2022 10:42

Tgt Ion:180 Resp: 165350
Ion Ratio Lower Upper
180 100
182 91.3 73.5 110.3
145 34.9 27.9 41.9

