

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
 Data File : VW023069.D
 Acq On : 16 May 2022 22:42
 Operator : SY/VA
 Sample : N2843-13
 Misc : 7.36g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4J3

Quant Time: May 17 03:13:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 17 02:41:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	259168	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	194699	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	50187	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	94982	17.863	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	71.440%
7) Chloroethane-d5	2.885	69	75181	21.733	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.920%
11) 1,1-Dichloroethene-d2	4.013	63	87539	12.741	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	50.960%
21) 2-Butanone-d5	7.080	46	49839	49.298	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.600%
24) Chloroform-d	7.647	84	179739	23.672	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.680%
26) 1,2-Dichloroethane-d4	8.494	65	102	0.024	ug/L	0.19
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.080%#
32) Benzene-d6	8.275	84	313269	27.915	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	111.640%
36) 1,2-Dichloropropane-d6	9.274	67	100732	31.954	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	127.800%#
41) Toluene-d8	10.323	98	248957	22.965	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.840%
43) trans-1,3-Dichloroprop...	10.579	79	31801	21.909	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.640%
47) 2-Hexanone-d5	10.920	63	36555	60.744	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.480%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	89329	30.402	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	121.600%#
66) 1,2-Dichlorobenzene-d4	13.847	152	44889	25.587	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.360%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	3150	0.732	ug/L	# 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
Data File : VW023069.D
Acq On : 16 May 2022 22:42
Operator : SY/VA
Sample : N2843-13
Misc : 7.36g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4J3

Quant Time: May 17 03:13:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 17 02:41:35 2022
Response via : Initial Calibration

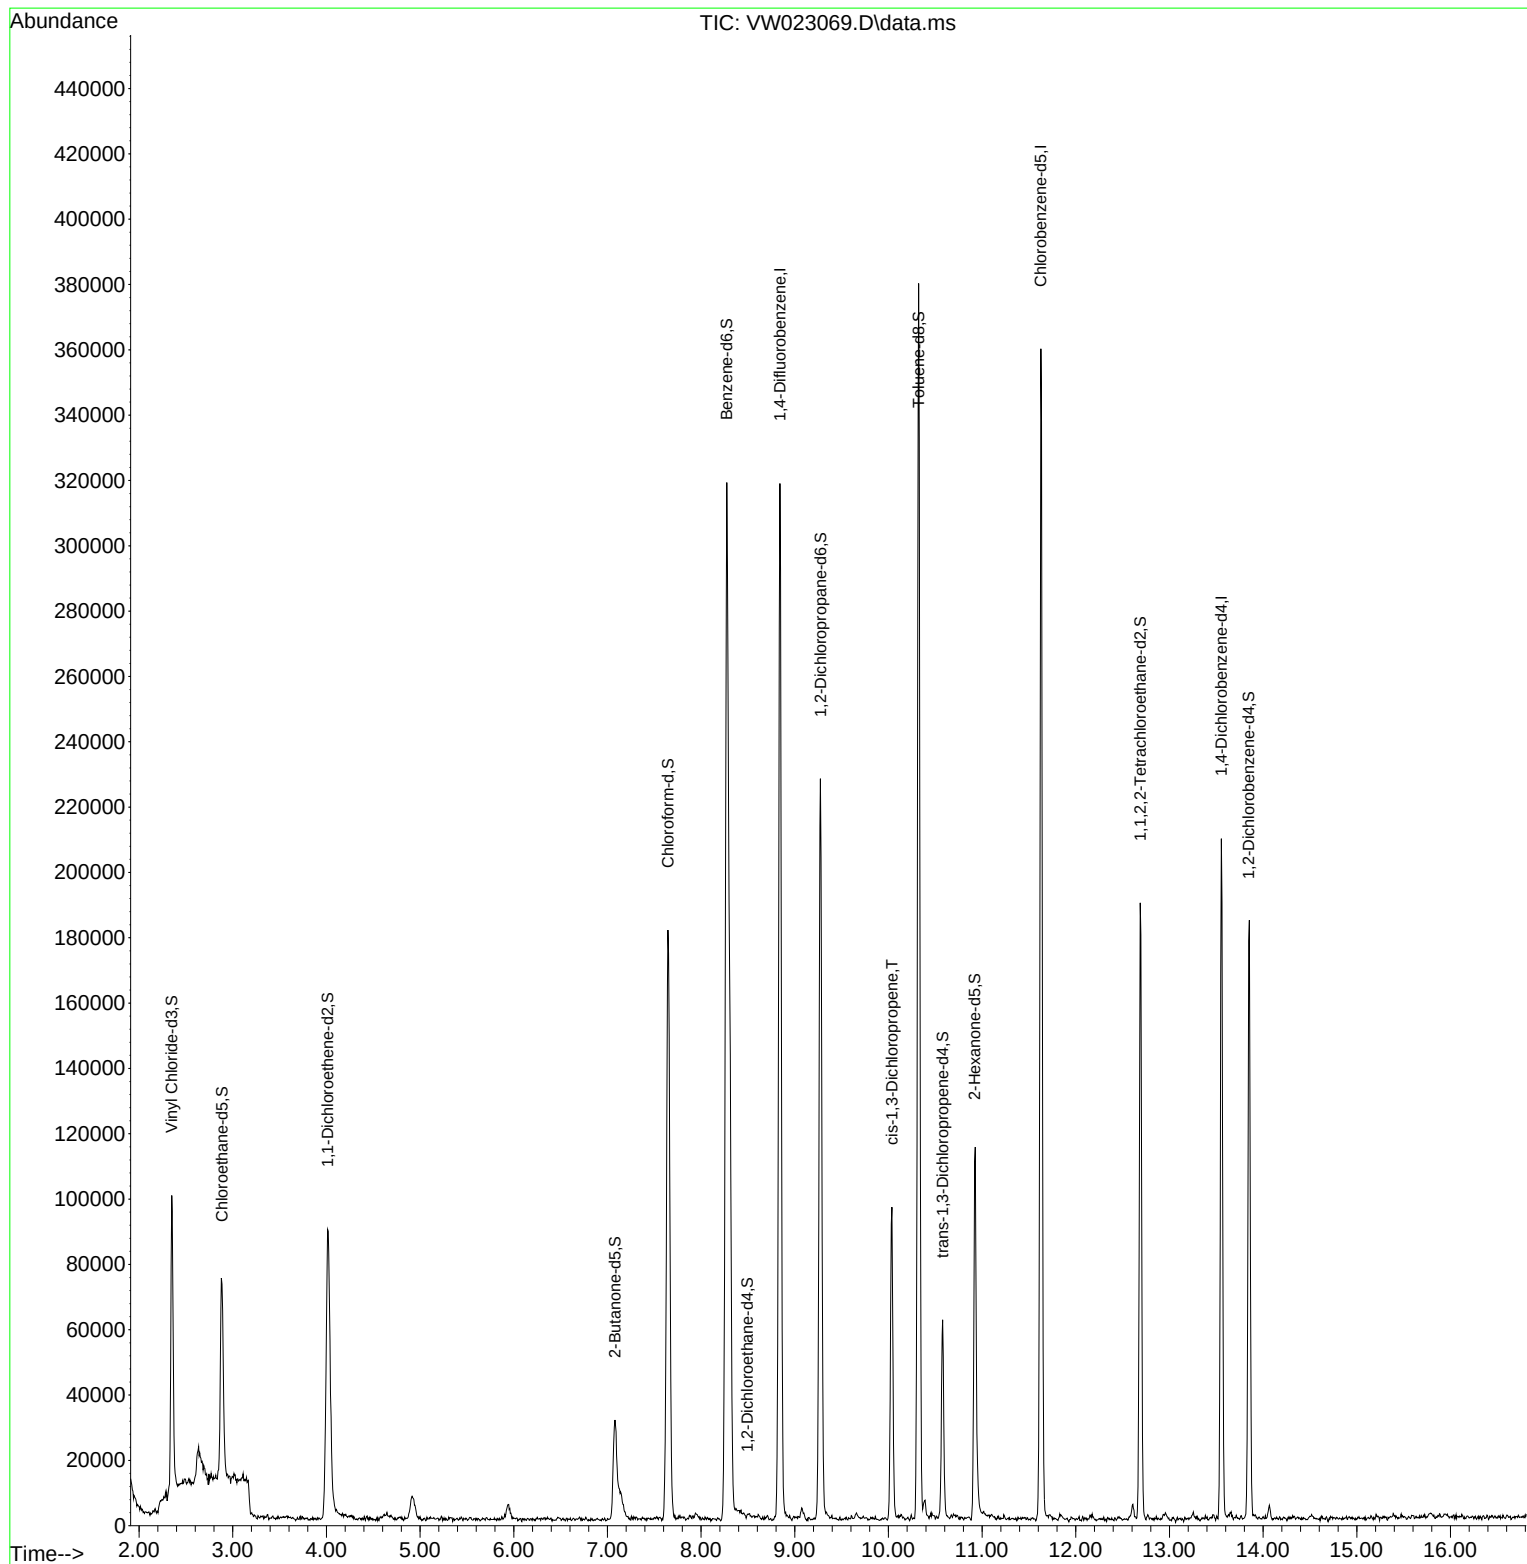

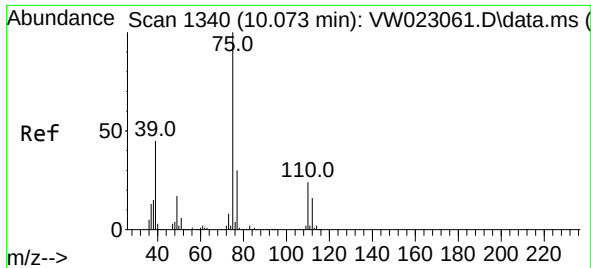

#39

cis-1,3-Dichloropropene

Concen: 0.732 ug/L

RT: 10.036 min Scan# 11

Delta R.T. -0.037 min

Lab File: VW023069.D


Acq: 16 May 2022 22:42

Instrument :

MSVOA_W

ClientSampleId :

EW4J3

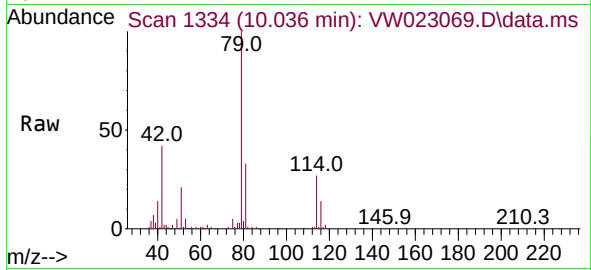

Tgt Ion: 75 Resp: 3150

Ion Ratio Lower Upper

75 100

77 50.8 22.1 41.1#

