

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
 Data File : VW023082.D
 Acq On : 17 May 2022 03:56
 Operator : SY/VA
 Sample : N2843-09
 Misc : 6.98g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW4H9

Quant Time: May 17 06:02:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 17 02:41:35 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	298557	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	252699	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	94595	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	89176	14.559	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.240%
7) Chloroethane-d5	2.885	69	69792	17.514	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.040%
11) 1,1-Dichloroethene-d2	4.013	63	96158	12.149	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.600%
21) 2-Butanone-d5	7.080	46	44466	38.181	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.360%
24) Chloroform-d	7.653	84	196396	22.453	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.800%
26) 1,2-Dichloroethane-d4	8.305	65	114549	23.877	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.520%
32) Benzene-d6	8.275	84	340278	23.362	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.440%
36) 1,2-Dichloropropane-d6	9.274	67	110535	27.016	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	108.080%
41) Toluene-d8	10.323	98	290524	20.648	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	10.579	79	34541	18.335	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	73.360%
47) 2-Hexanone-d5	10.927	63	34279	43.888	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.780%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	107512	28.192	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.760%
66) 1,2-Dichlorobenzene-d4	13.853	152	74371	22.491	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.960%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.030	75	3106	0.556	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
Data File : VW023082.D
Acq On : 17 May 2022 03:56
Operator : SY/VA
Sample : N2843-09
Misc : 6.98g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW4H9

Quant Time: May 17 06:02:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 17 02:41:35 2022
Response via : Initial Calibration

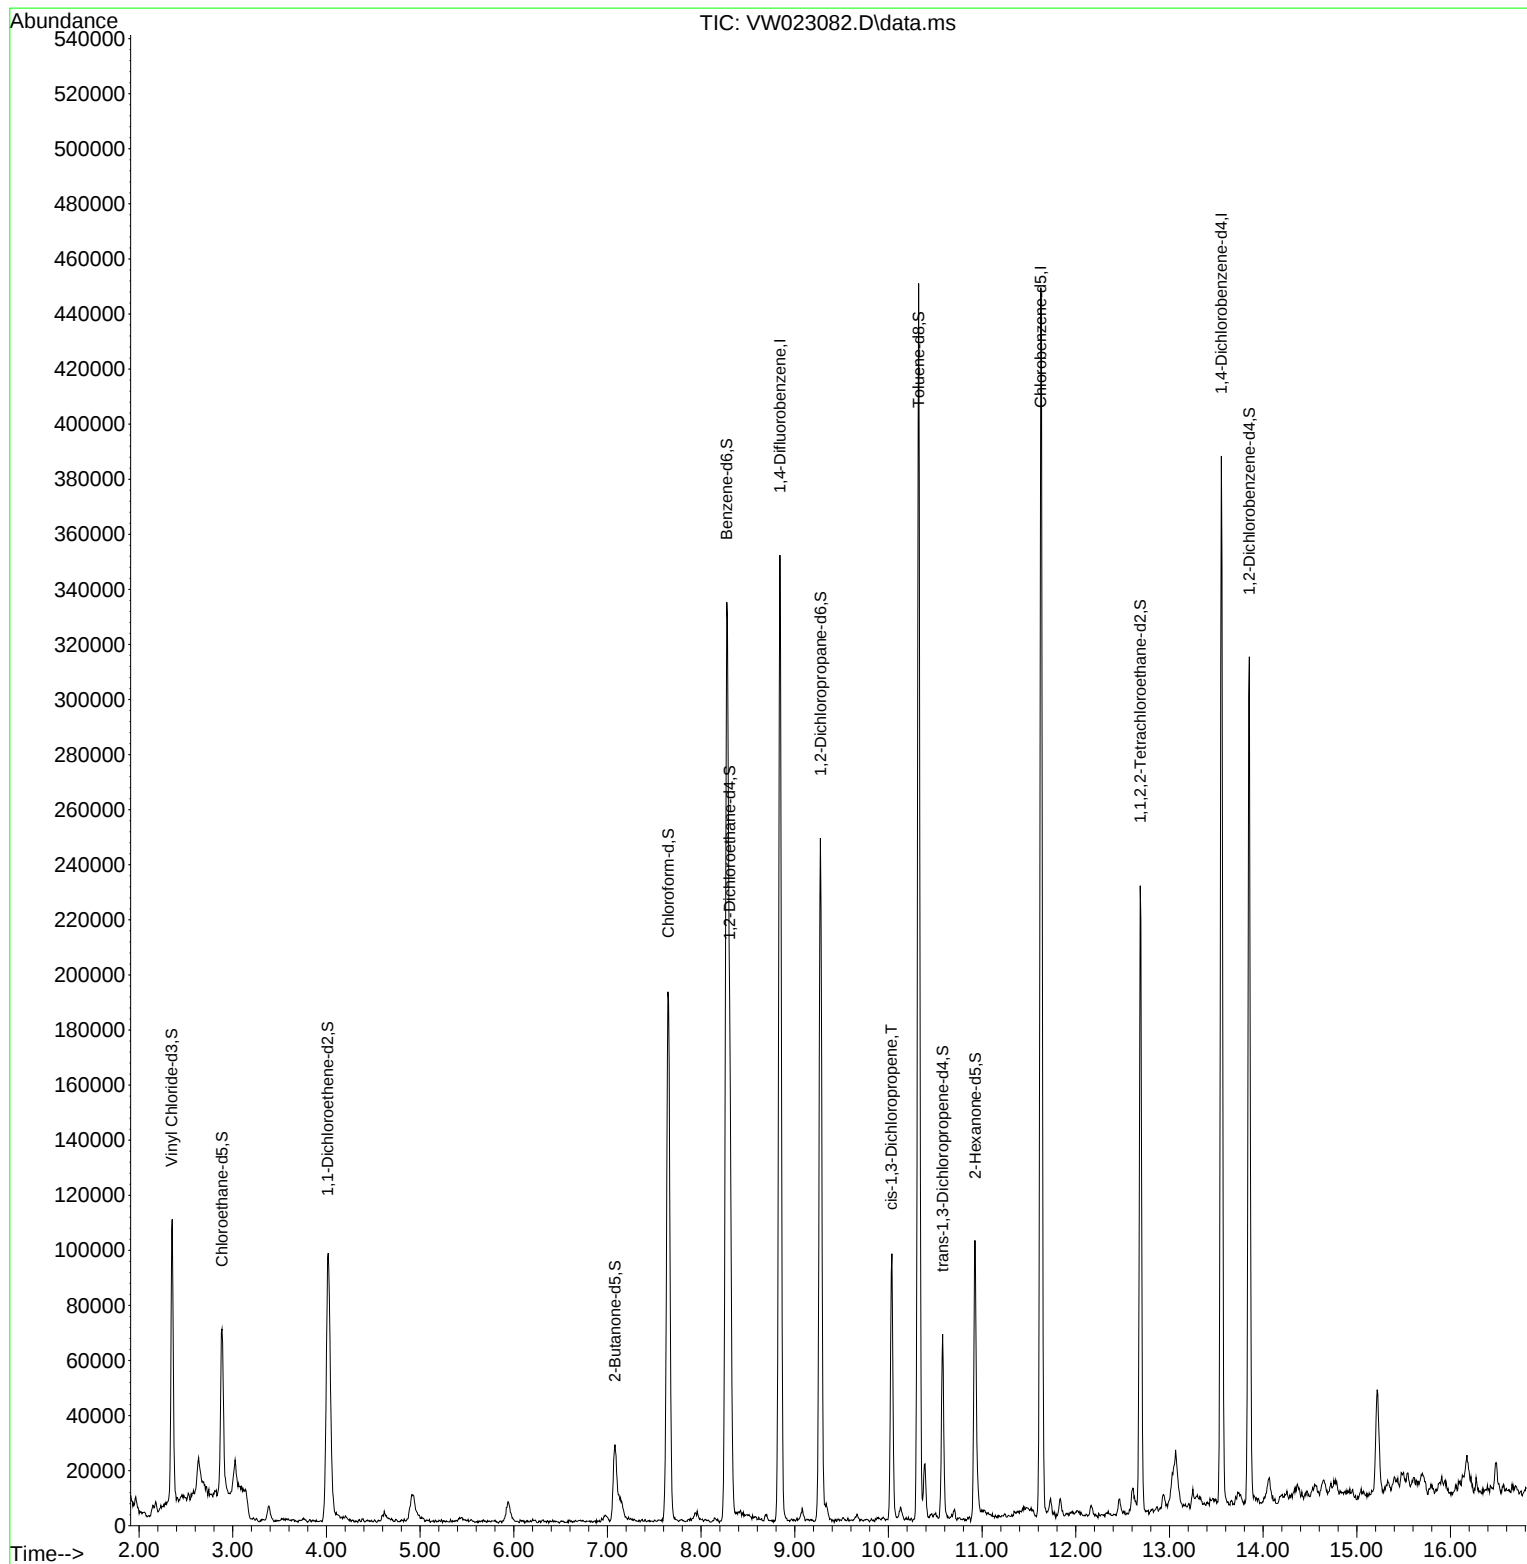

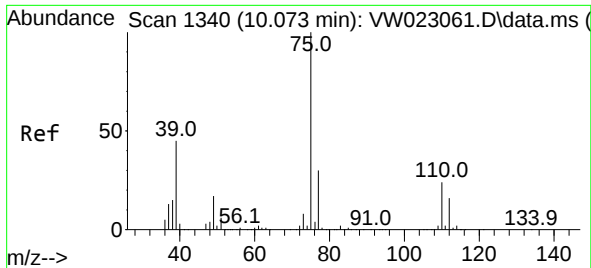

#39

cis-1,3-Dichloropropene

Concen: 0.556 ug/L

RT: 10.030 min Scan# 11

Delta R.T. -0.043 min

Lab File: VW023082.D


Acq: 17 May 2022 03:56

Instrument :

MSVOA_W

ClientSampleId :

EW4H9

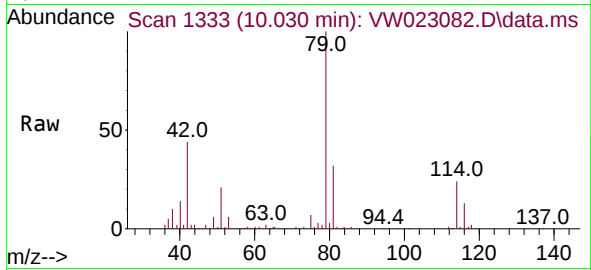

Tgt Ion: 75 Resp: 3106

Ion Ratio Lower Upper

75 100

77 39.0 22.1 41.1

