




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
 Data File : VW023045.D
 Acq On : 16 May 2022 11:56
 Operator : SY/VA
 Sample : N2767-09RE
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM4RE

Manual IntegrationsAPPROVED

Quant Time: May 17 01:26:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 17 01:24:30 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/17/2022
 Supervised By :Mahesh Dadoda 05/18/2022

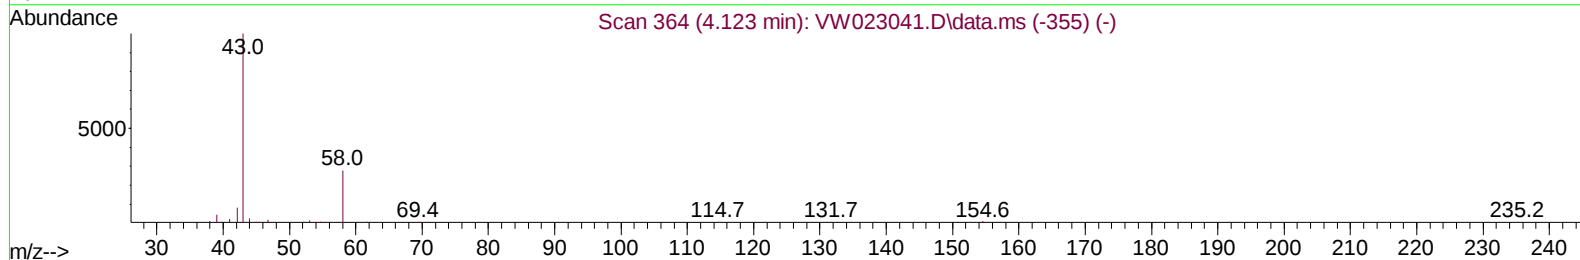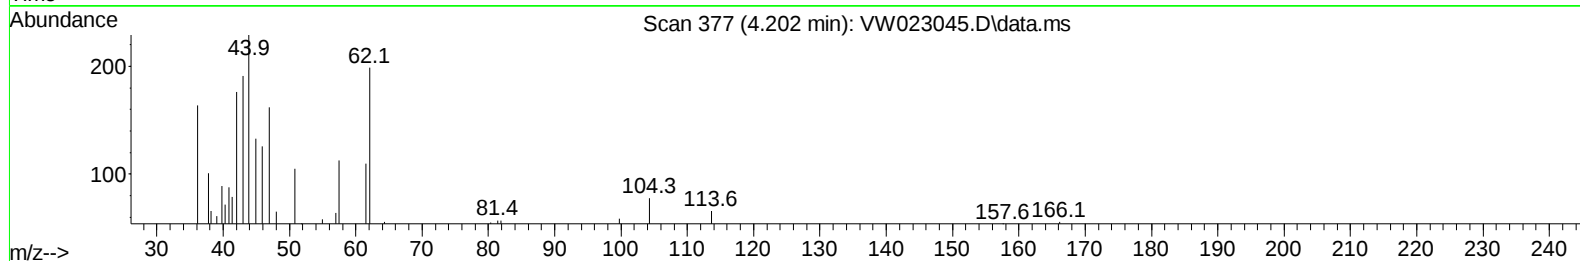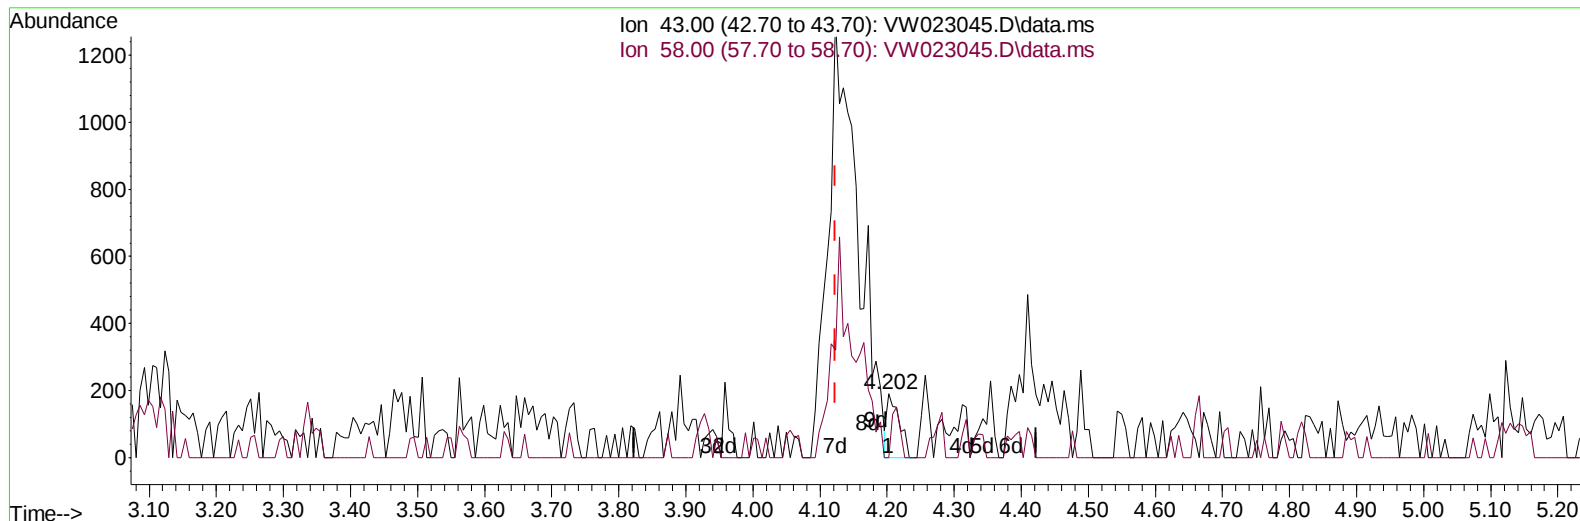

TIC: VW023045.D\data.ms

(13) Acetone (T)

4.202min (+ 0.079) 0.99 ug/L

response 240

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	53.75
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
 Data File : VW023045.D
 Acq On : 16 May 2022 11:56
 Operator : SY/VA
 Sample : N2767-09RE
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2022
 Supervised By :Mahesh Dadoda 05/18/2022

Quant Time: May 17 01:26:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 17 01:24:30 2022
 Response via : Initial Calibration

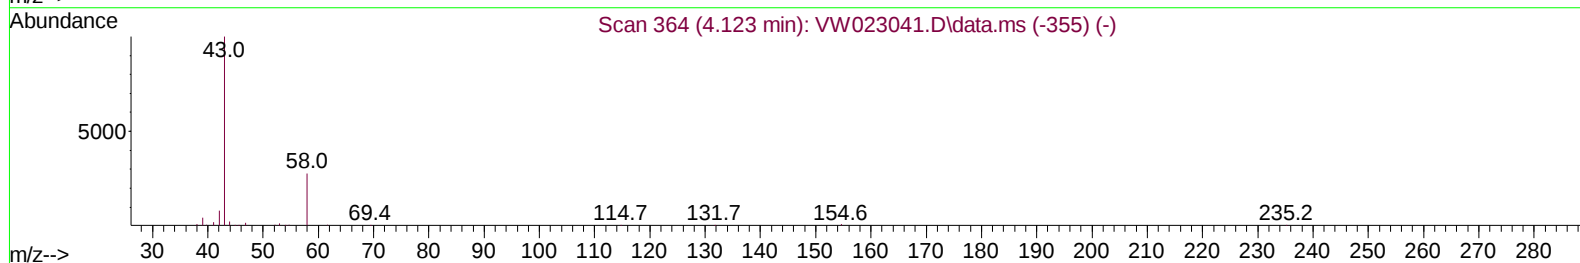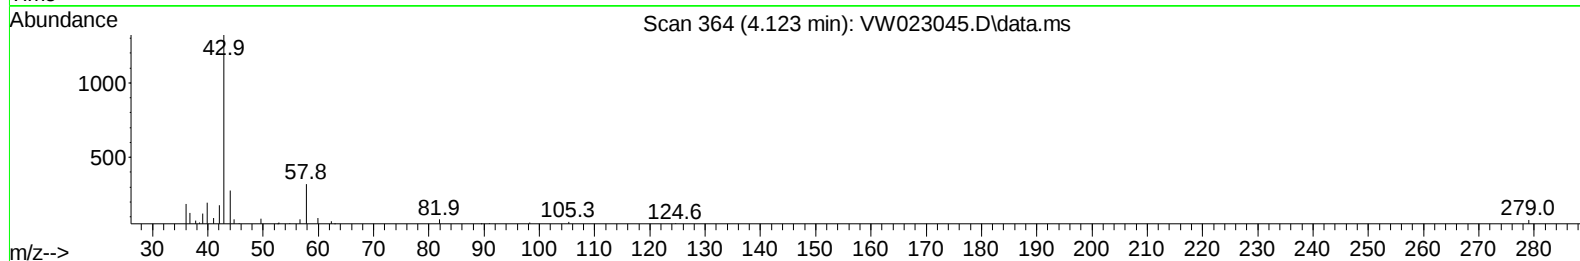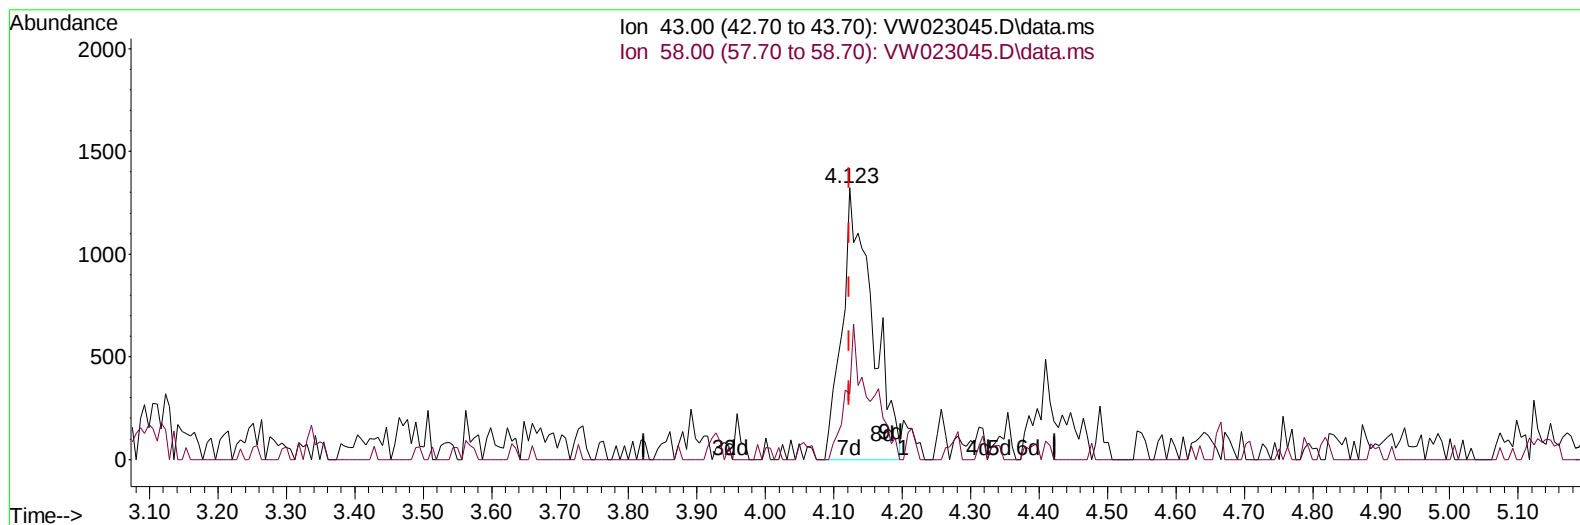

TIC: VW023045.D\data.ms

(13) Acetone (T)

4.123min (+ 0.000) 16.62 ug/L m

response 4017

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	3.21
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
 Data File : VW023045.D
 Acq On : 16 May 2022 11:56
 Operator : SY/VA
 Sample : N2767-09RE
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGPM4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2022
 Supervised By :Mahesh Dadoda 05/18/2022

Quant Time: May 17 01:26:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 17 01:24:30 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	82773	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	63709	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	16998	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	31484	18.540	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	74.160%	
7) Chloroethane-d5	2.885	69	31926	28.897	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	115.600%	
11) 1,1-Dichloroethene-d2	4.013	63	34456	15.703	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	62.800%	
21) 2-Butanone-d5	7.086	46	18976	58.770	ug/L	0.01
Spiked Amount 50.000	Range 20	- 135	Recovery	=	117.540%	
24) Chloroform-d	7.653	84	60655	25.012	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	100.040%	
26) 1,2-Dichloroethane-d4	8.305	65	34186	25.703	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	102.800%	
32) Benzene-d6	8.275	84	103753	28.254	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	113.000%	
36) 1,2-Dichloropropane-d6	9.274	67	33124	32.112	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	128.440%#	
41) Toluene-d8	10.323	98	83303	23.483	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	93.920%	
43) trans-1,3-Dichloroprop...	10.579	79	11106	23.383	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	93.520%	
47) 2-Hexanone-d5	10.927	63	12460	63.276	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	126.560%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	29485	30.667	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	122.680%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	13608	22.902	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	91.600%	
Target Compounds					Qvalue	
13) Acetone	4.123	43	4017m	16.617	ug/L	
46) Tetrachloroethene	10.866	164	1448	1.867	ug/L #	61
52) Ethylbenzene	11.731	91	28921	6.181	ug/L	91
53) m,p-Xylene	11.835	106	46442	25.188	ug/L	93
54) o-Xylene	12.164	106	14277	8.069	ug/L	100
62) 1,3,5-Trimethylbenzene	12.944	105	647	0.499	ug/L #	82
63) 1,2,4-Trimethylbenzene	13.249	105	1102	0.567	ug/L #	67

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW051622\
Data File : VW023045.D
Acq On : 16 May 2022 11:56
Operator : SY/VA
Sample : N2767-09RE
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGPM4RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/17/2022
Supervised By :Mahesh Dadoda 05/18/2022

Quant Time: May 17 01:26:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 17 01:24:30 2022
Response via : Initial Calibration

