




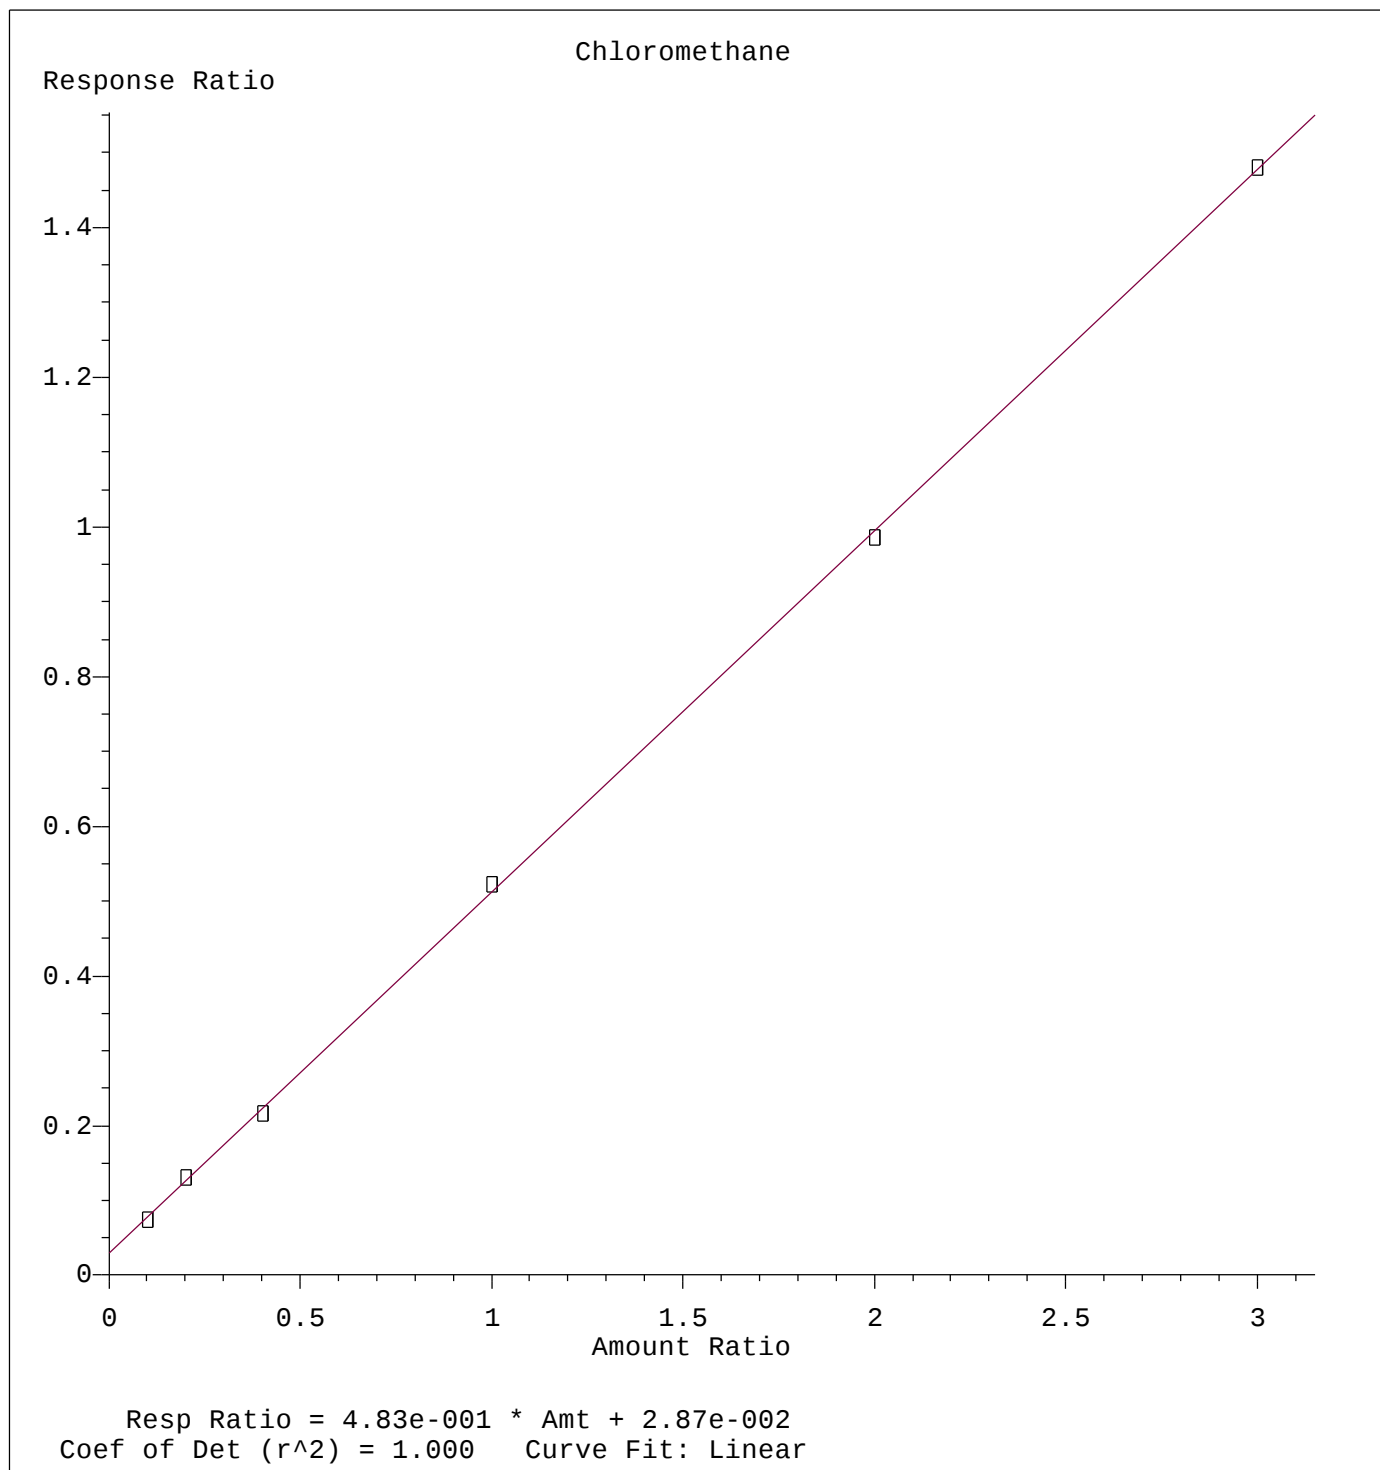

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051719S.M
Calibration Table Last Updated: Sat May 18 01:59:40 2019

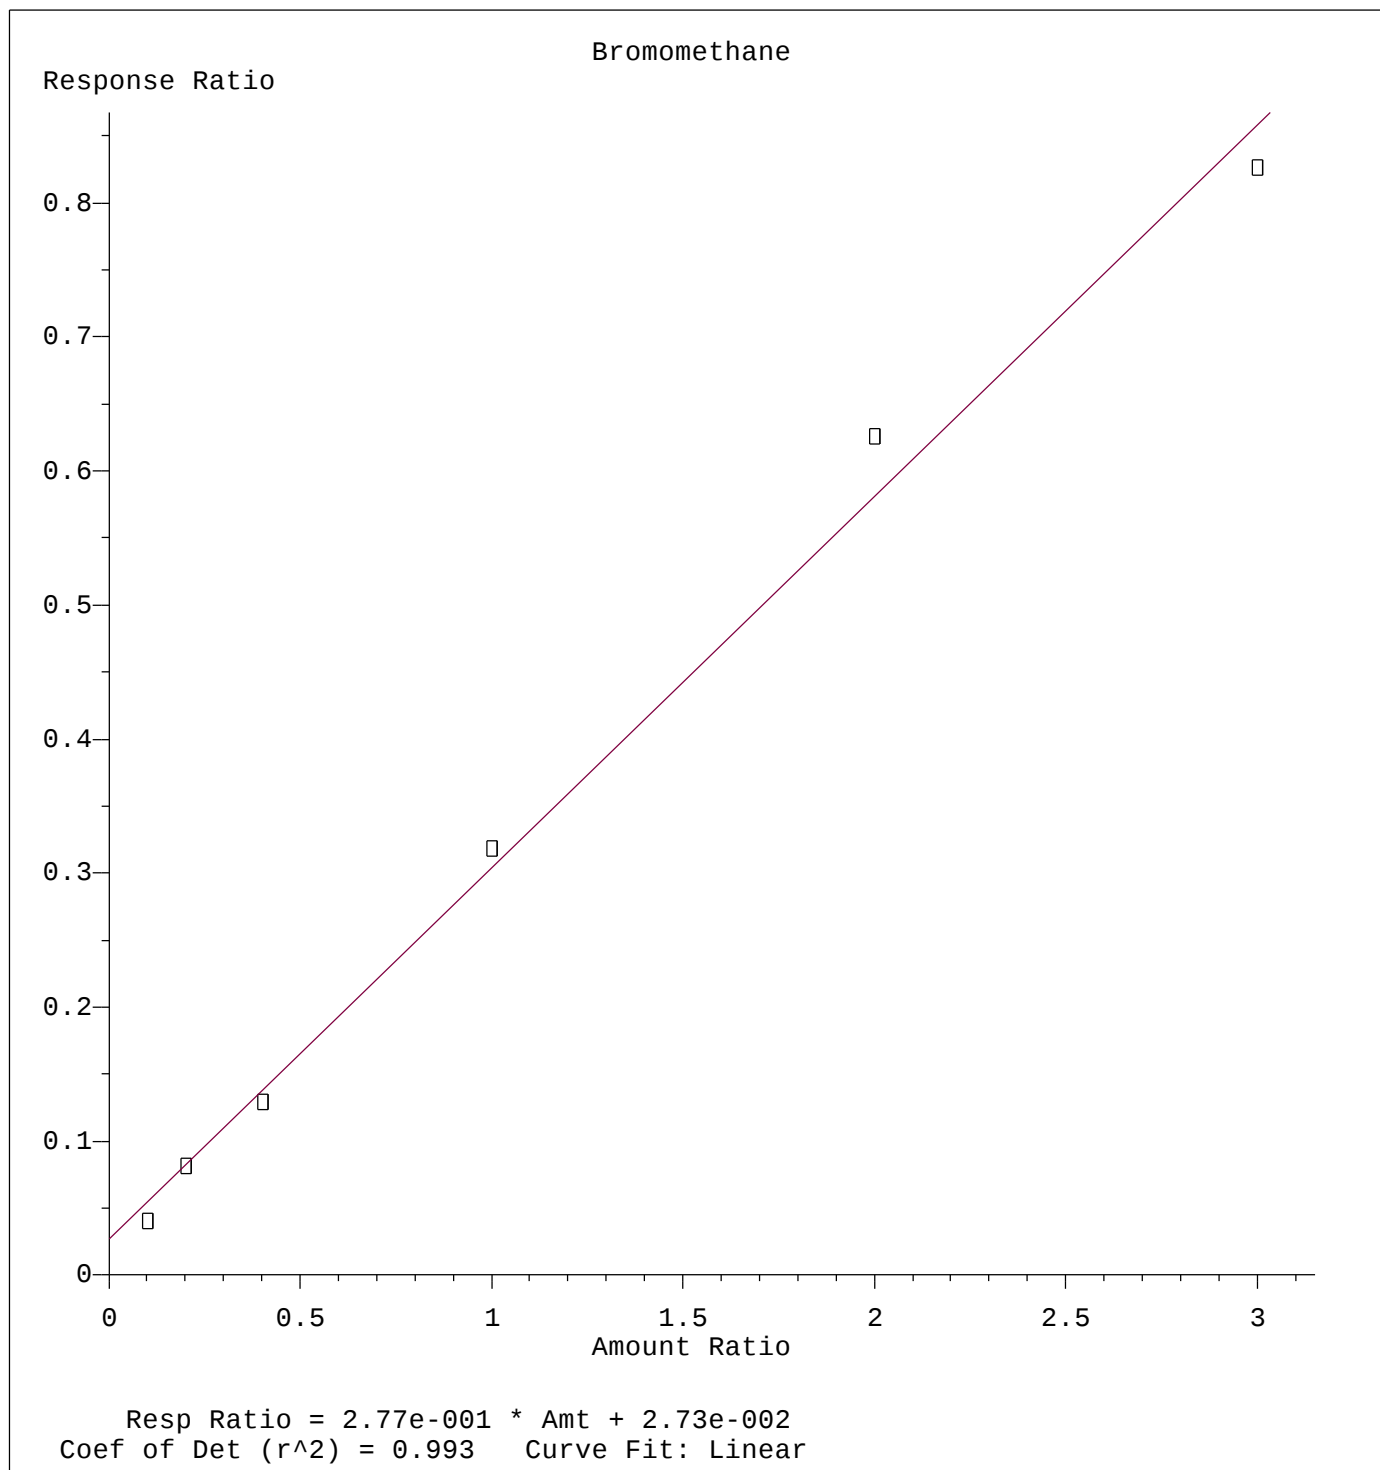


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051719S.M
Calibration Table Last Updated: Sat May 18 01:59:40 2019

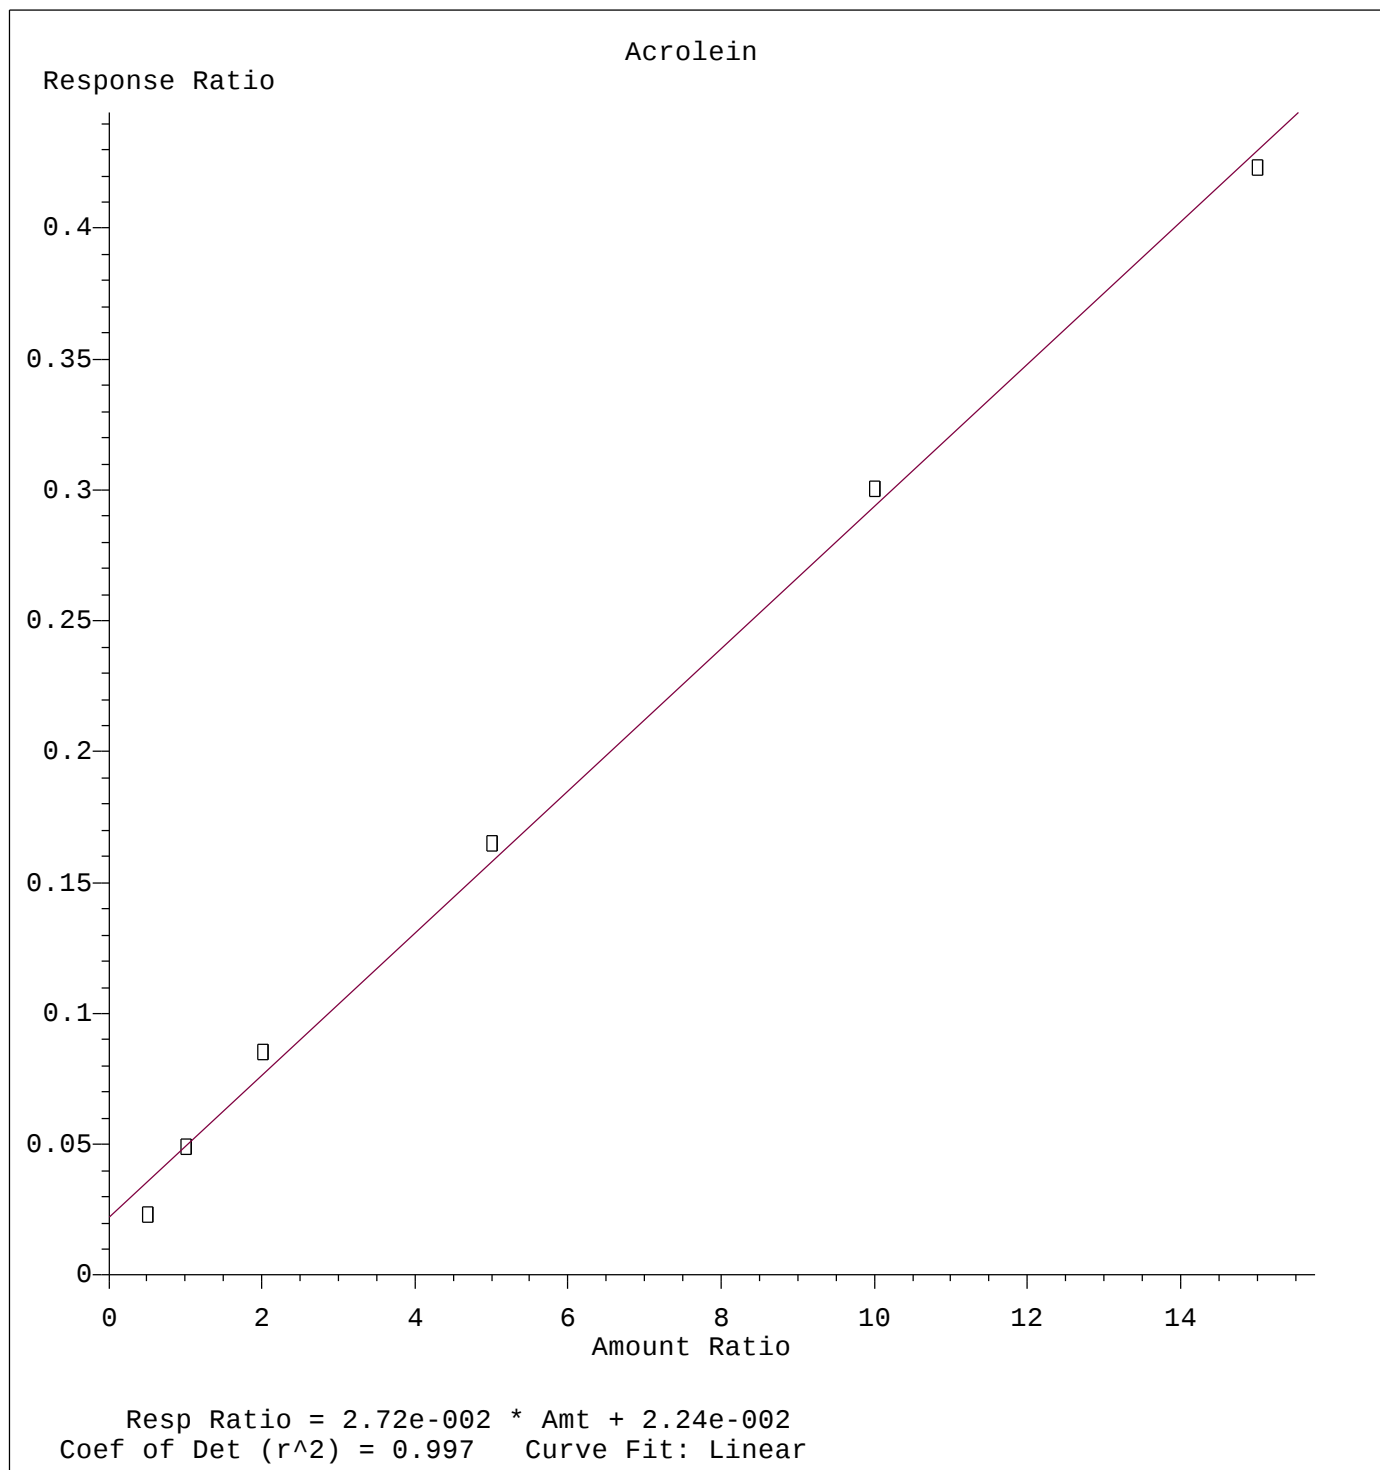

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051719S.M
Calibration Table Last Updated: Sat May 18 01:59:40 2019


Methylene Chloride

Response Ratio

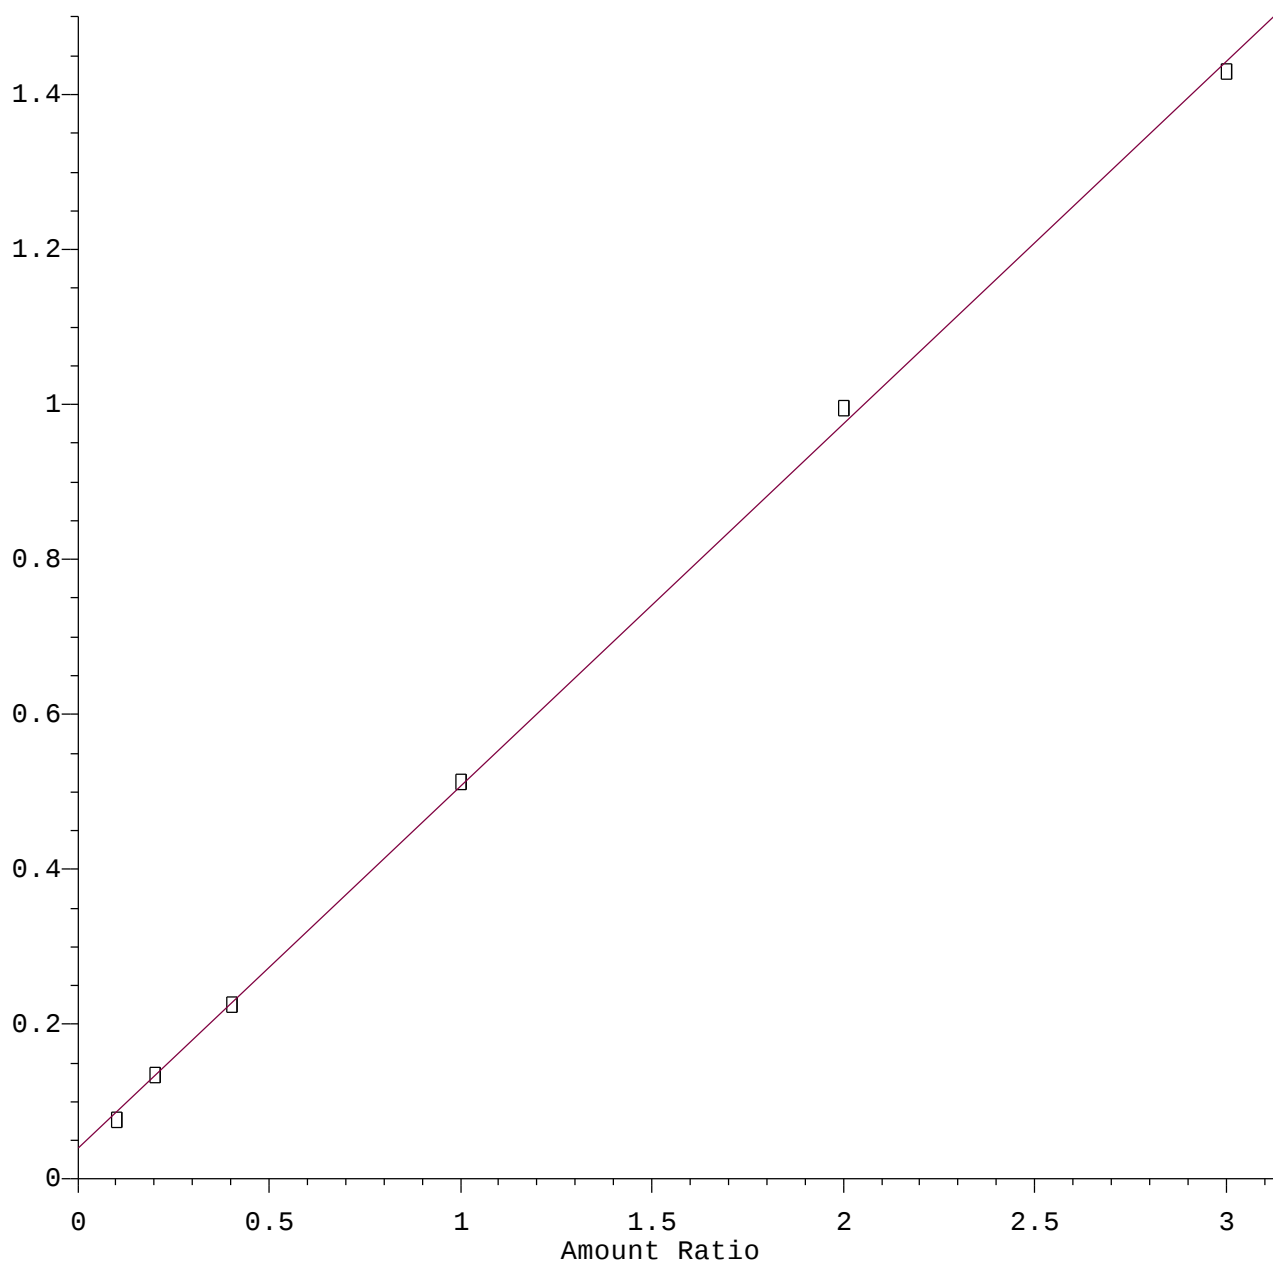

Resp Ratio = $4.68 \times 10^{-1} \times \text{Amt} + 3.88 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051719S.M
Calibration Table Last Updated: Sat May 18 01:59:40 2019

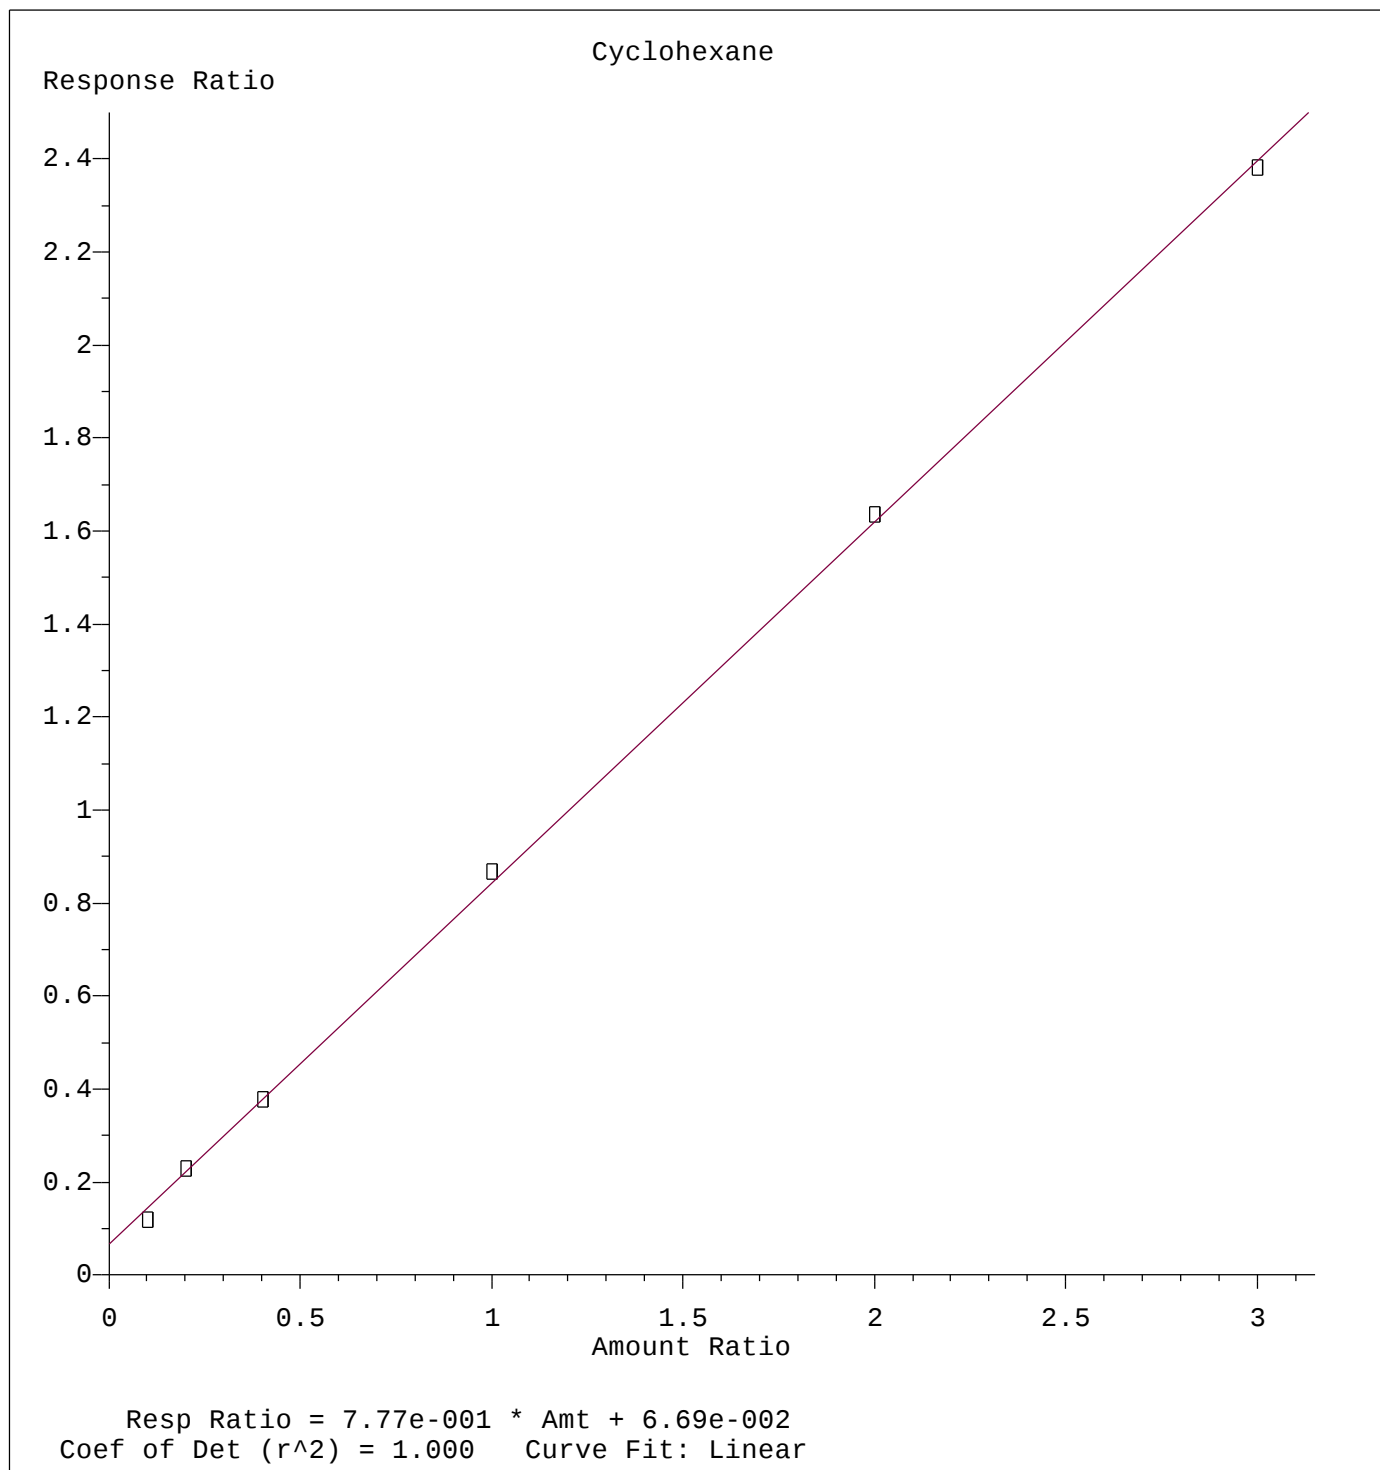

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051719S.M
Calibration Table Last Updated: Sat May 18 01:59:40 2019

Dichlorodifluoromethane

Response Ratio

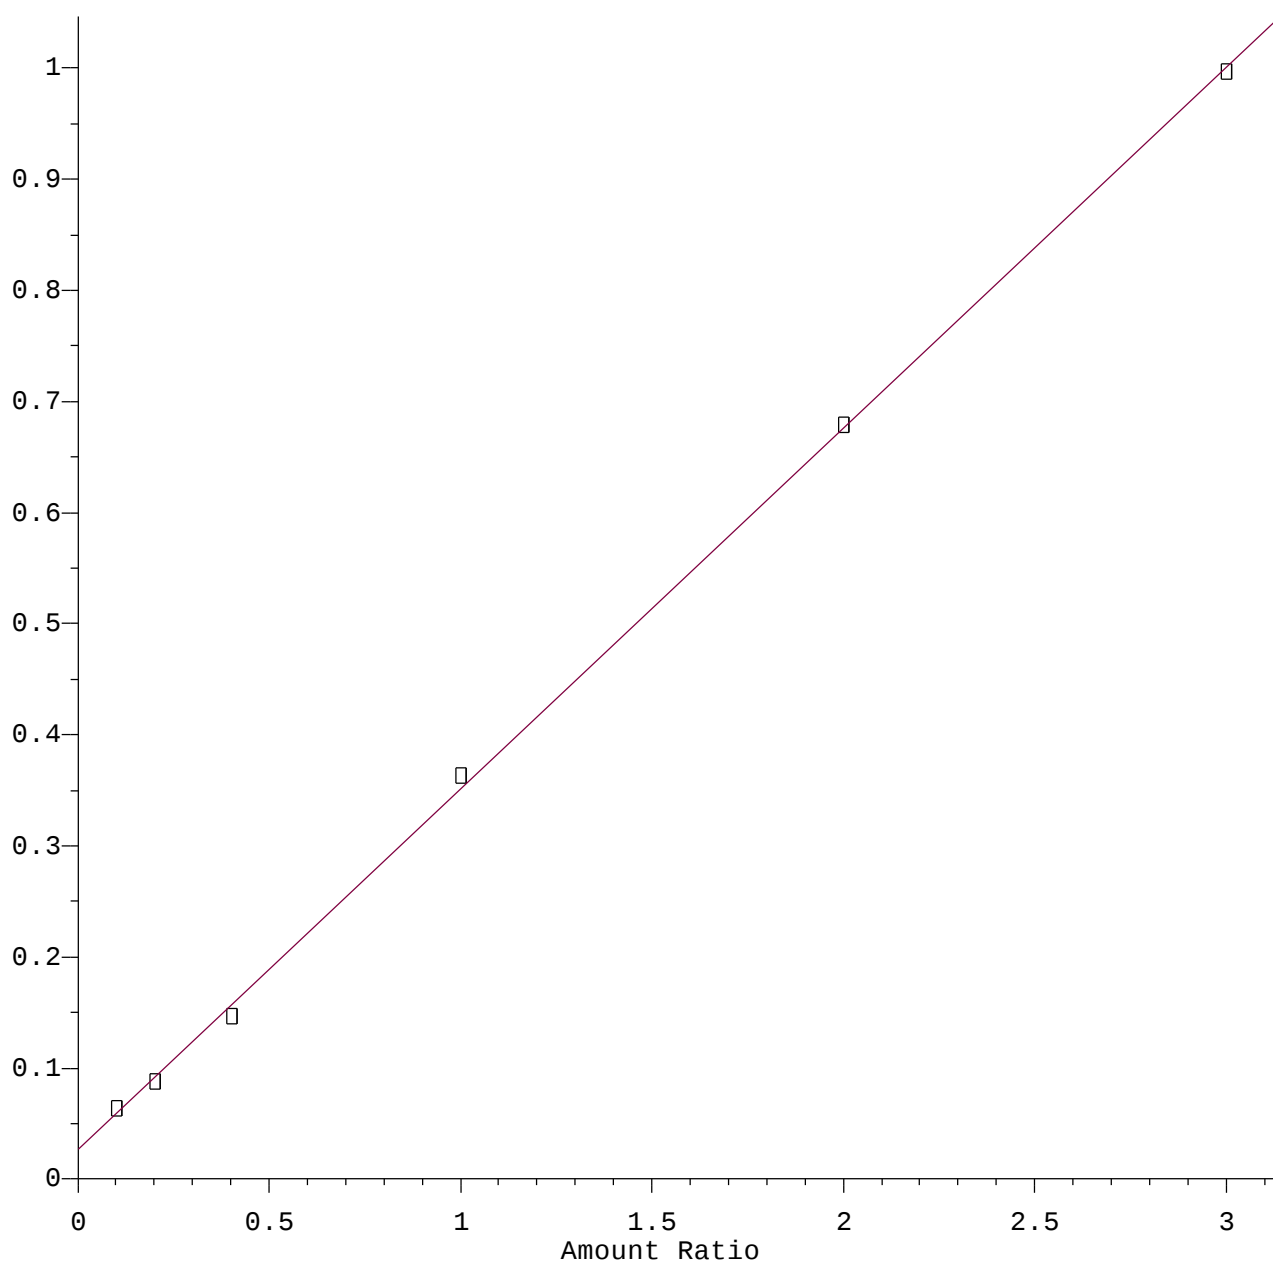

Resp Ratio = $3.25 \times 10^{-1} \times \text{Amt} + 2.64 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051719S.M
Calibration Table Last Updated: Sat May 18 01:59:40 2019