


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW051719\
 Data File : VW010424.D
 Acq On : 17 May 2019 20:35
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W051719S.M
 Title : SW846 8260
 Last Update : Sat May 18 01:59:40 2019

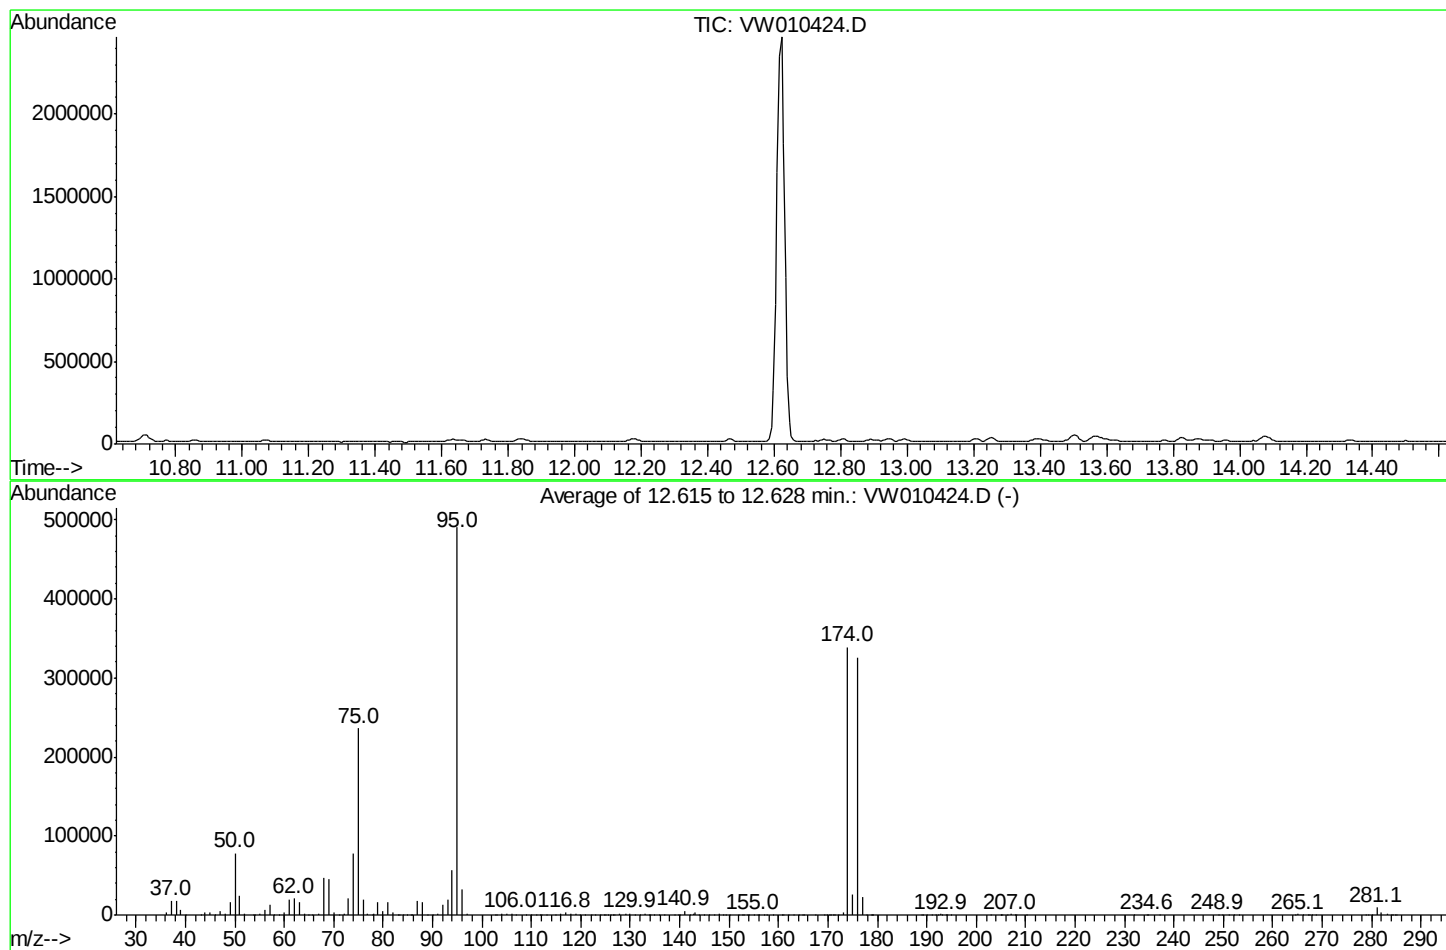

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1745

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	78478	PASS
75	95	30	60	48.1	235754	PASS
95	95	100	100	100.0	490470	PASS
96	95	5	9	6.6	32370	PASS
173	174	0.00	2	0.8	2552	PASS
174	95	50	100	69.1	339008	PASS
175	174	5	9	7.8	26586	PASS
176	174	95	101	95.9	325184	PASS
177	176	5	9	6.8	22138	PASS