


Toluene-d8

Response Ratio

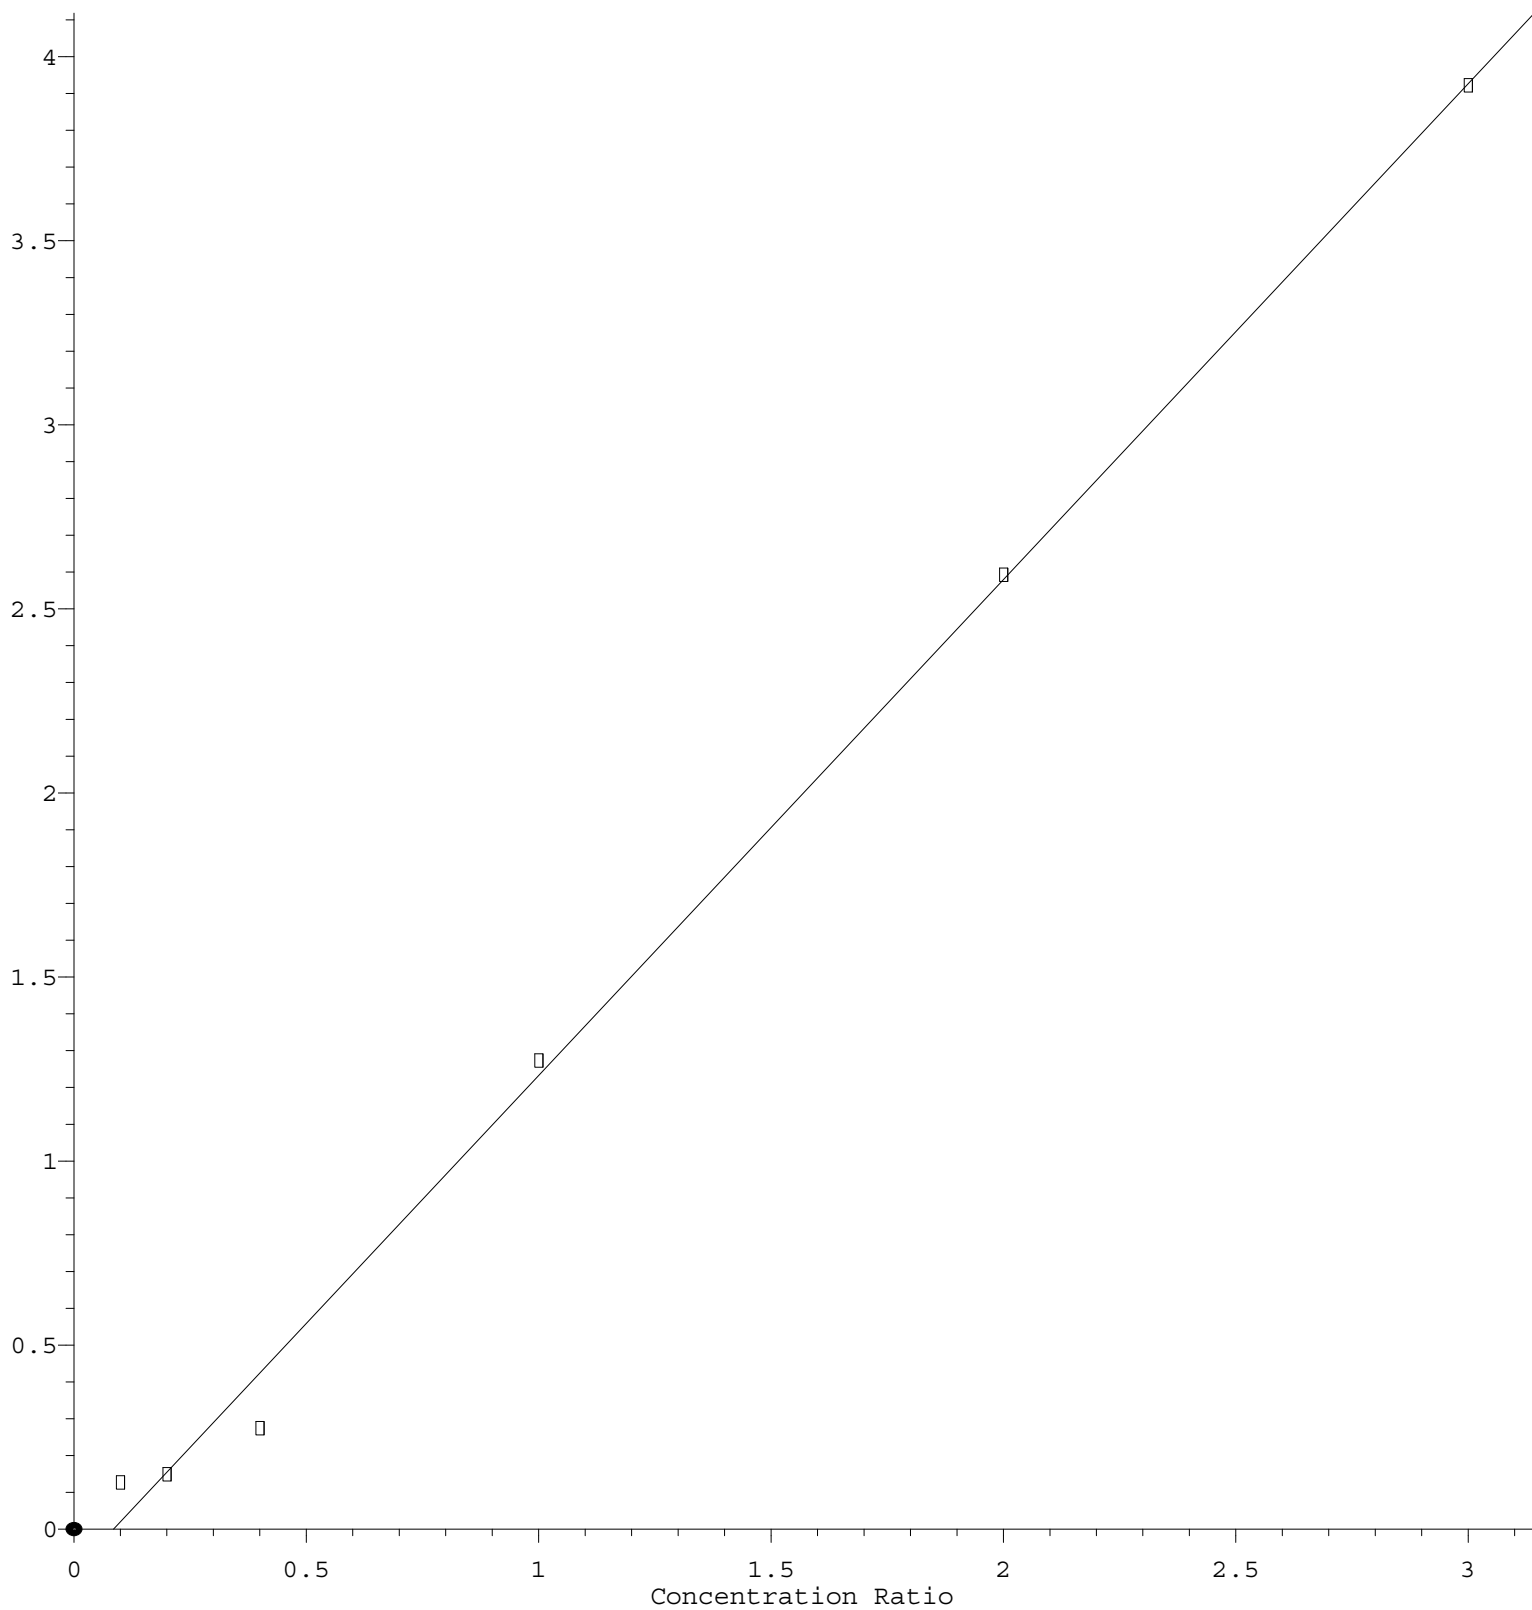

$$\text{Response} = 1.347\text{e}+000 * \text{Amt} - 1.151\text{e}-001$$


Coef of Det (r^2) = 0.997079 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W051921S.M

Calibration Table Last Updated: Thu May 20 03:59:48 2021

4-Bromofluorobenzene

Response Ratio

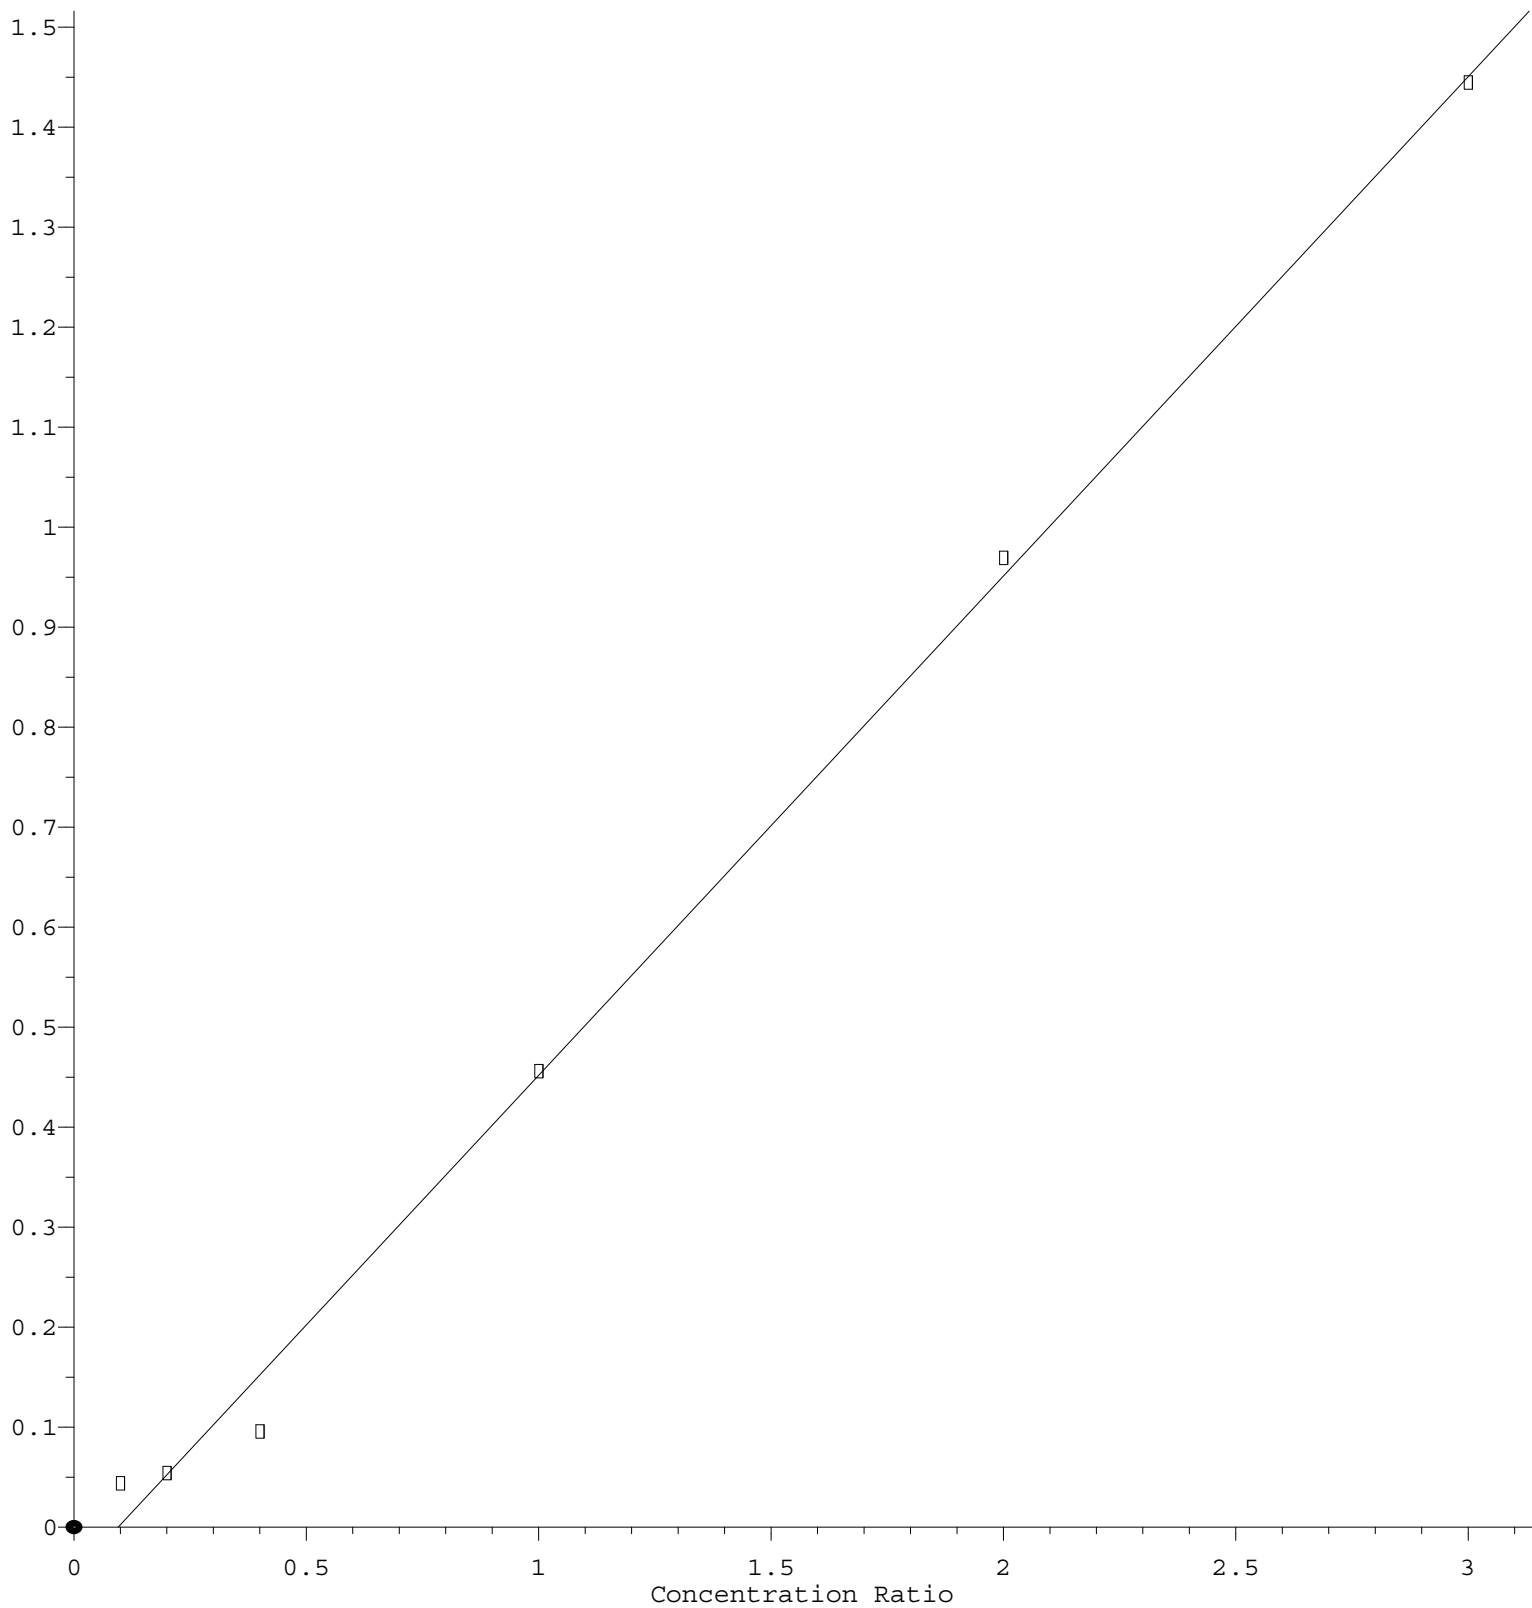

$$\text{Response} = 4.995\text{e-}001 * \text{Amt} - 4.727\text{e-}002$$


Coef of Det (r^2) = 0.996854 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W051921S.M

Calibration Table Last Updated: Thu May 20 03:59:48 2021

Methylene Chloride

Response Ratio

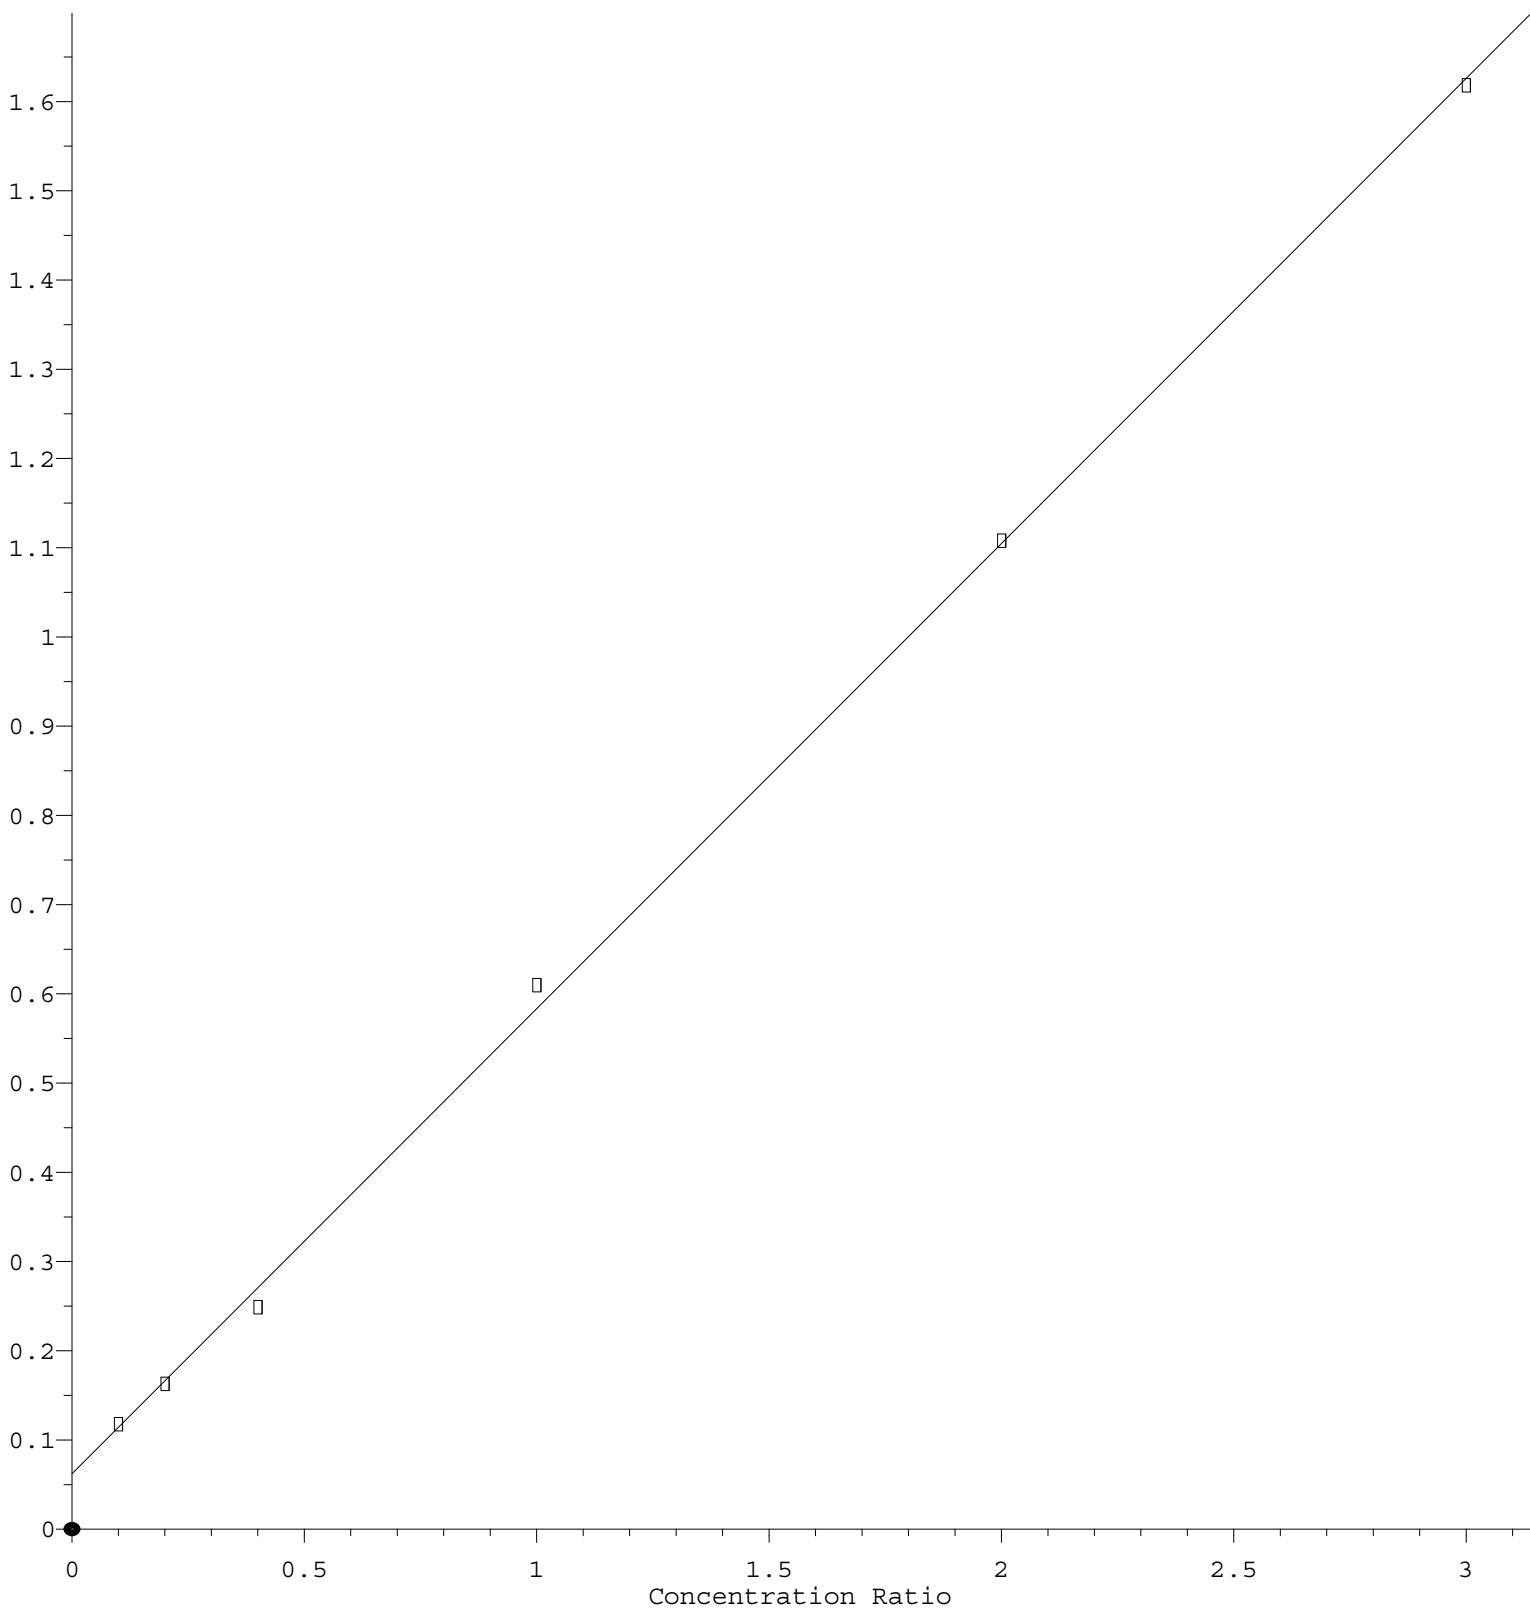

$$\text{Response} = 5.214\text{e-}001 * \text{Amt} + 6.198\text{e-}002$$


Coef of Det (r^2) = 0.999307 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W051921S.M

Calibration Table Last Updated: Thu May 20 03:59:48 2021

1,2-Dichloroethane-d4

Response Ratio

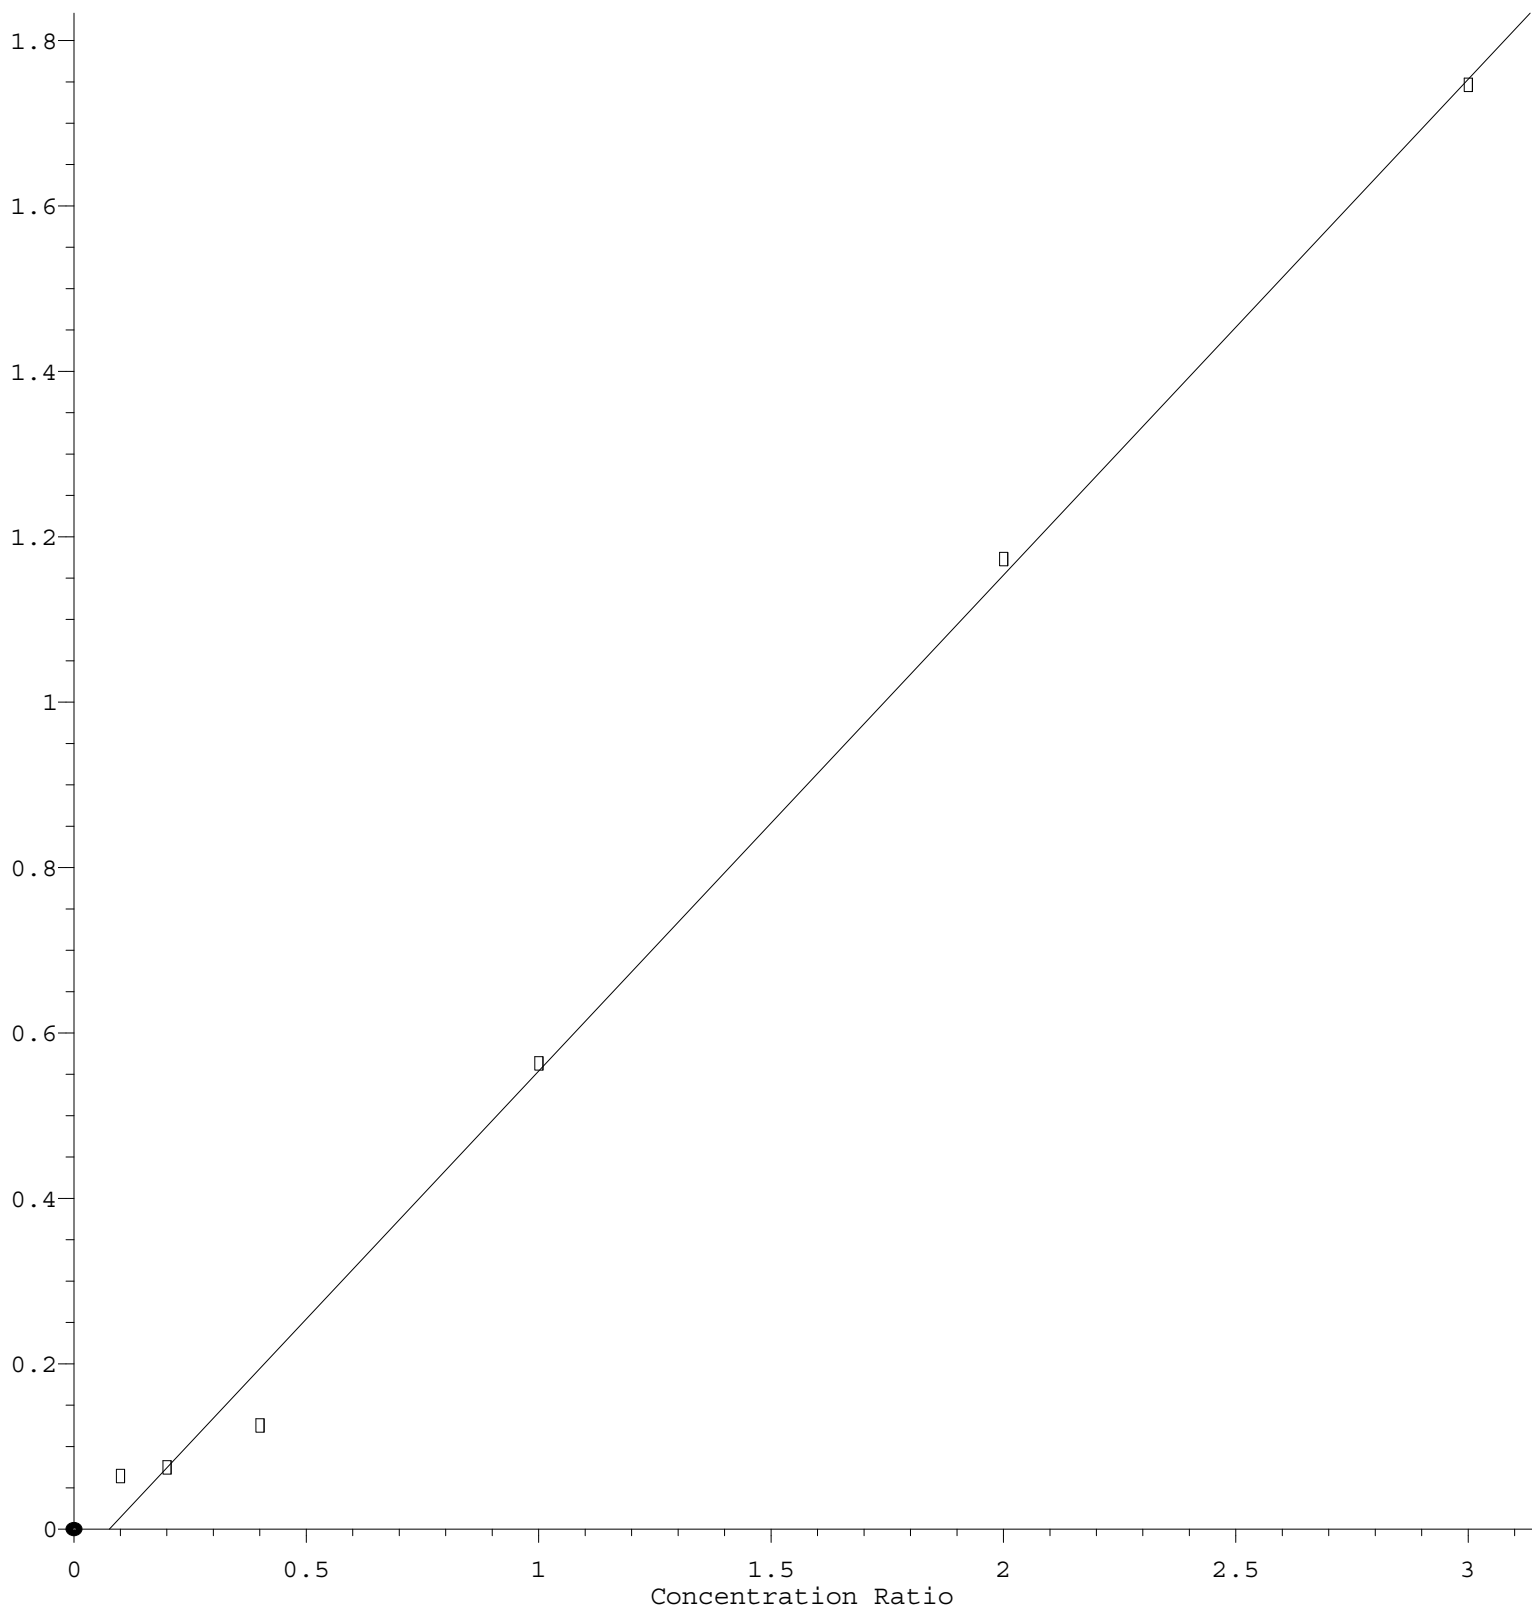

$$\text{Response} = 5.998\text{e-}001 * \text{Amt} - 4.538\text{e-}002$$


Coef of Det (r^2) = 0.996818 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W051921S.M

Calibration Table Last Updated: Thu May 20 03:59:48 2021

Dibromofluoromethane

Response Ratio

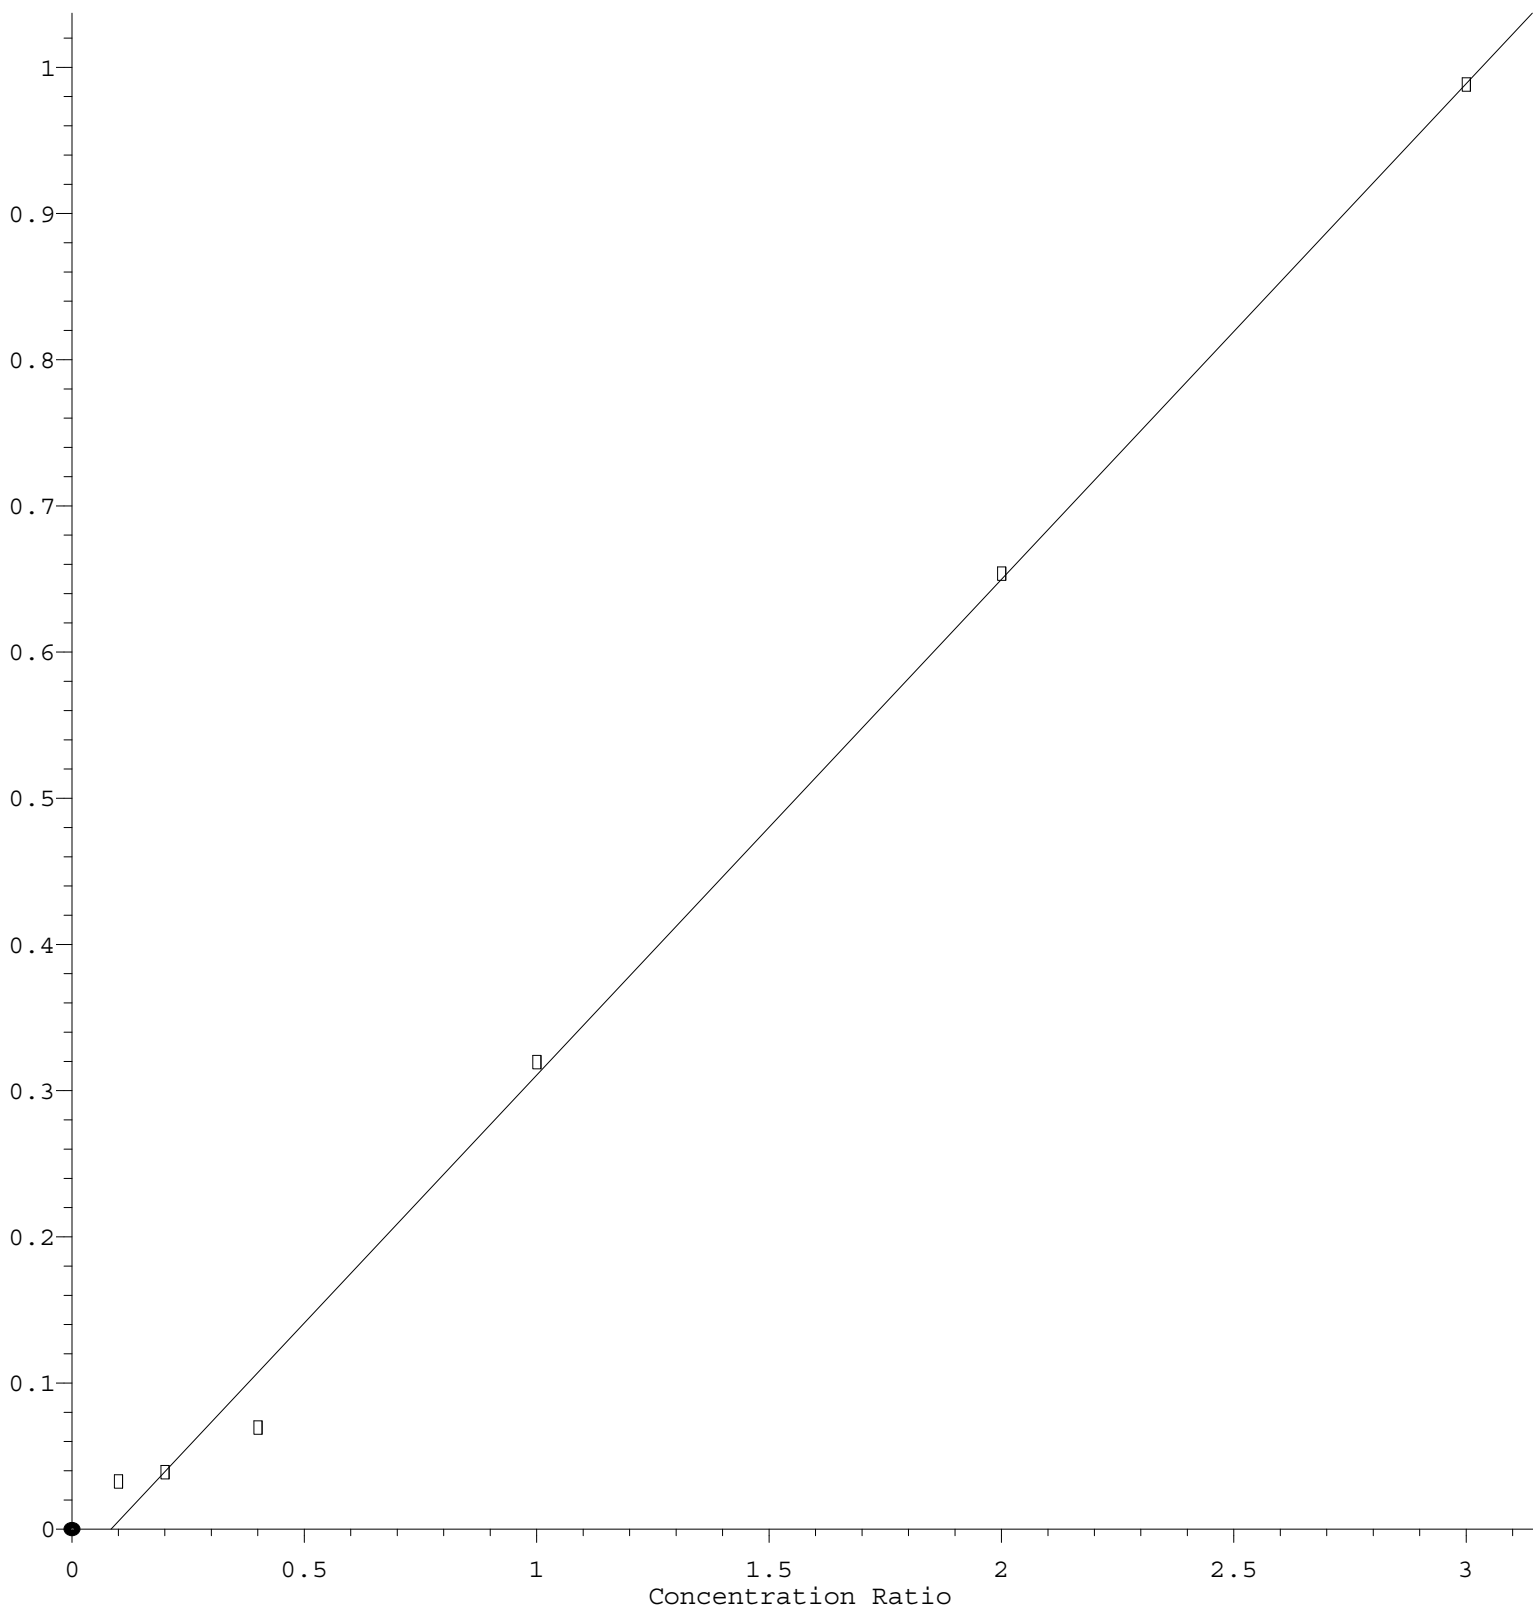

$$\text{Response} = 3.392\text{e-}001 * \text{Amt} - 2.843\text{e-}002$$


Coef of Det (r^2) = 0.997098 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W051921S.M

Calibration Table Last Updated: Thu May 20 03:59:48 2021

Tert butyl alcohol

Response Ratio

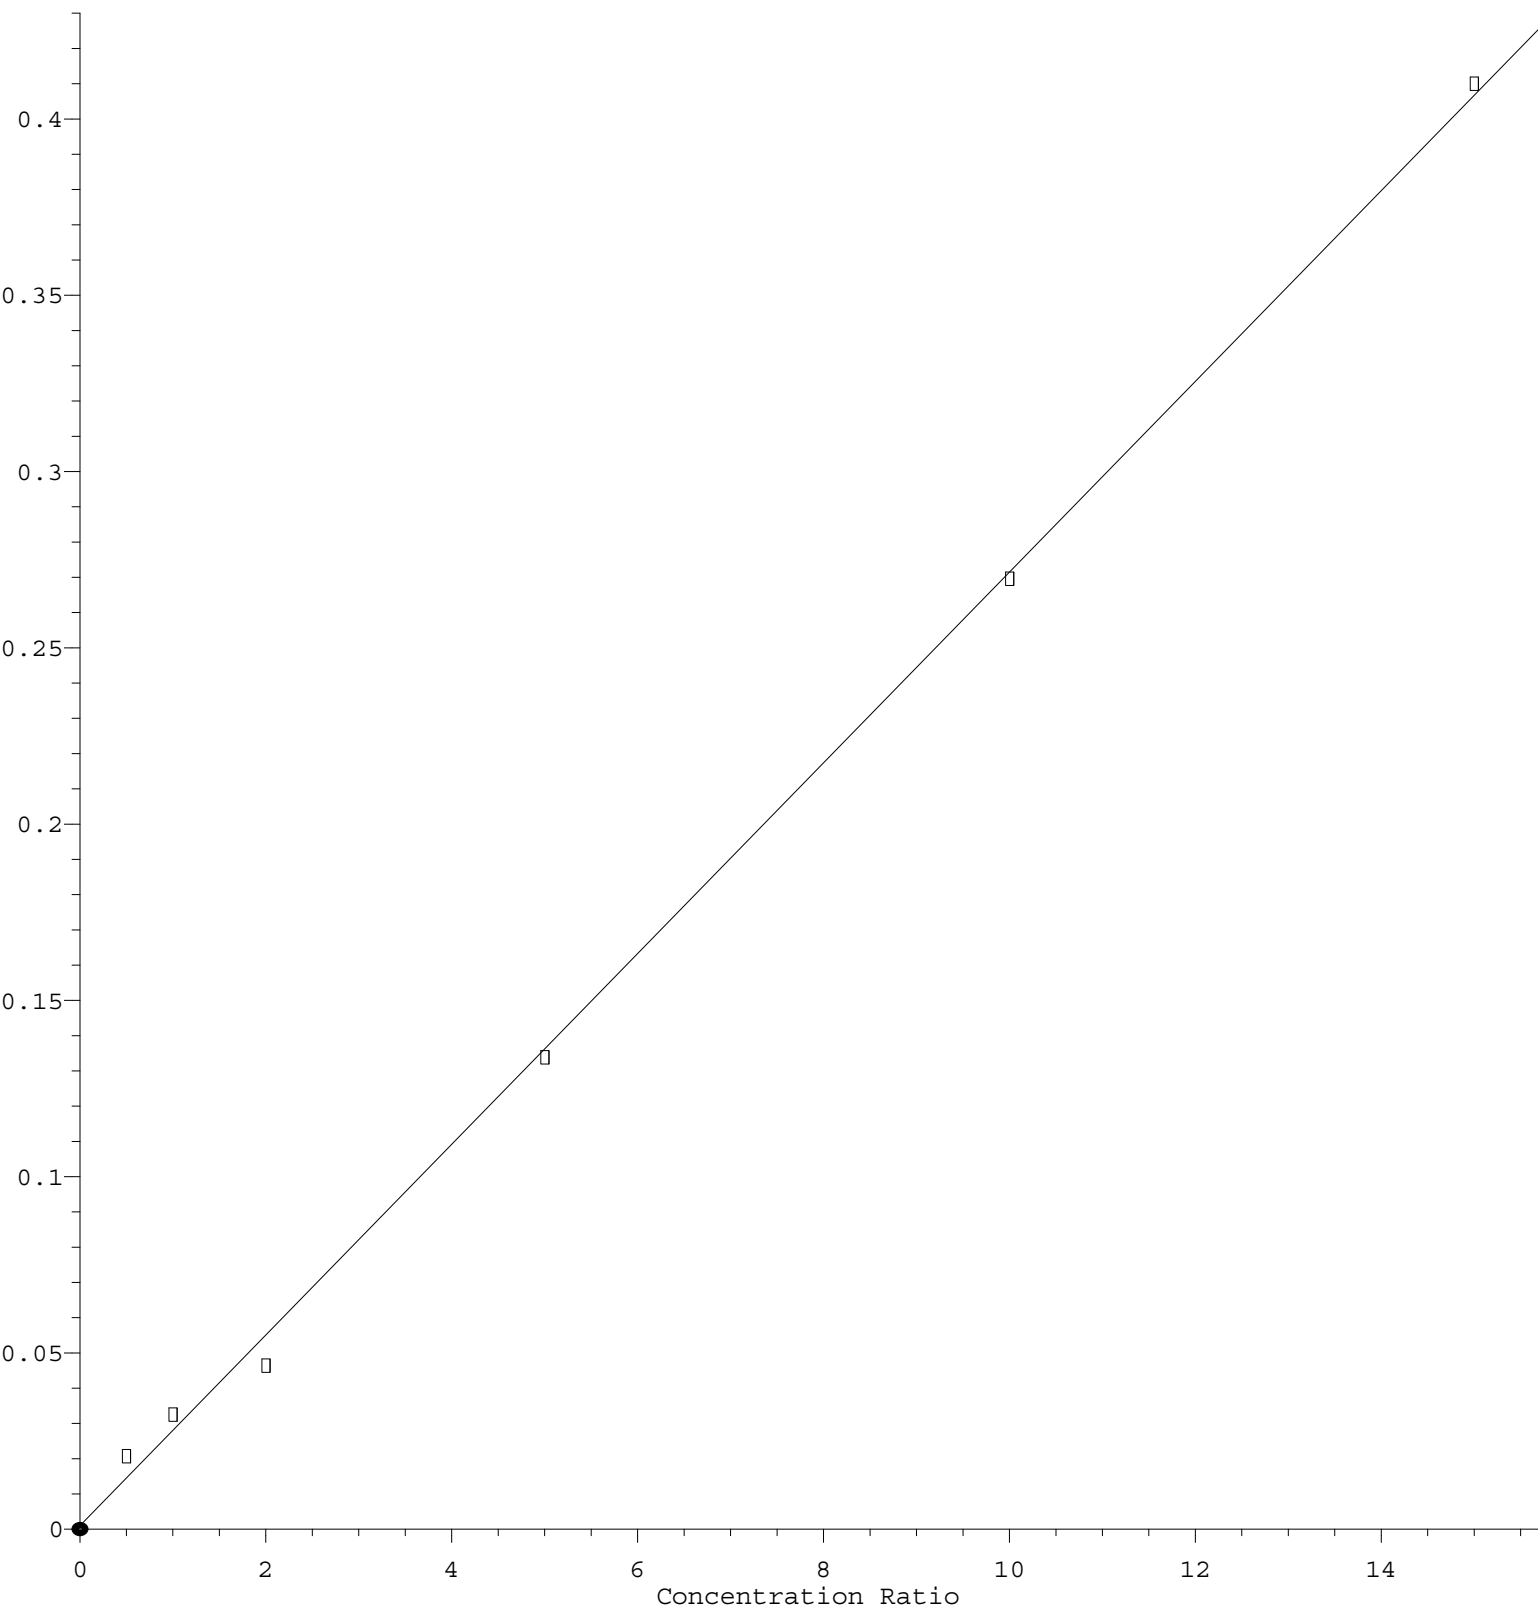

Response = 2.707e-002 * Amt + 1.041e-003
 Coef of Det (r^2) = 0.998755 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W051921S.M
 Calibration Table Last Updated: Thu May 20 03:59:48 2021