



Dichlorodifluoromethane

Response Ratio

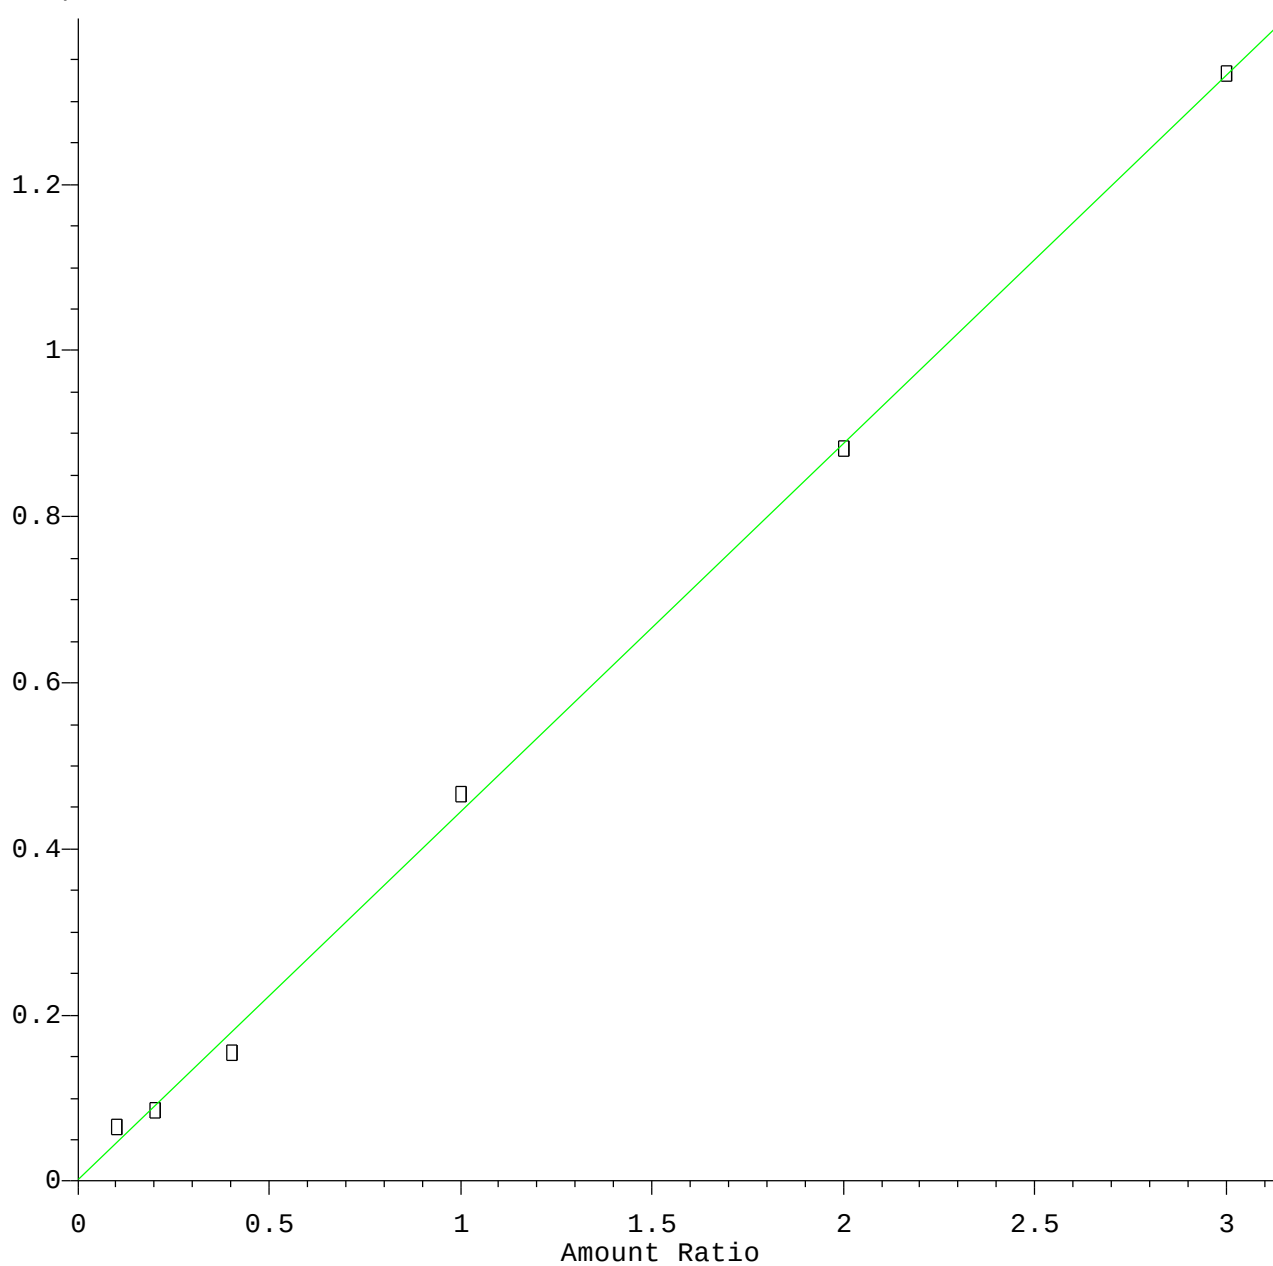

Resp Ratio = $4.43 \times 10^{-1} \times \text{Amt} + 2.49 \times 10^{-3}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
Calibration Table Last Updated: Tue May 21 06:38:43 2019

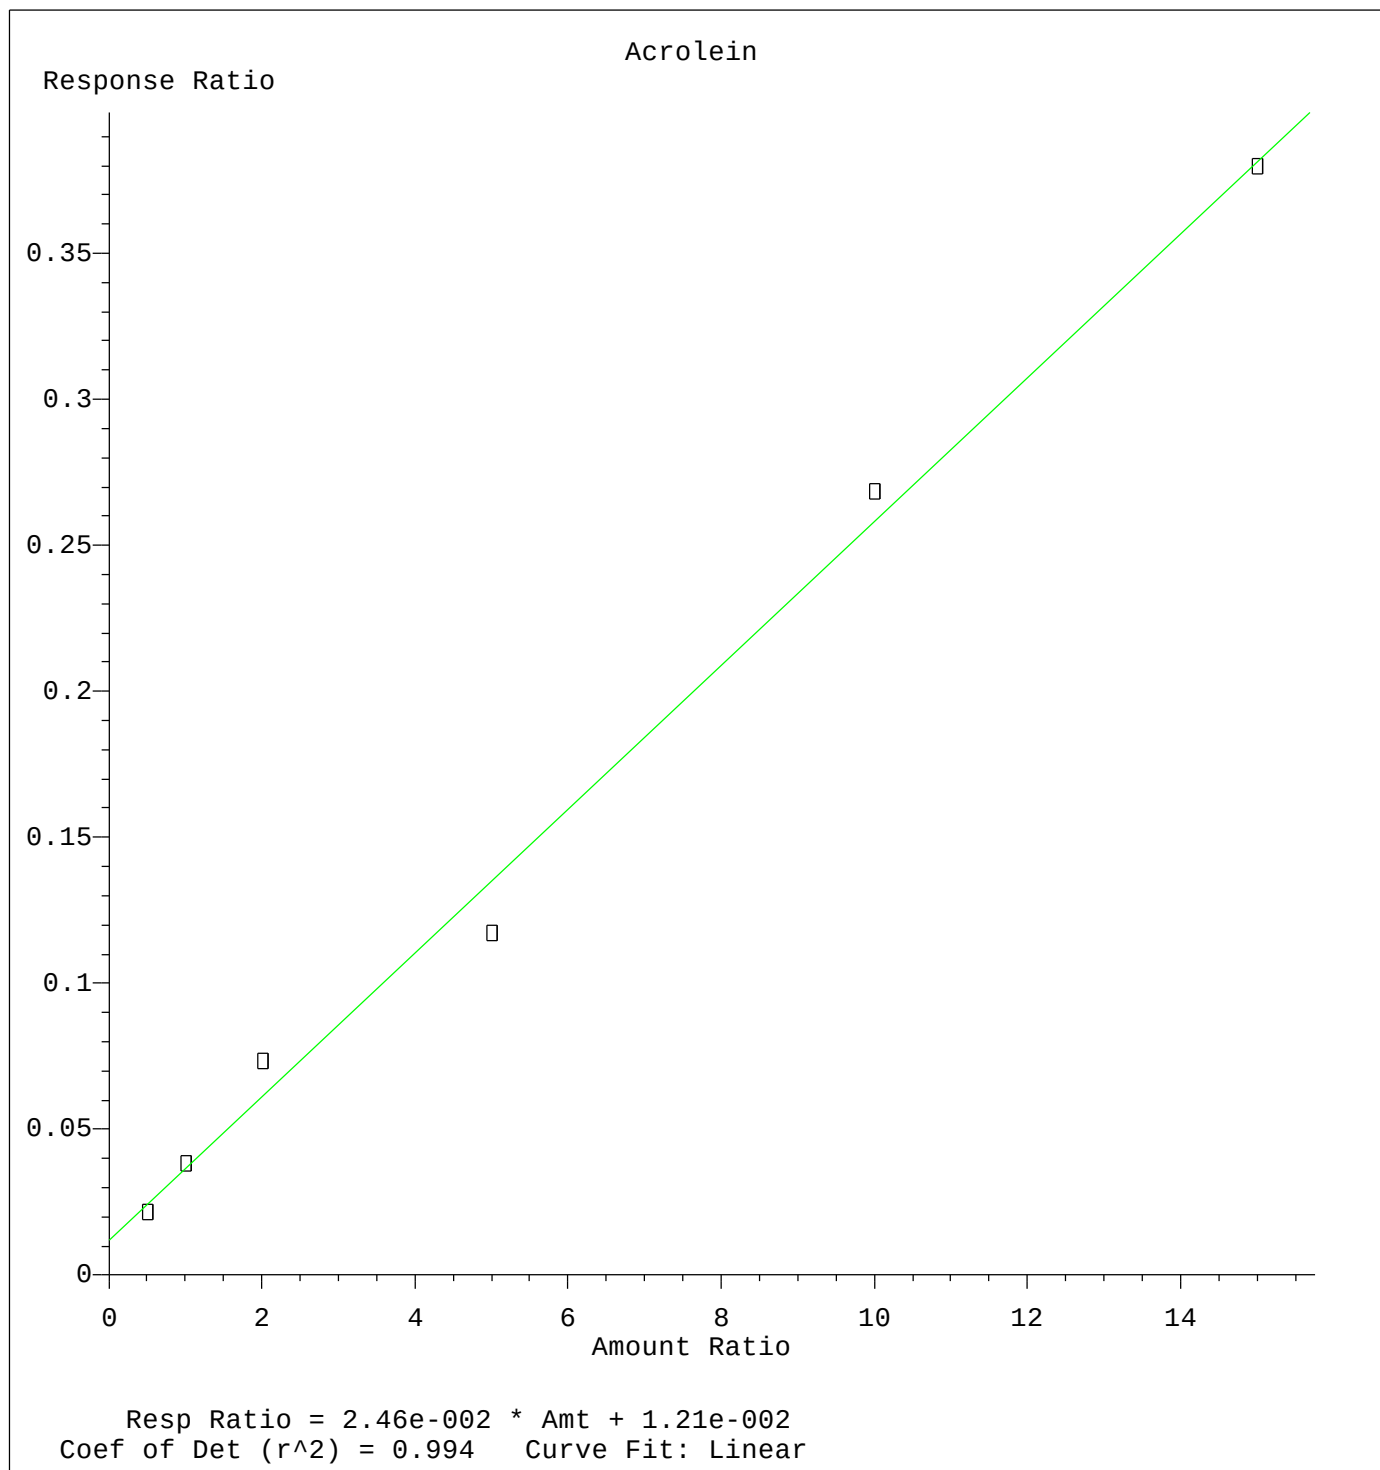

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
Calibration Table Last Updated: Tue May 21 06:38:43 2019

Methylene Chloride

Response Ratio

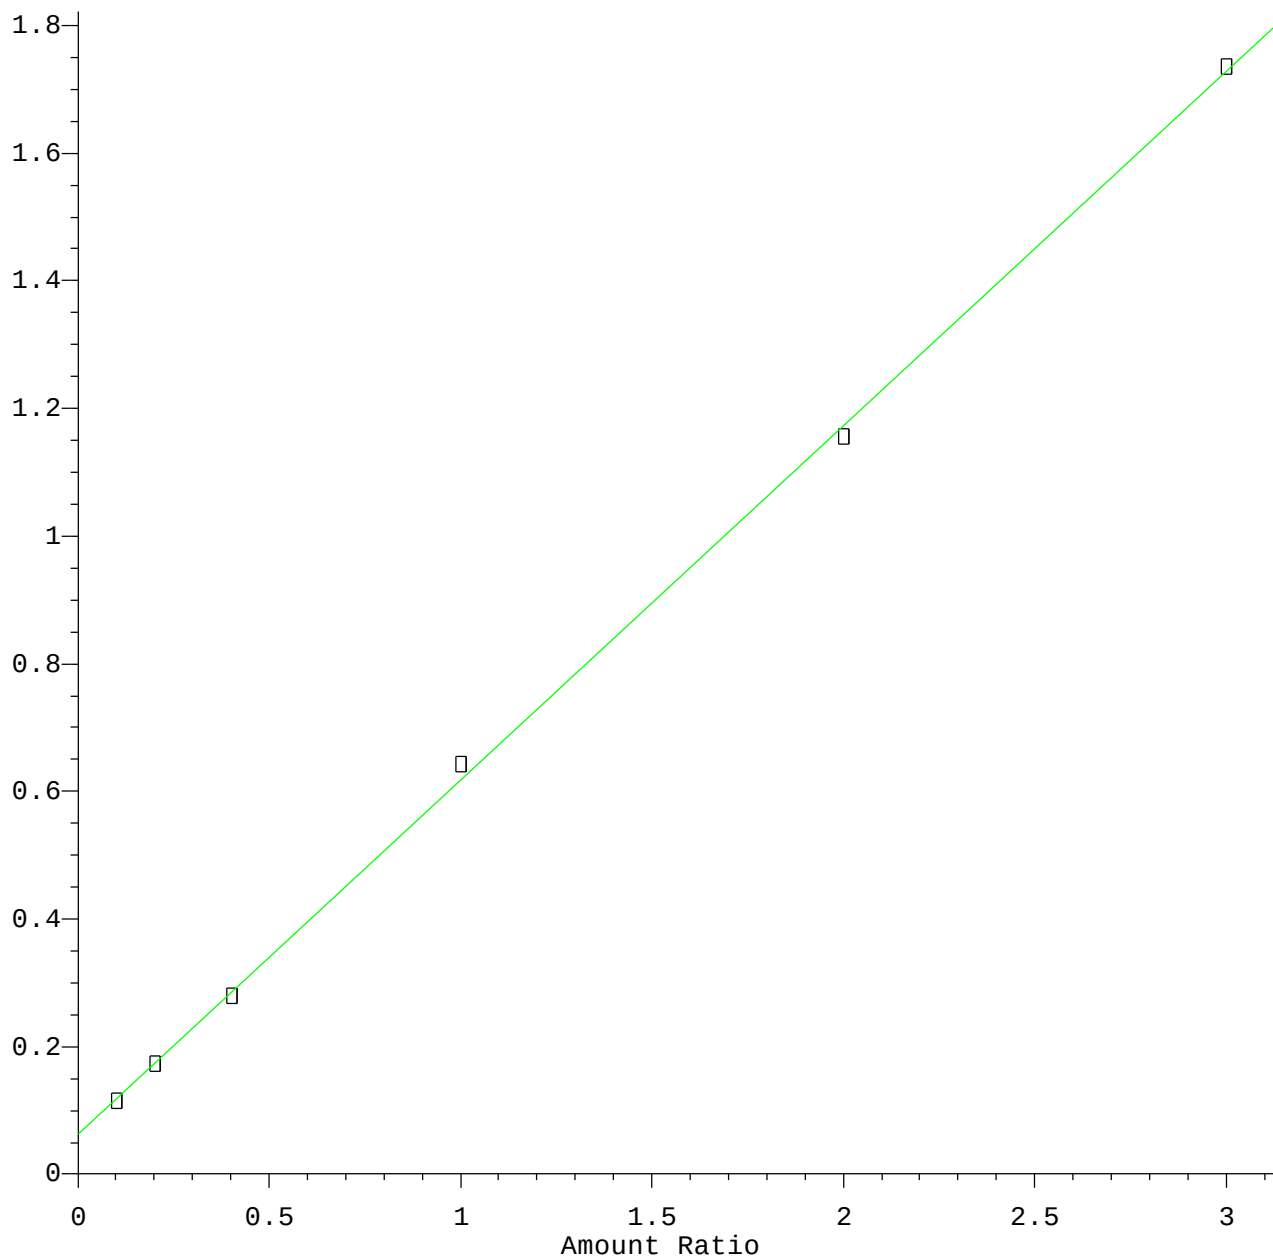

Resp Ratio = 5.55e-001 * Amt + 6.27e-002
Coef of Det (r²) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
Calibration Table Last Updated: Tue May 21 06:38:43 2019