

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW052119\
 Data File : VW010492.D
 Acq On : 21 May 2019 17:20
 Operator : SY/VA
 Sample : K2966-02
 Misc : 6.67G/5ML/MSVOA W/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 FESB-14(4.5-5)

Quant Time: May 22 07:29:45 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 21 06:38:43 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	102879	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	191945	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	168061	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	71267	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	62866	59.20	ug/l	0.00
Spiked Amount 50.000			Recovery	=	118.40%	
35) Dibromofluoromethane	7.88	113	61252	52.59	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.18%	
50) Toluene-d8	10.32	98	234256	52.65	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.30%	
62) 4-Bromofluorobenzene	12.62	95	85281	48.12	ug/l	0.00
Spiked Amount 50.000			Recovery	=	96.24%	
Target Compounds						
16) Acetone	4.13	43	7075	32.641	ug/l	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW052119\
Data File : VW010492.D
Acq On : 21 May 2019 17:20
Operator : SY/VA
Sample : K2966-02
Misc : 6.67G/5ML/MSVOA W/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
FESB-14(4.5-5)

Quant Time: May 22 07:29:45 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
Quant Title : SW846 8260
QLast Update : Tue May 21 06:38:43 2019
Response via : Initial Calibration

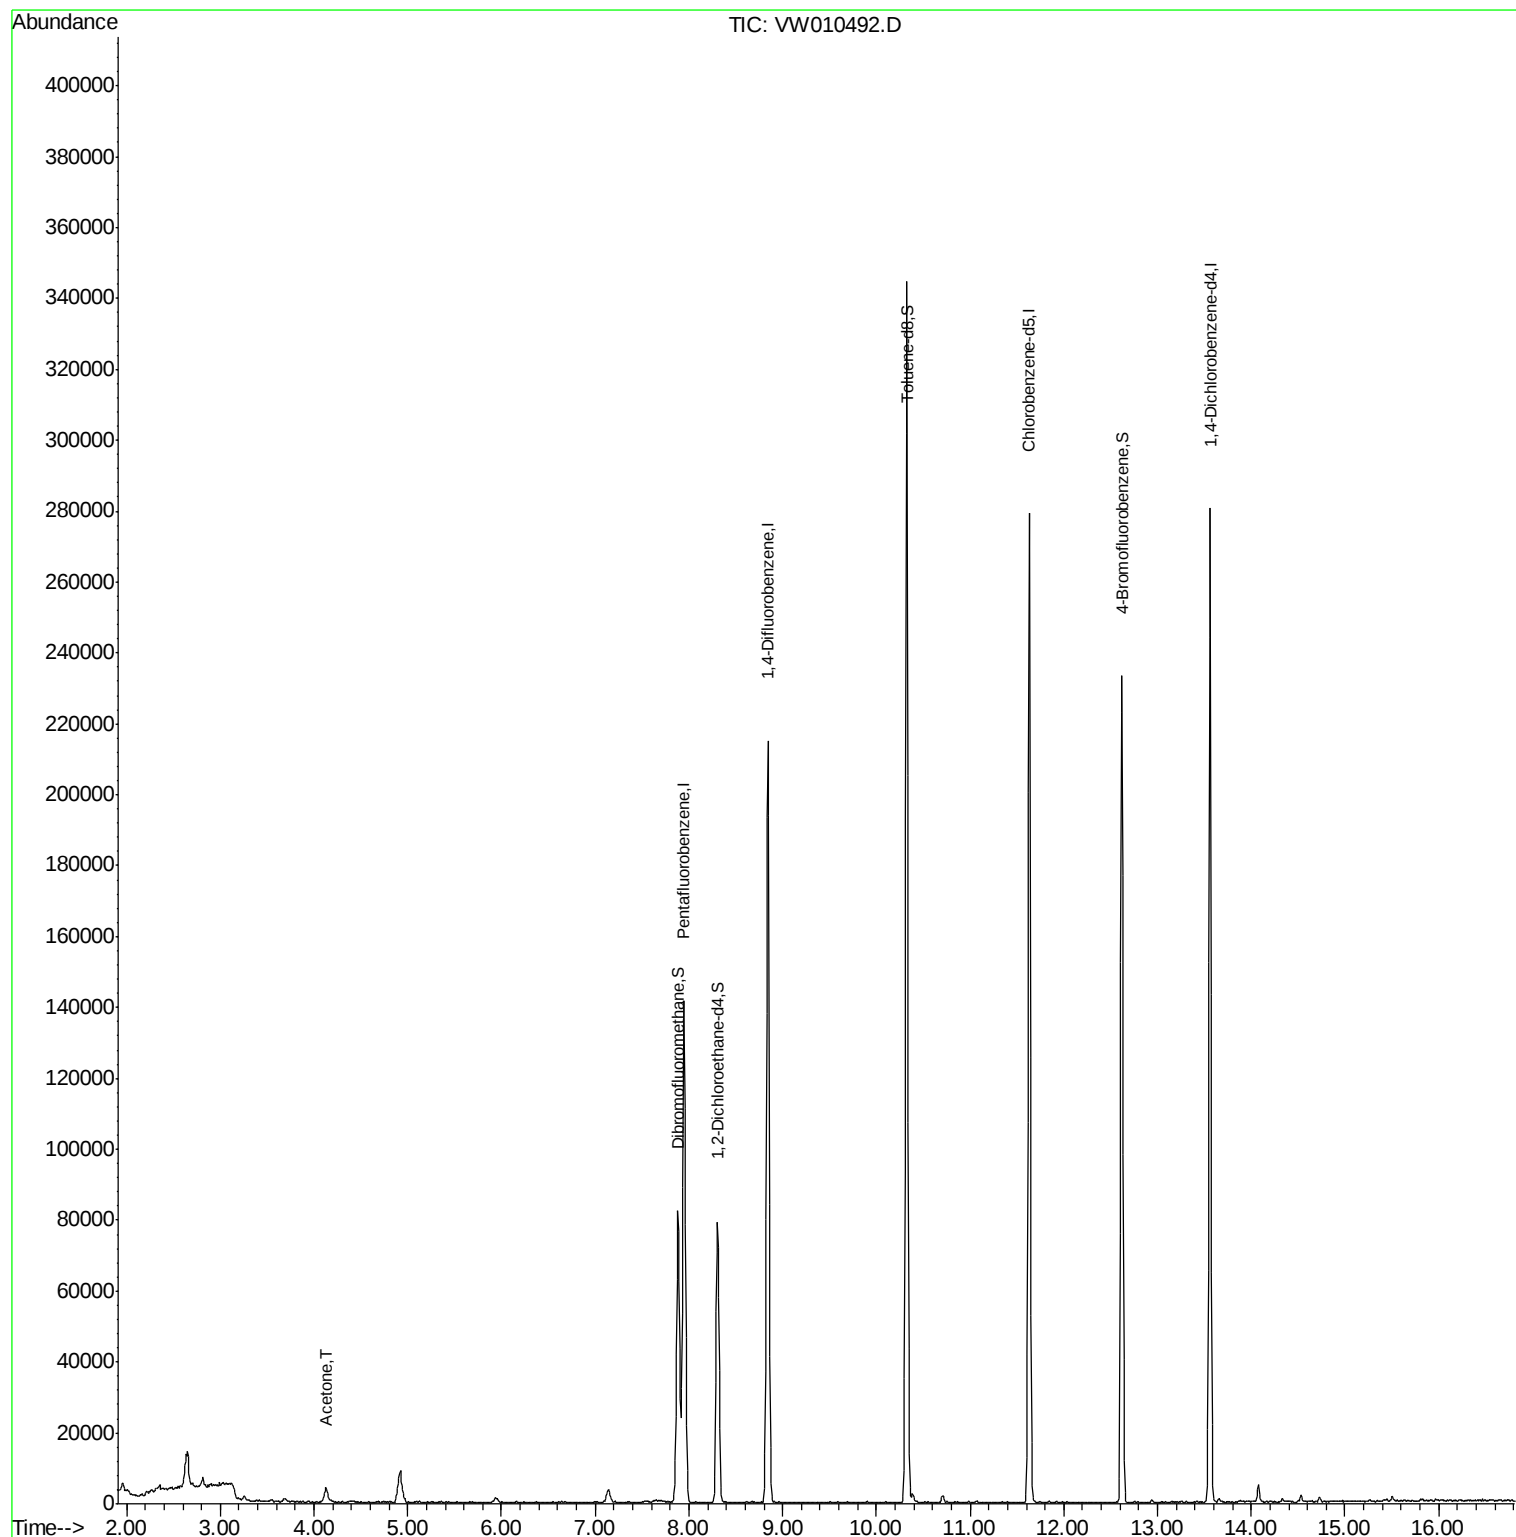

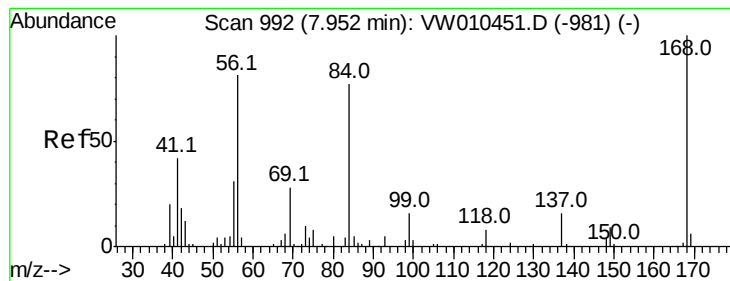

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW010492.D

Acq: 21 May 2019 17:20

Instrument :

MSVOA_W

ClientSampleId :


FESB-14(4.5-5)

Tot Ion:168 Resp: 102879

Ion Ratio Lower Upper

168 100

99 63.1 46.1 69.1

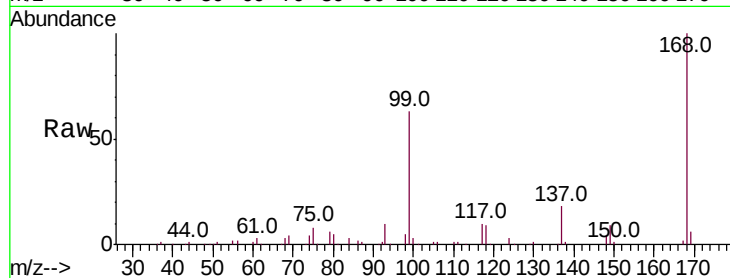

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

50000

40000

30000

20000



10000

0

7.90

8.00

Time-->

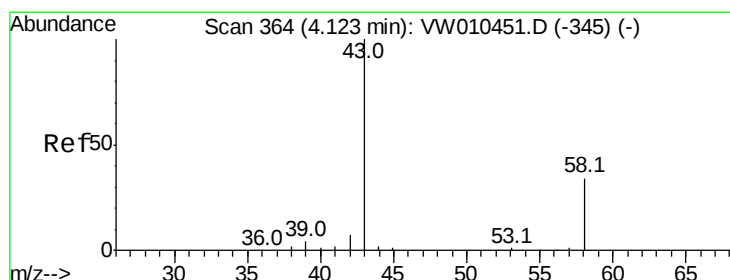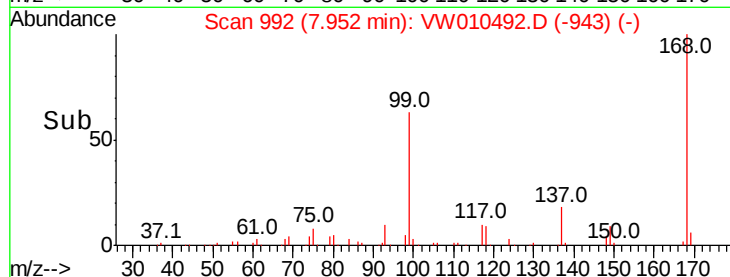

#16

Acetone

Concen: 32.641 ug/l

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW010492.D


Acq: 21 May 2019 17:20

Tgt Ion: 43 Resp: 7075

Ion Ratio Lower Upper

43 100

58 37.6 27.0 40.4

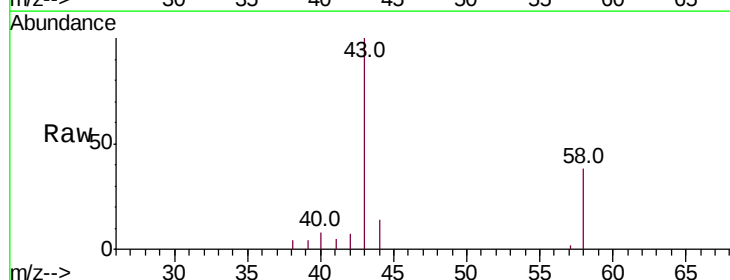

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.13

2500

2000

1500

1000

500


0


4.00

4.10

4.20

Time-->




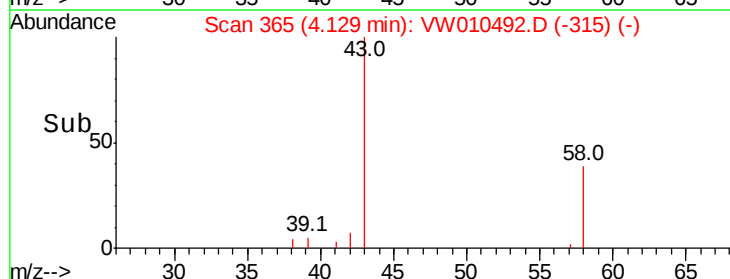


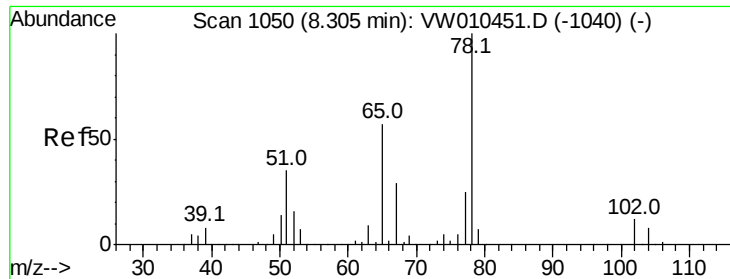

#33
 1,2-Dichloroethane-d4
 Concen: 59.202 ug/l
 RT: 8.31 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: VW010492.D
 Acq: 21 May 2019 17:20




Instrument :
 MSVOA_W
 ClientSampleId :
 FESB-14(4.5-5)


Tot Ion: 65 Resp: 62866
 Ion Ratio Lower Upper
 65 100
 67 52.2 0.0 103.6

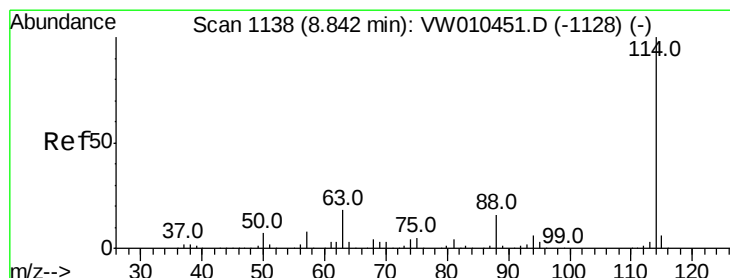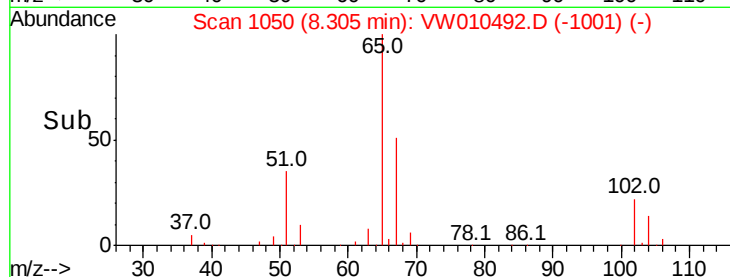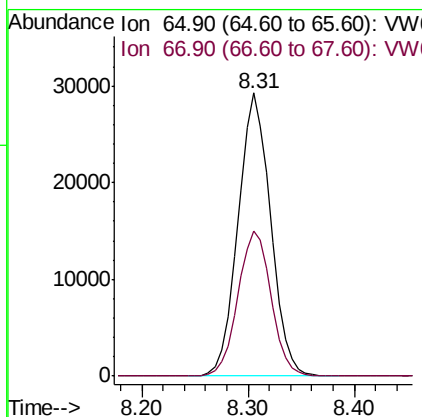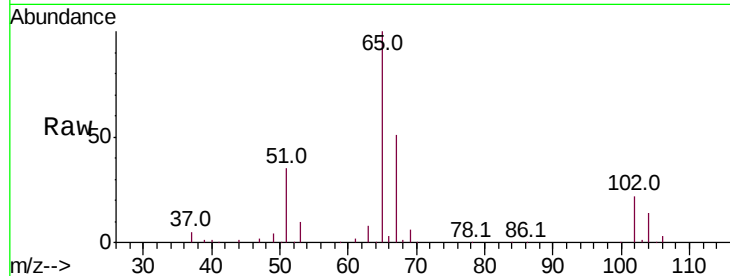

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW010492.D
 Acq: 21 May 2019 17:20

Tgt Ion: 114 Resp: 191945
 Ion Ratio Lower Upper
 114 100
 63 18.7 0.0 36.0
 88 16.4 0.0 32.0


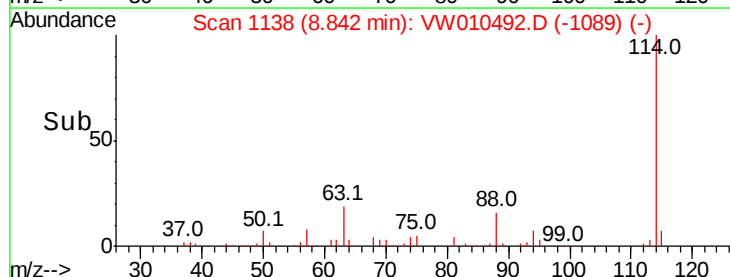
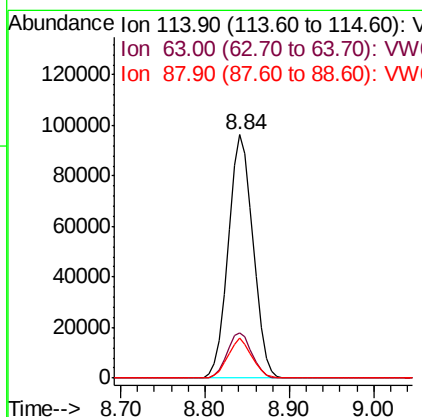
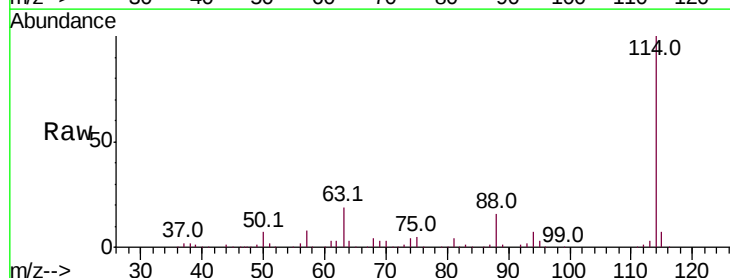


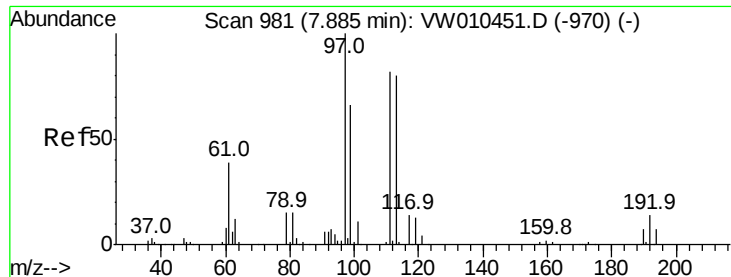

#35
 Dibromofluoromethane
 Concen: 52.591 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. 0.00 min
 Lab File: VW010492.D
 Acq: 21 May 2019 17:20




Instrument :
 MSVOA_W
 ClientSampleId :
 FESB-14(4.5-5)


Tot Ion:113 Resp: 61252
 Ion Ratio Lower Upper
 113 100
 111 102.0 82.2 123.4
 192 16.5 14.3 21.5

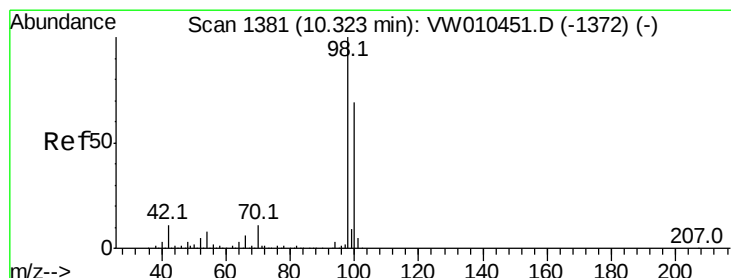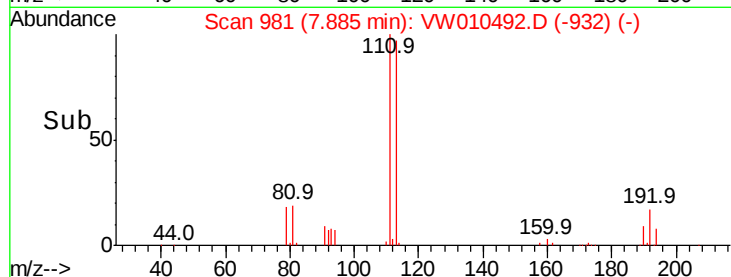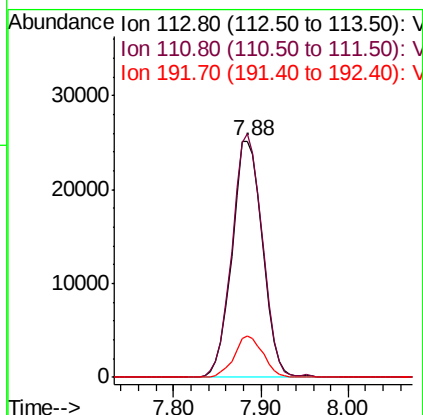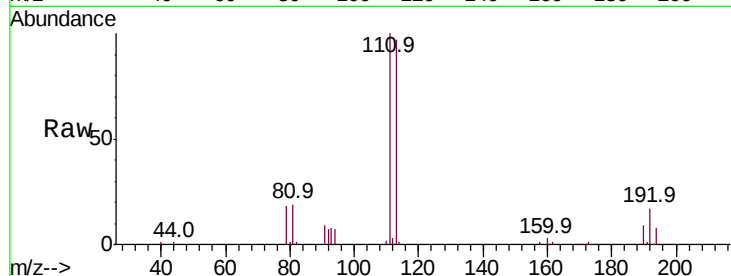

#50
 Toluene-d8
 Concen: 52.649 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. 0.00 min
 Lab File: VW010492.D
 Acq: 21 May 2019 17:20

Tgt Ion: 98 Resp: 234256
 Ion Ratio Lower Upper
 98 100
 100 67.5 53.7 80.5

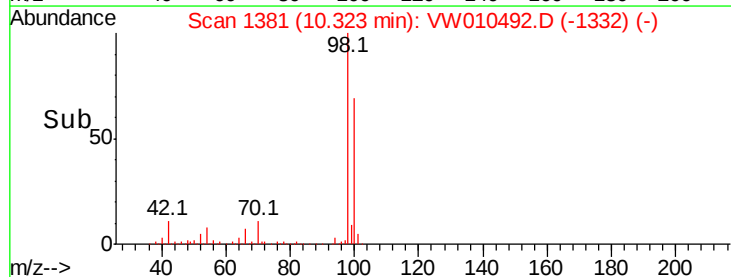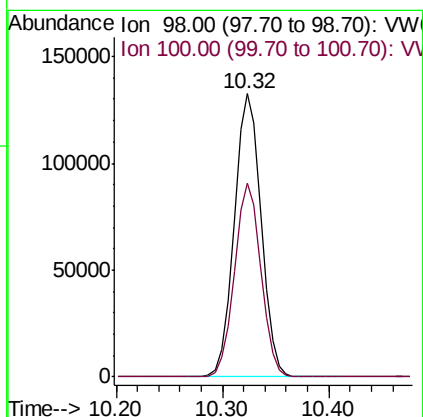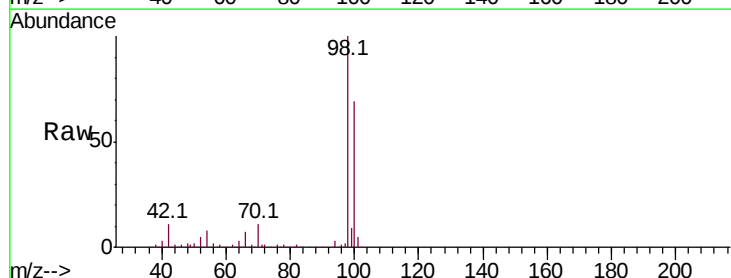

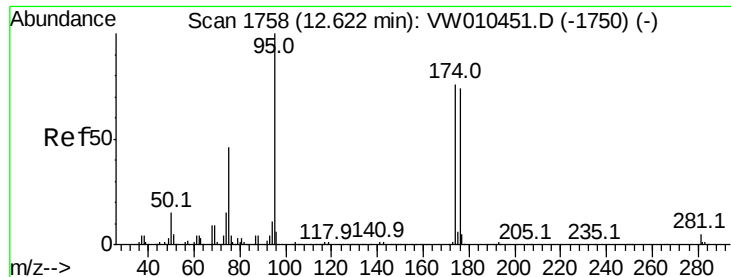

#62

4-Bromofluorobenzene

Concen: 48.120 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW010492.D

Acq: 21 May 2019 17:20

Instrument :

MSVOA_W

ClientSampleId :

FESB-14(4.5-5)


Tot Ion: 95 Resp: 85281

Ion Ratio Lower Upper

95 100

174 68.3 0.0 148.6




176 65.3 0.0 144.2

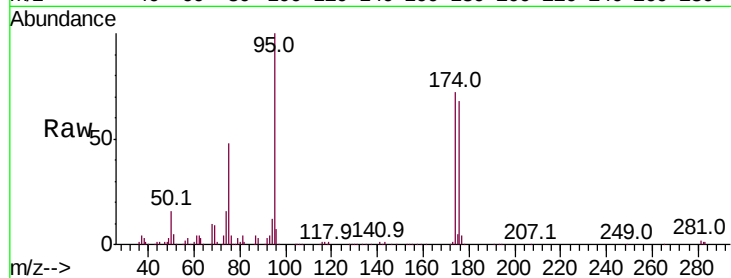

Abundance Ion 94.90 (94.60 to 95.60): VW

Ion 173.80 (173.50 to 174.50): VW

Ion 175.80 (175.50 to 176.50): VW

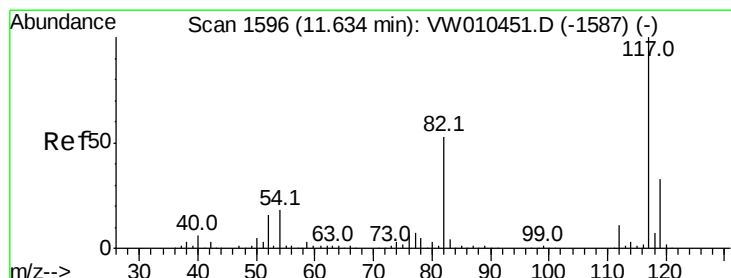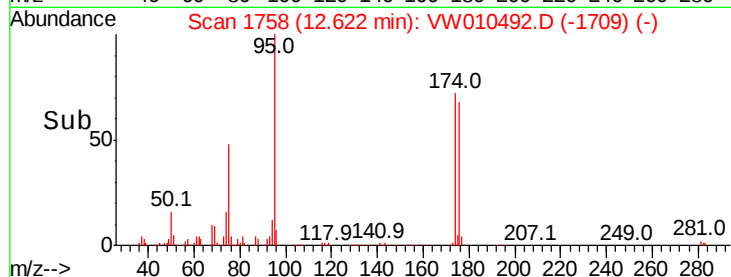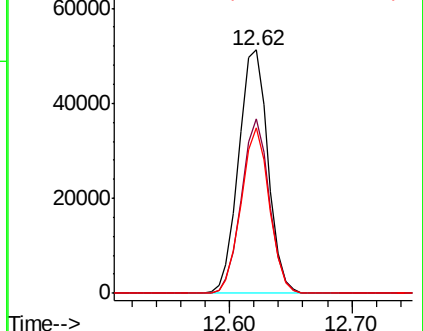

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.63 min Scan# 1596

Delta R.T. 0.00 min

Lab File: VW010492.D

Acq: 21 May 2019 17:20


Tgt Ion: 117 Resp: 168061

Ion Ratio Lower Upper

117 100

82 54.1 42.8 64.2



119 31.5 26.3 39.5

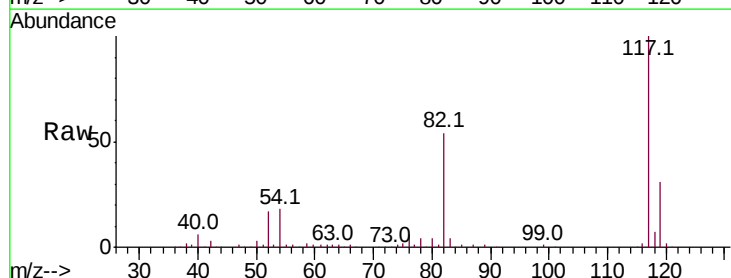


Abundance Ion 116.90 (116.60 to 117.60): VW

Ion 82.00 (81.70 to 82.70): VW

Ion 118.90 (118.60 to 119.60): VW

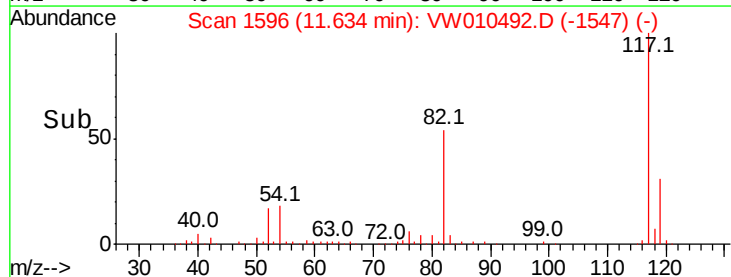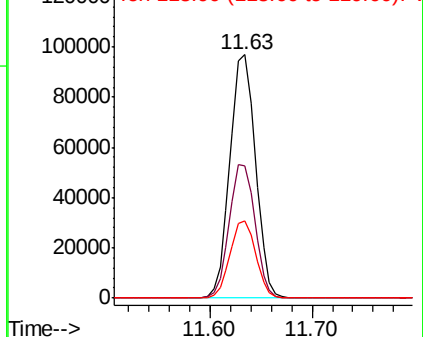

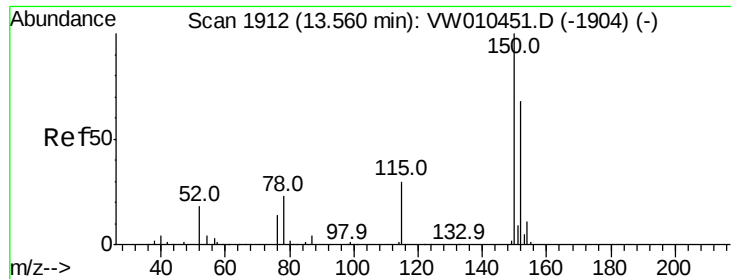

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. 0.00 min

Lab File: VW010492.D

Acq: 21 May 2019 17:20

Instrument :

MSVOA_W

ClientSampleId :

FESB-14(4.5-5)


Tot Ion:152 Resp: 71267

Ion Ratio Lower Upper

152 100

115 65.5 30.3 91.0

150 158.8 0.0 349.8

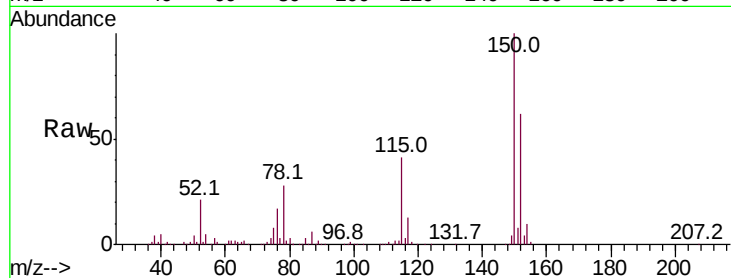

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

