
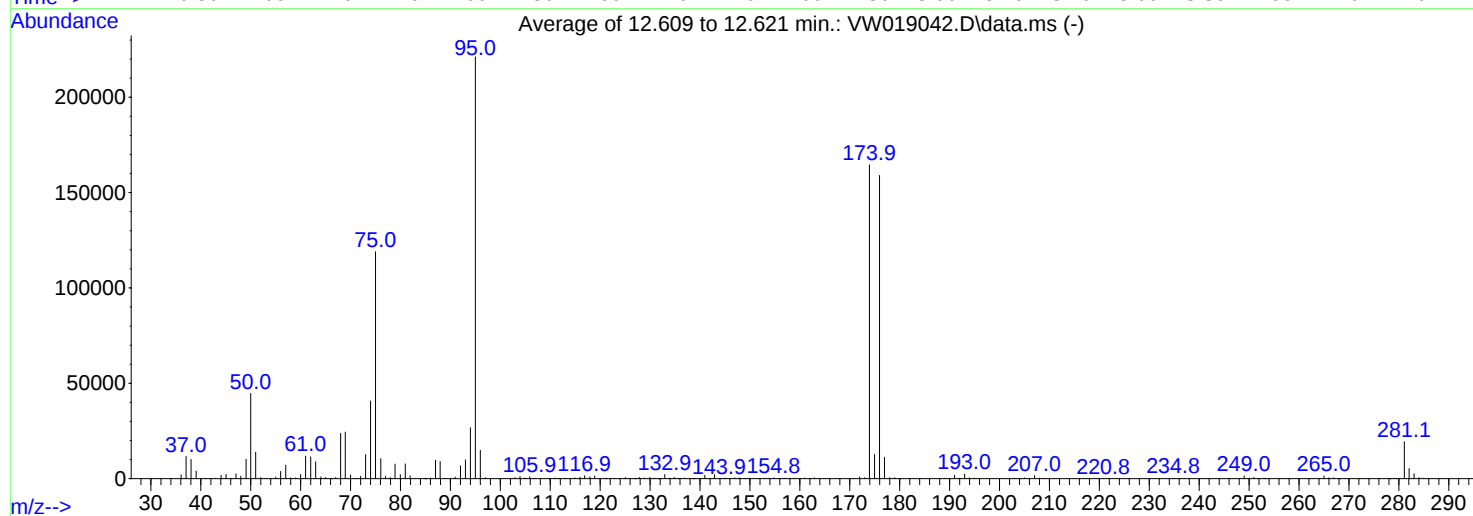


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052121\
Data File : VW019042.D
Acq On : 20 May 2021 10:07
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W051921S.M
Title : SW846 8260
Last Update : Thu May 20 03:59:48 2021

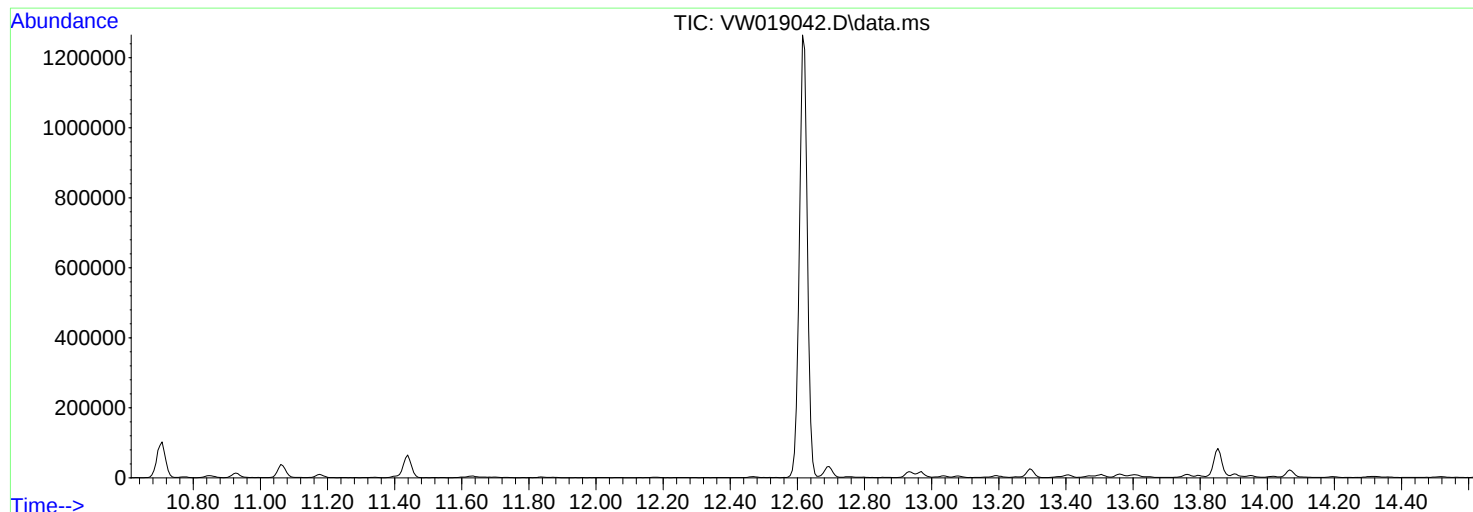

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	44605	PASS
75	95	30	60	53.8	118955	PASS
95	95	100	100	100.0	221184	PASS
96	95	5	9	6.7	14857	PASS
173	174	0.00	2	0.3	493	PASS
174	95	50	100	74.4	164565	PASS
175	174	5	9	7.7	12683	PASS
176	174	95	101	96.6	159029	PASS
177	176	5	9	7.0	11180	PASS