
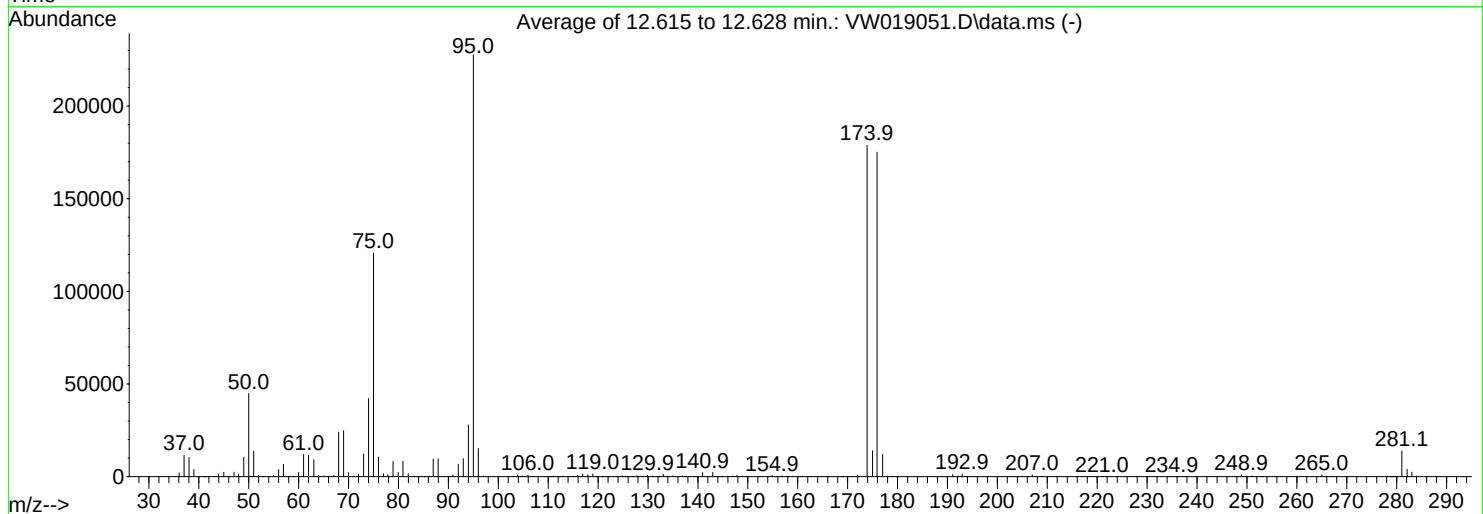


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052221\
 Data File : VW019051.D
 Acq On : 21 May 2021 09:28
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W051921S.M
 Title : SW846 8260
 Last Update : Thu May 20 03:59:48 2021

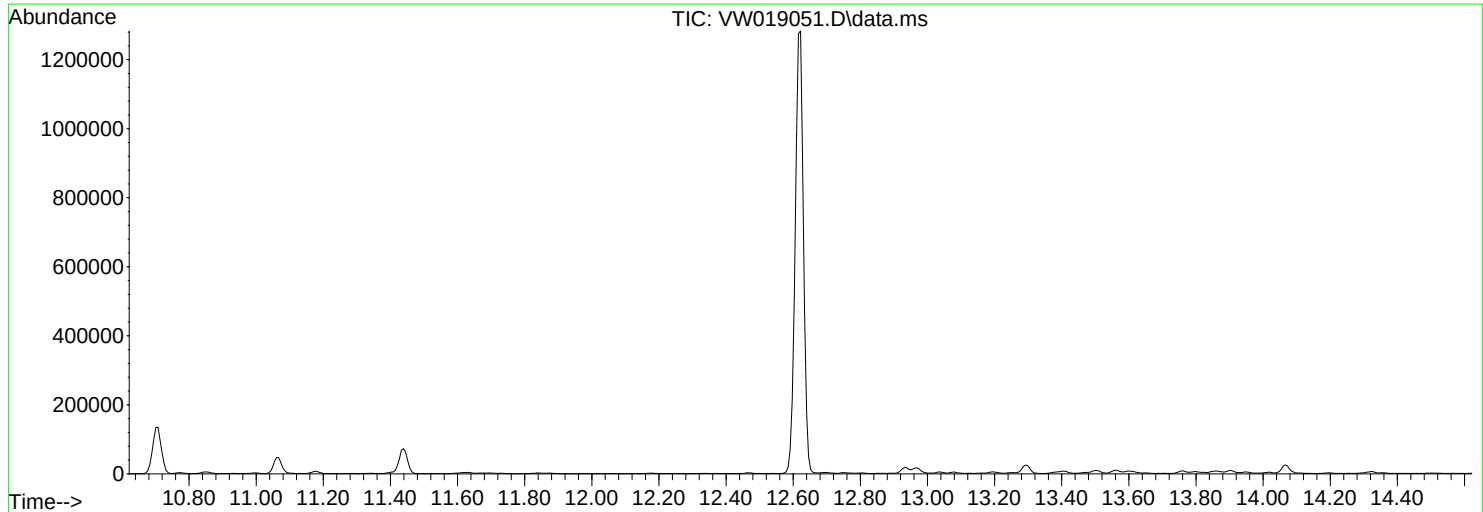

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	44880	PASS
75	95	30	60	53.0	120656	PASS
95	95	100	100	100.0	227669	PASS
96	95	5	9	6.7	15236	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	78.6	178837	PASS
175	174	5	9	7.8	13964	PASS
176	174	95	101	98.0	175189	PASS
177	176	5	9	6.8	11971	PASS