


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052223\
 Data File : VW026020.D
 Acq On : 22 May 2023 10:54
 Operator : SY/MD
 Sample : 02851-10RE
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0FK3RE

Manual IntegrationsAPPROVED

Quant Time: May 23 02:17:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 23 01:22:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/23/2023
 Supervised By :Mahesh Dadoda 05/25/2023

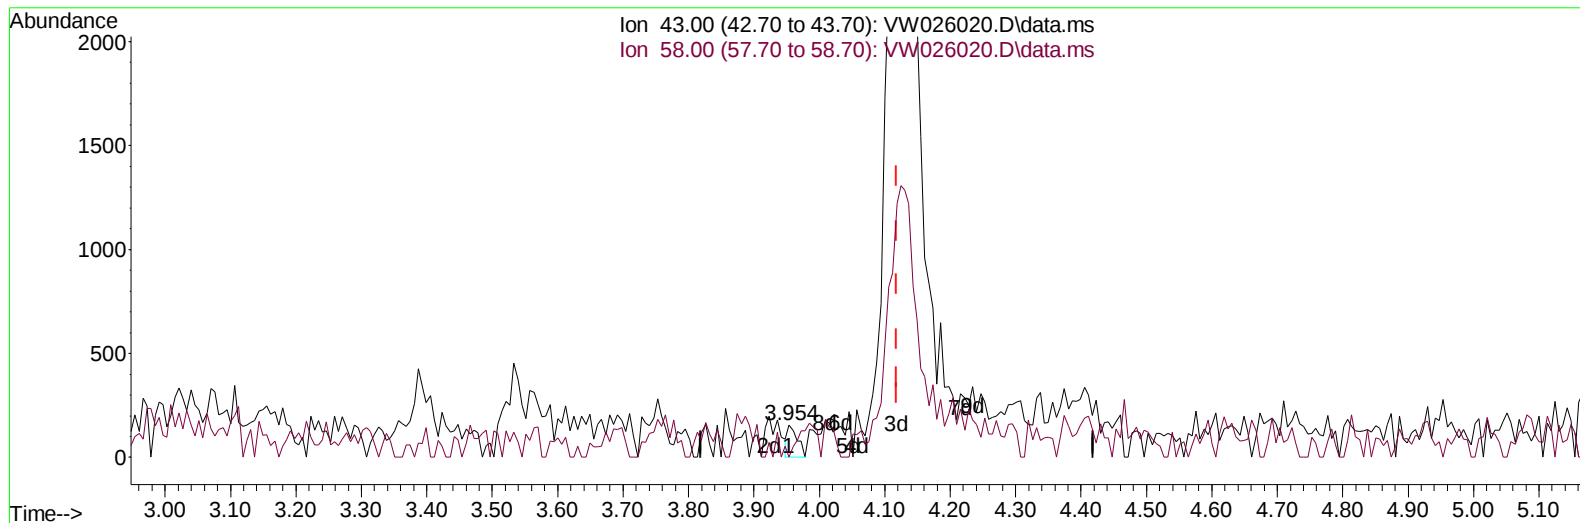




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052223\
 Data File : VW026020.D
 Acq On : 22 May 2023 10:54
 Operator : SY/MD
 Sample : 02851-10RE
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0FK3RE

Manual IntegrationsAPPROVED

Quant Time: May 23 02:17:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 23 01:22:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/23/2023
 Supervised By :Mahesh Dadoda 05/25/2023

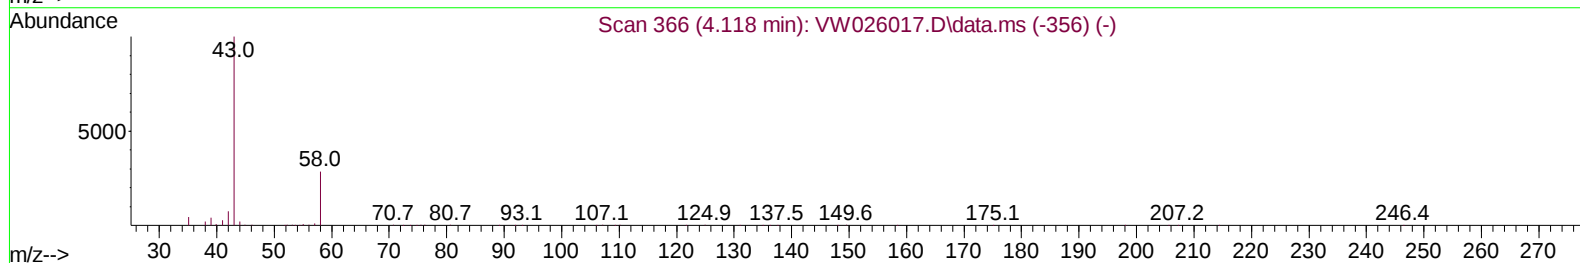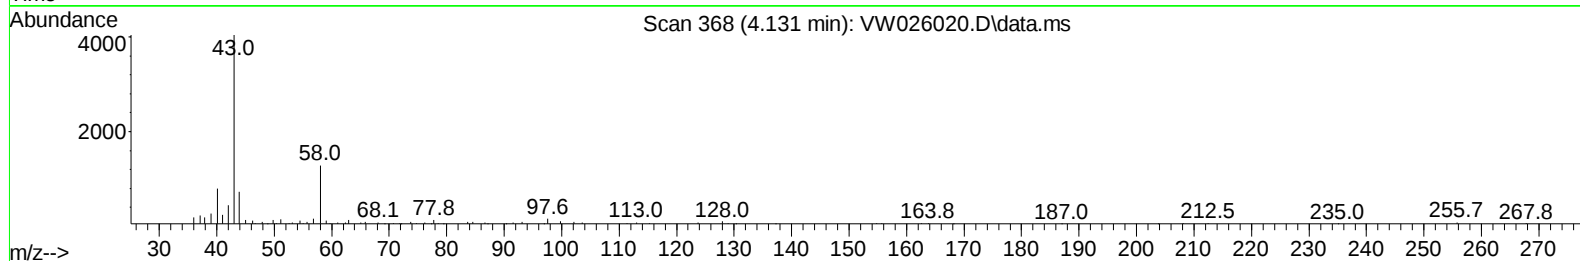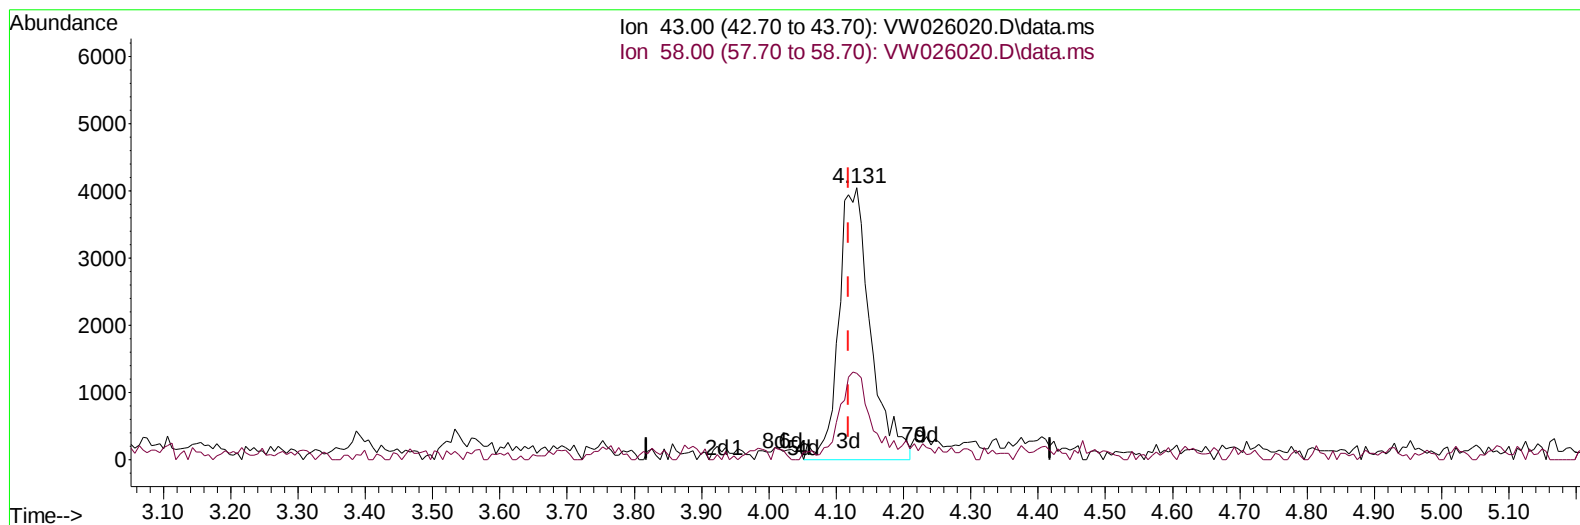

TIC: VW026020.D\data.ms

(13) Acetone (T)

4.131min (+ 0.012) 10.65 ug/L m

response 13291

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	29.10	0.33
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052223\
 Data File : VW026020.D
 Acq On : 22 May 2023 10:54
 Operator : SY/MD
 Sample : 02851-10RE
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0FK3RE

Manual IntegrationsAPPROVED

Quant Time: May 23 02:17:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 23 01:22:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/23/2023
 Supervised By :Mahesh Dadoda 05/25/2023

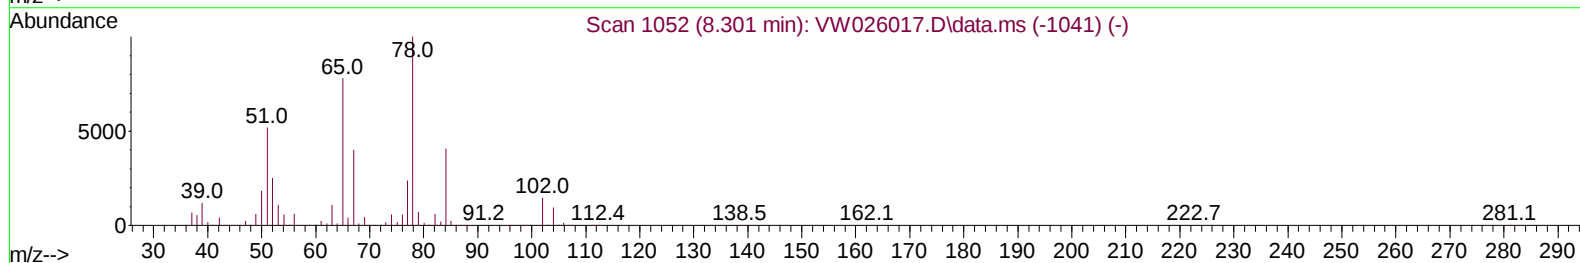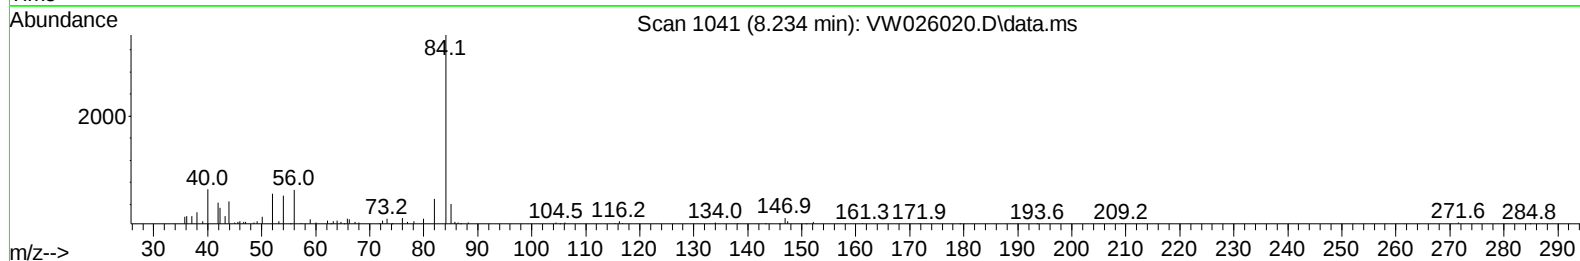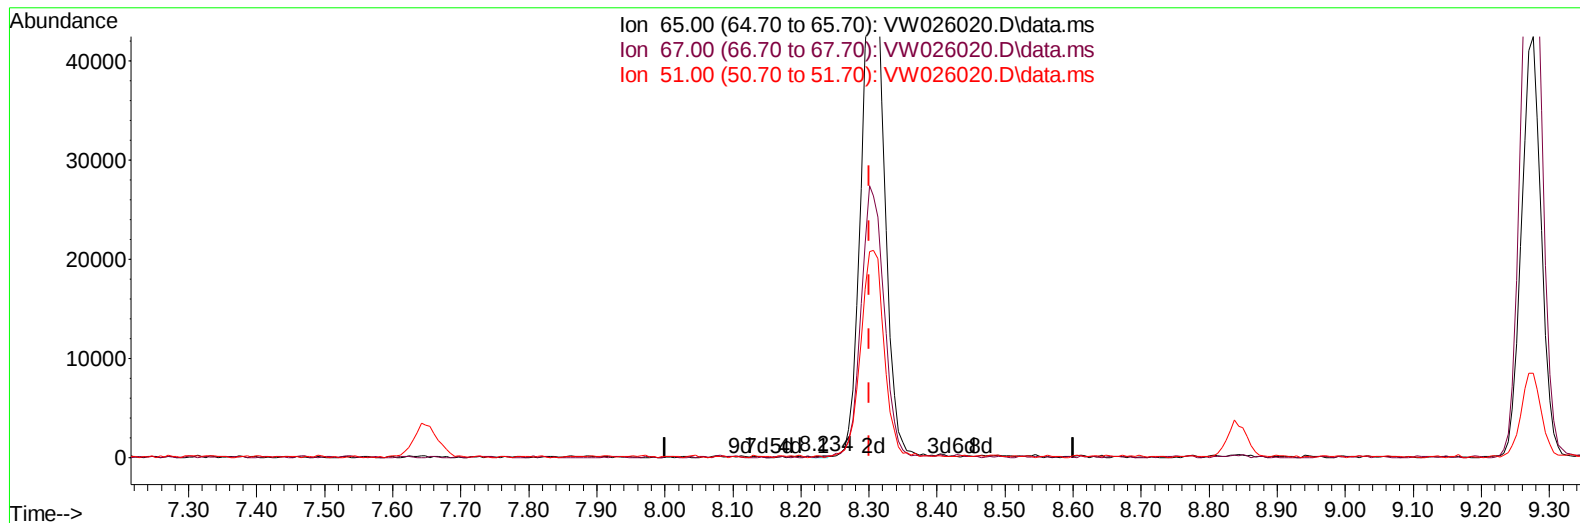

TIC: VW026020.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.234min (-0.067) 0.03 ug/L

response 153

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	52.29
51.00	112.30	94.77
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052223\
 Data File : VW026020.D
 Acq On : 22 May 2023 10:54
 Operator : SY/MD
 Sample : 02851-10RE
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0FK3RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/23/2023
 Supervised By :Mahesh Dadoda 05/25/2023

Quant Time: May 23 02:17:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 23 01:22:37 2023
 Response via : Initial Calibration

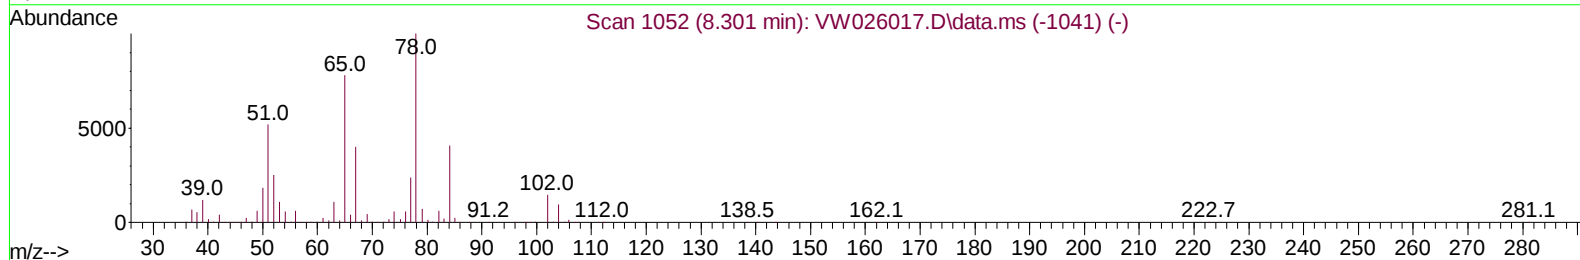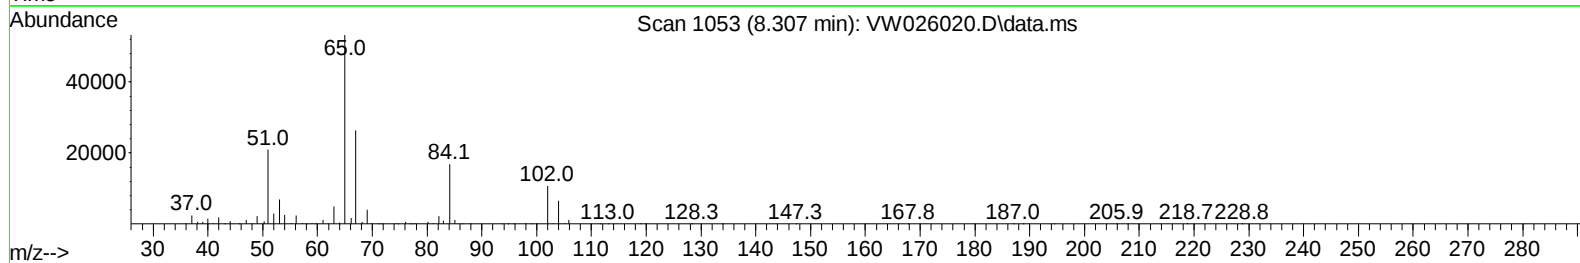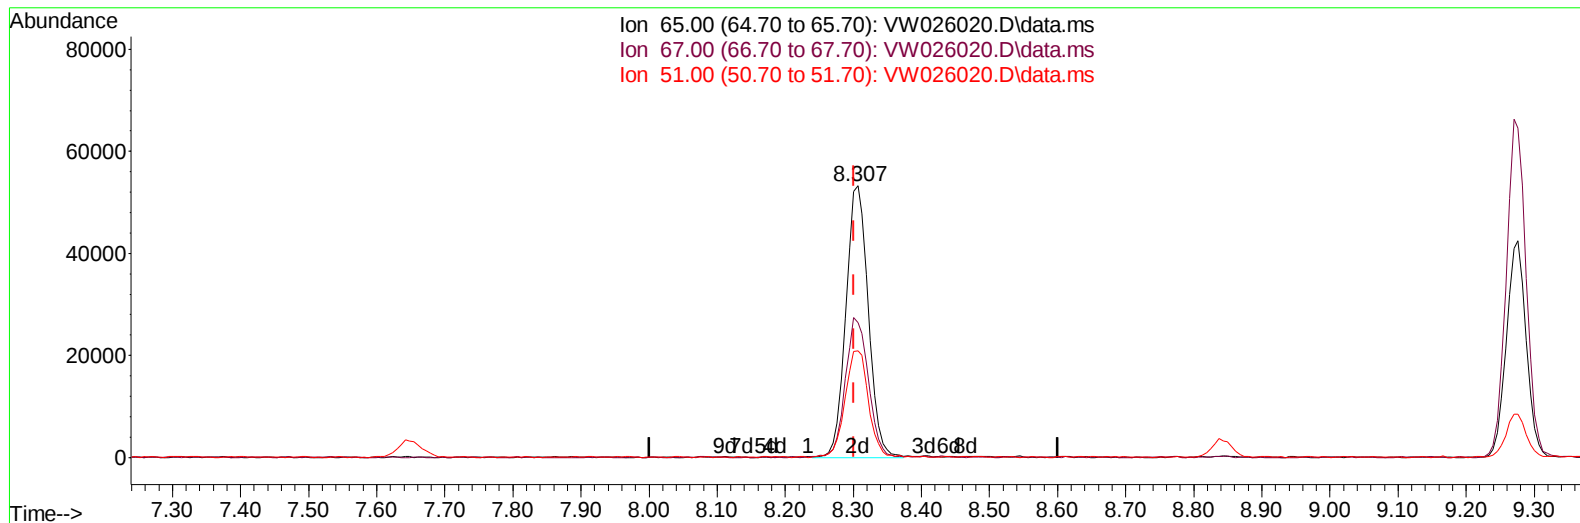

TIC: VW026020.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 24.73 ug/L m

response 121155

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.90	0.07#
51.00	112.30	0.12#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052223\
 Data File : VW026020.D
 Acq On : 22 May 2023 10:54
 Operator : SY/MD
 Sample : 02851-10RE
 Misc : 5.78g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 H0FK3RE

Manual IntegrationsAPPROVED

Quant Time: May 23 02:17:50 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue May 23 01:22:37 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/23/2023
 Supervised By :Mahesh Dadoda 05/25/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	300514	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	274930	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	108408	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	80408	18.882	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	75.520%	
7) Chloroethane-d5	2.899	69	71918	22.780	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	91.120%	
11) 1,1-Dichloroethene-d2	4.015	65	41782	19.594	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	78.360%	
21) 2-Butanone-d5	7.075	46	71309	50.653	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	101.300%	
24) Chloroform-d	7.648	84	199030	22.968	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.880%	
26) 1,2-Dichloroethane-d4	8.307	65	121155m	24.725	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	98.920%	
32) Benzene-d6	8.276	84	375216	20.887	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	83.560%	
36) 1,2-Dichloropropane-d6	9.270	67	133808	23.280	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	93.120%	
41) Toluene-d8	10.325	98	304806	19.027	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	76.120%	
43) trans-1,3-Dichloroprop...	10.575	79	45927	19.712	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	78.840%	
47) 2-Hexanone-d5	10.922	63	43290	44.168	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	88.340%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	115299	26.318	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	105.280%	
66) 1,2-Dichlorobenzene-d4	13.848	152	92734	23.466	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.880%	
Target Compounds						
13) Acetone	4.131	43	13291m	10.647	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052223\
Data File : VW026020.D
Acq On : 22 May 2023 10:54
Operator : SY/MD
Sample : 02851-10RE
Misc : 5.78g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
H0FK3RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/23/2023
Supervised By :Mahesh Dadoda 05/25/2023

Quant Time: May 23 02:17:50 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050123SMA.M
Quant Title : SFAM01.0
QLast Update : Tue May 23 01:22:37 2023
Response via : Initial Calibration

