

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW052419\
 Data File : VW010544.D
 Acq On : 24 May 2019 11:24
 Operator : SY/VA
 Sample : VW0524SBL01
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0524SBL01

Quant Time: May 25 01:43:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 21 06:38:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	132914	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	231260	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	199883	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	87102	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	66802	48.69	ug/l	0.00
Spiked Amount	50.000		Recovery	=	97.38%	
35) Dibromofluoromethane	7.88	113	68785	49.02	ug/l	0.00
Spiked Amount	50.000		Recovery	=	98.04%	
50) Toluene-d8	10.32	98	278244	51.90	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.80%	
62) 4-Bromofluorobenzene	12.62	95	99888	46.78	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.56%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW052419\
Data File : VW010544.D
Acq On : 24 May 2019 11:24
Operator : SY/VA
Sample : VW0524SBL01
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0524SBL01

Quant Time: May 25 01:43:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
Quant Title : SW846 8260
QLast Update : Tue May 21 06:38:43 2019
Response via : Initial Calibration

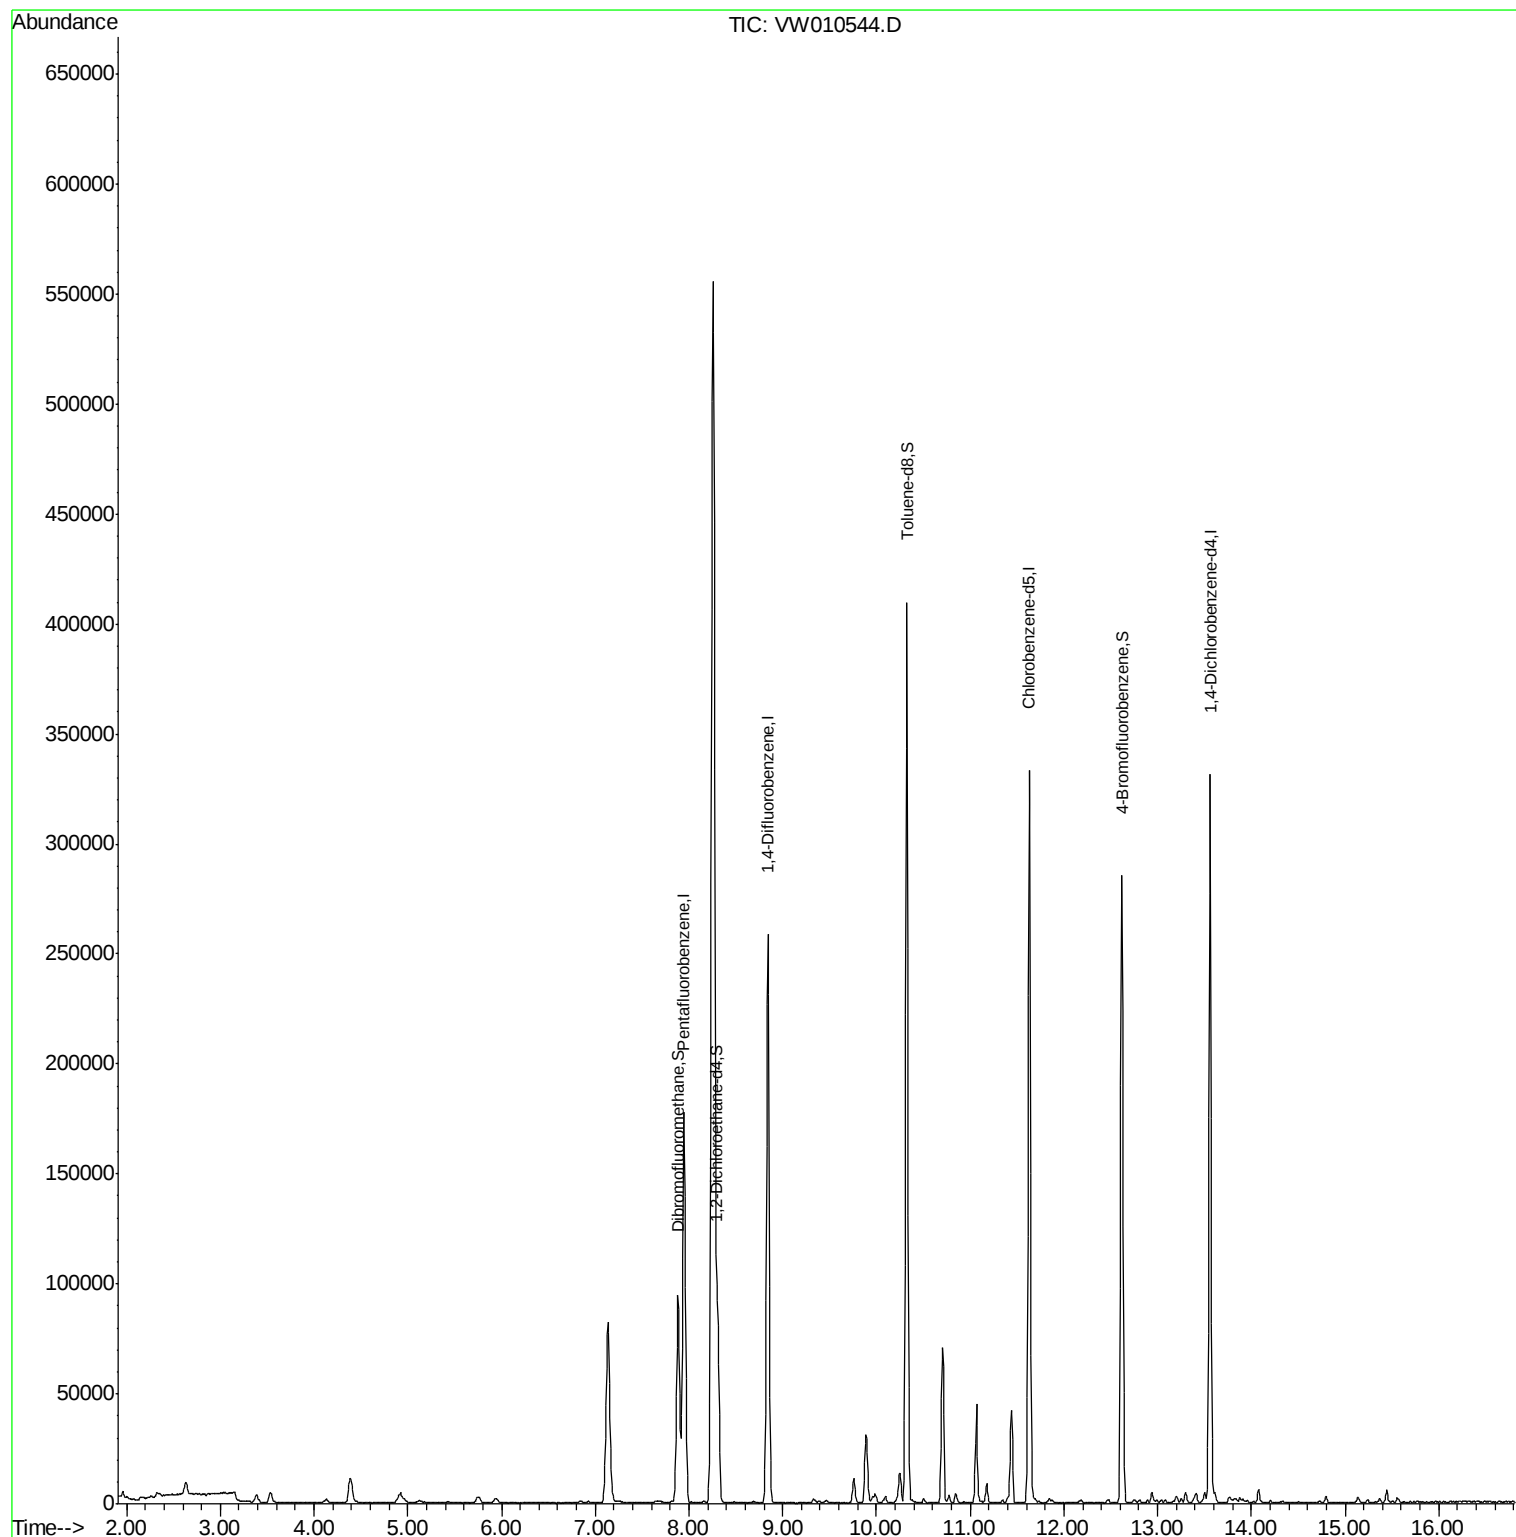

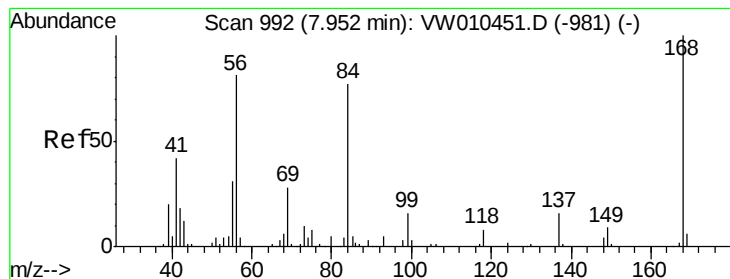

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.01 min

Lab File: VW010544.D

Acq: 24 May 2019 11:24

Instrument :

MSVOA_W

ClientSampleId :


VW0524SBL01

Tot Ion:168 Resp: 132914

Ion Ratio Lower Upper




168 100

99 63.7 46.1 69.1

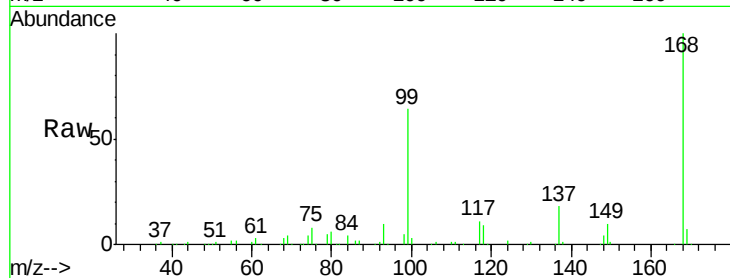

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

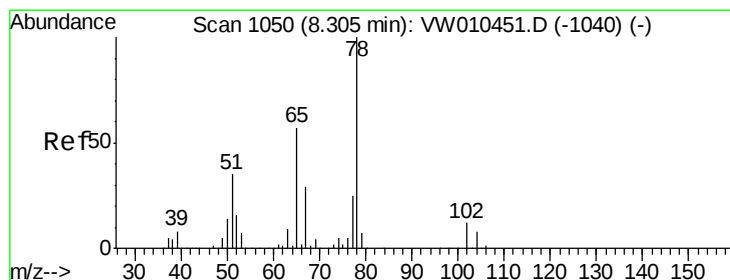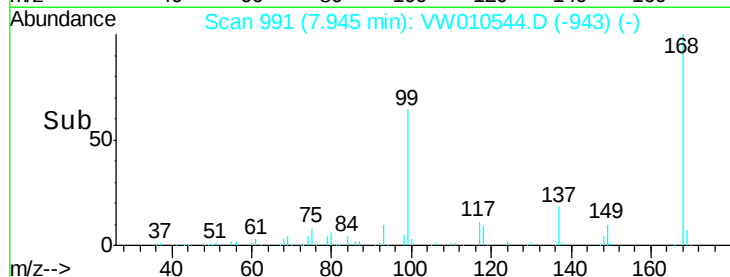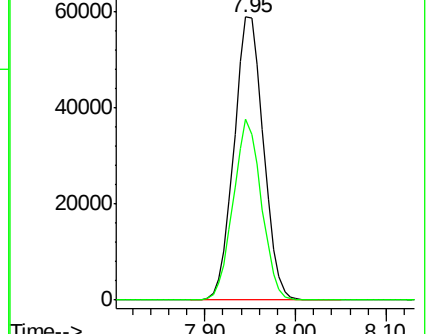

#33

1,2-Dichloroethane-d4

Concen: 48.693 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW010544.D


Acq: 24 May 2019 11:24

Tgt Ion: 65 Resp: 66802

Ion Ratio Lower Upper



65 100


67 54.9 0.0 103.6

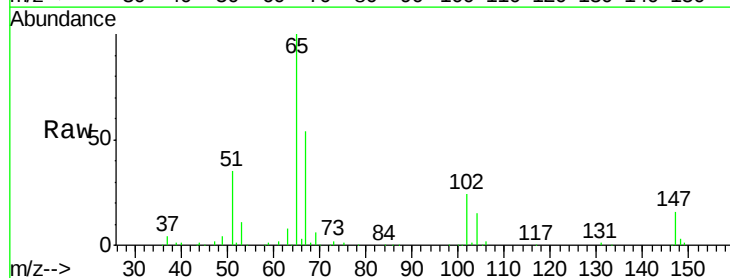

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

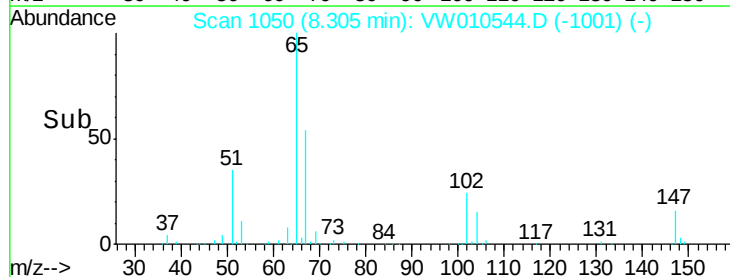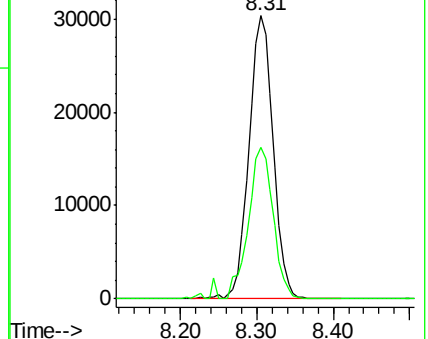


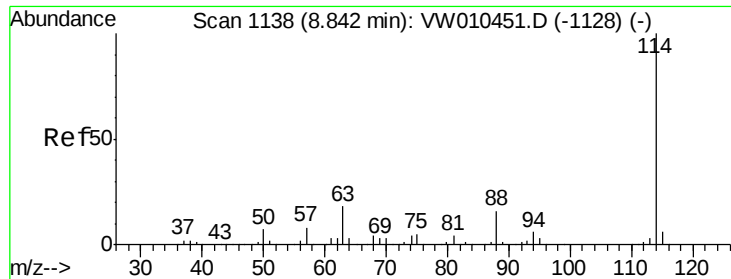




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.84 min Scan# 1138
Delta R.T. -0.00 min
Lab File: VW010544.D
Acq: 24 May 2019 11:24

Instrument :
MSVOA_W
ClientSampleId :
VW0524SBL01

Tot Ion:114 Resp: 231260
Ion Ratio Lower Upper
114 100
63 18.5 0.0 36.0
88 15.8 0.0 32.0

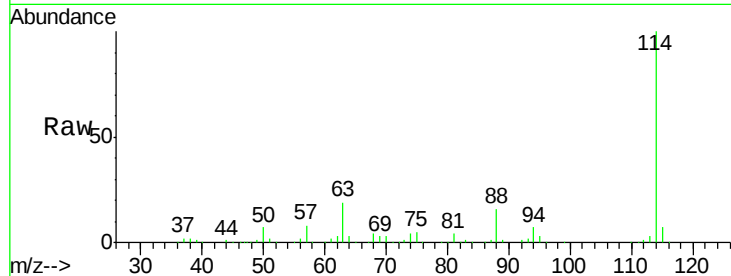


Abundance Ion 113.90 (113.60 to 114.60): V
Ion 63.00 (62.70 to 63.70): VW
Ion 87.90 (87.60 to 88.60): VW

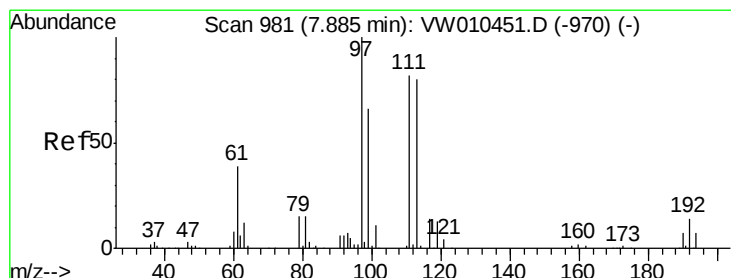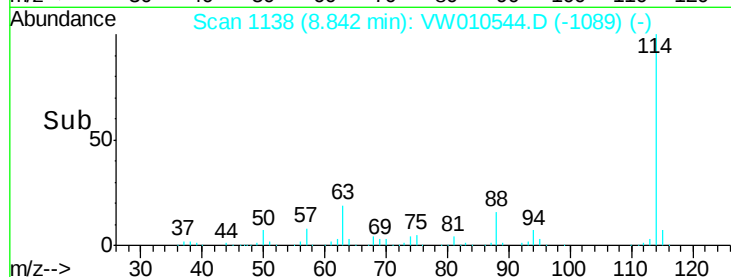
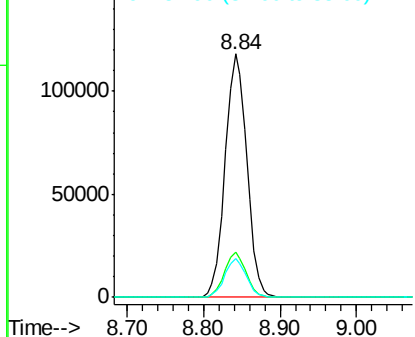



#35
Dibromofluoromethane
Concen: 49.019 ug/l
RT: 7.88 min Scan# 981
Delta R.T. -0.00 min
Lab File: VW010544.D
Acq: 24 May 2019 11:24

Tgt Ion:113 Resp: 68785
Ion Ratio Lower Upper
113 100
111 102.9 82.2 123.4
192 17.7 14.3 21.5

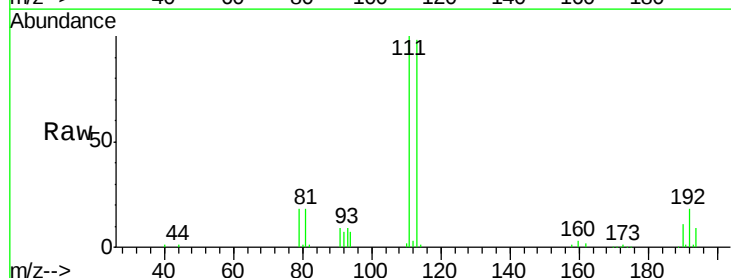

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

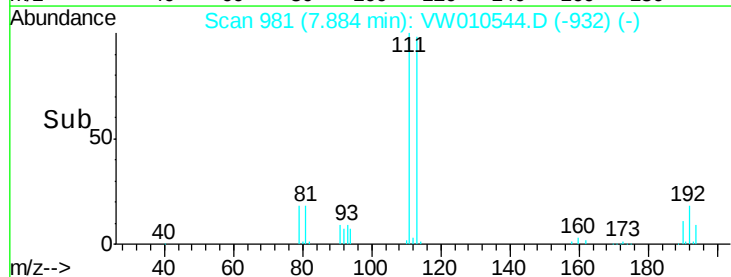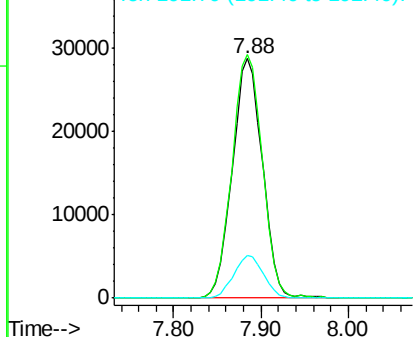

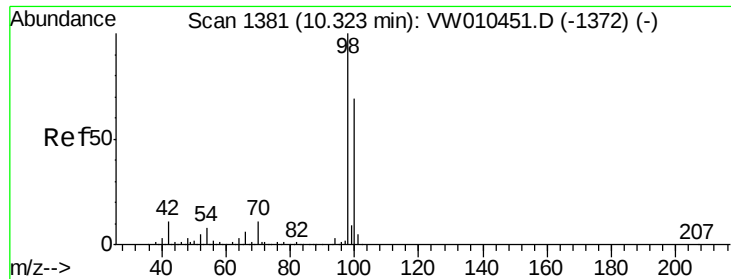

#50

Toluene-d8

Concen: 51.904 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW010544.D

Acq: 24 May 2019 11:24

Instrument :

MSVOA_W

ClientSampleId :





VW0524SBL01

Tot Ion: 98 Resp: 278244

Ion Ratio Lower Upper

98 100

100 67.5 53.7 80.5

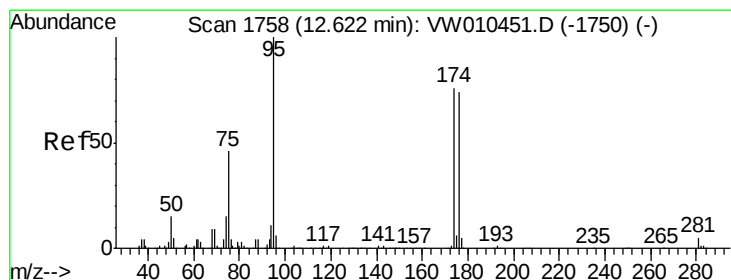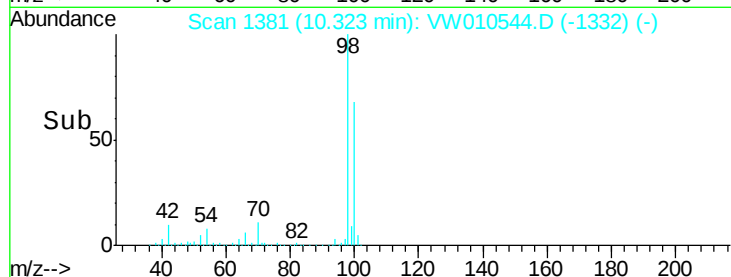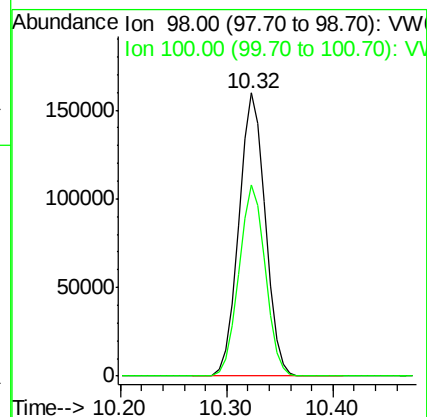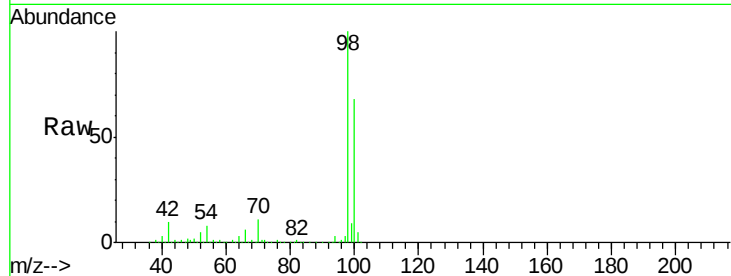

#62

4-Bromofluorobenzene

Concen: 46.780 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW010544.D

Acq: 24 May 2019 11:24




Tgt Ion: 95 Resp: 99888


Ion Ratio Lower Upper

95 100

174 71.8 0.0 148.6

176 69.8 0.0 144.2


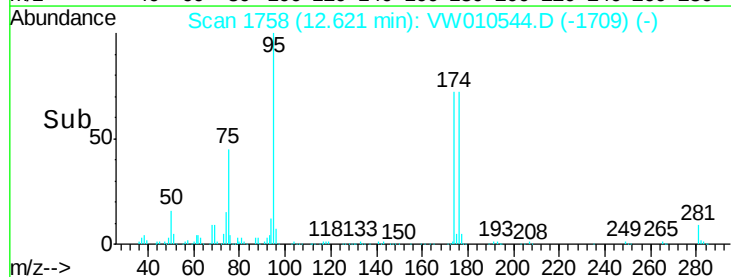
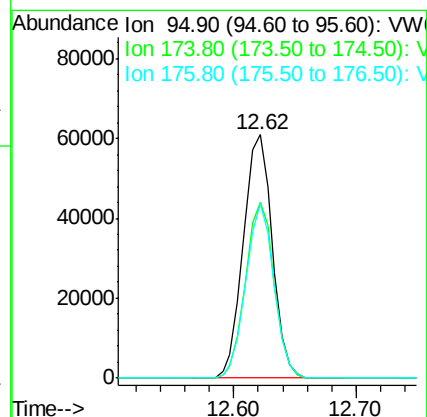
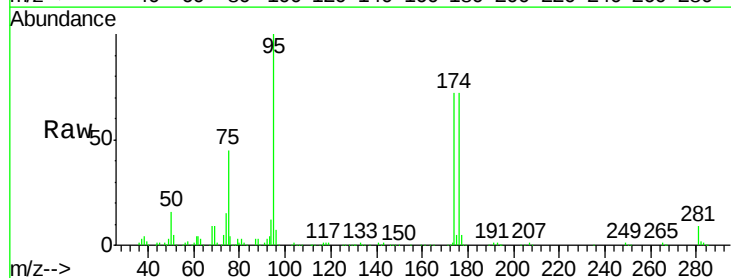


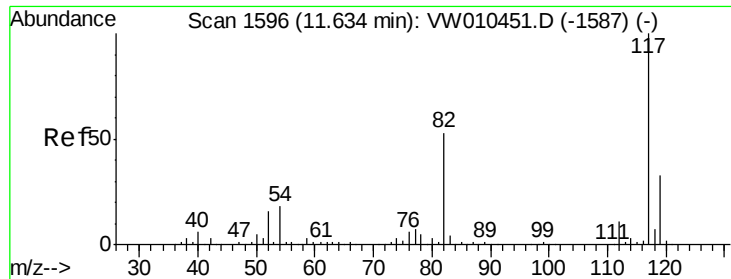

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW010544.D
Acq: 24 May 2019 11:24

Instrument :
MSVOA_W
ClientSampleId :
VW0524SBL01

Tot Ion:117 Resp: 199883
Ion Ratio Lower Upper
117 100
82 53.0 42.8 64.2
119 33.2 26.3 39.5

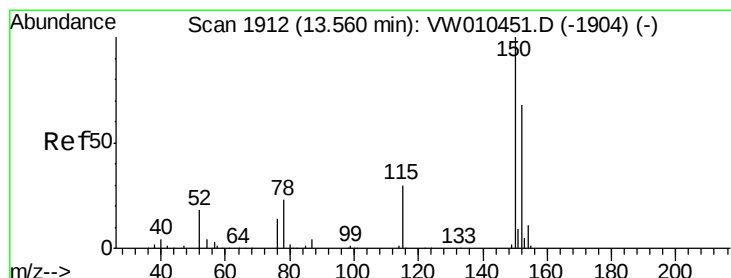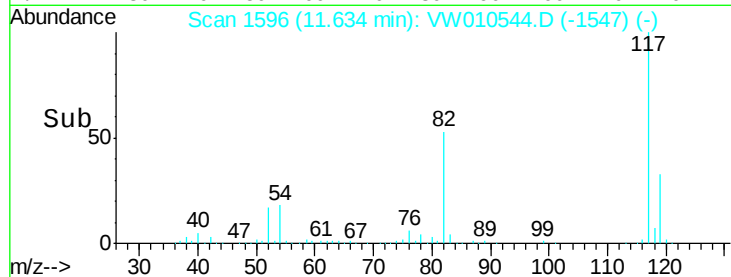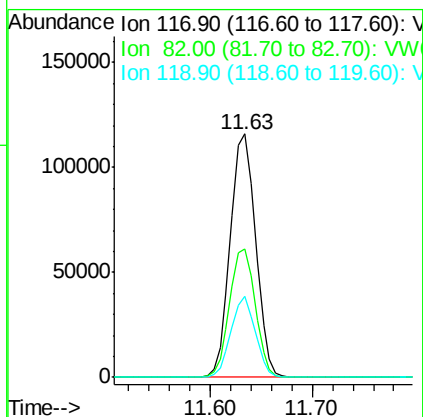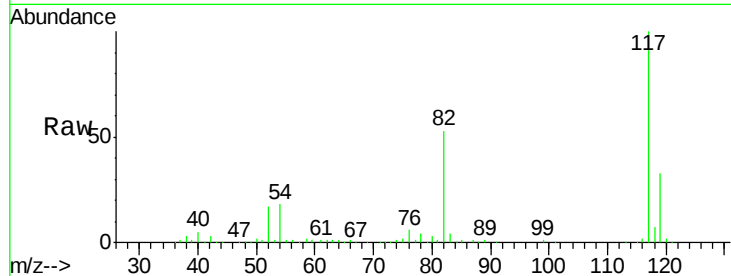

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW010544.D
Acq: 24 May 2019 11:24

Tgt Ion:152 Resp: 87102
Ion Ratio Lower Upper
152 100
115 63.1 30.3 91.0
150 158.2 0.0 349.8

