
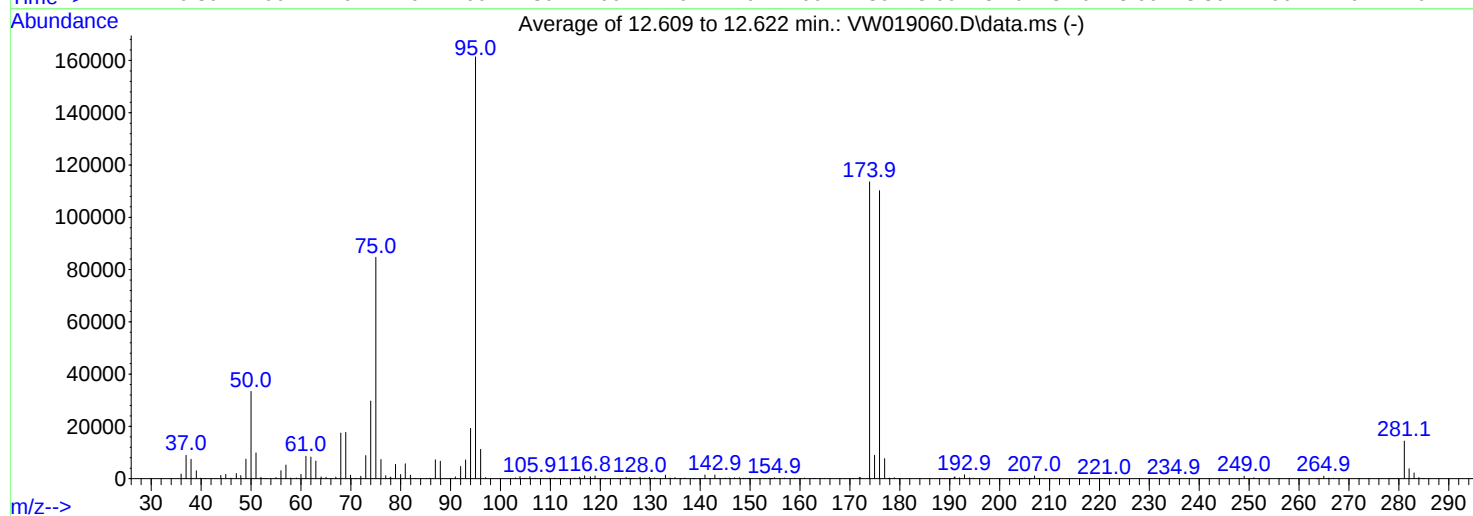


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052421\
Data File : VW019060.D
Acq On : 24 May 2021 09:50
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W052421S.M
Title : SW846 8260
Last Update : Mon May 24 14:01:57 2021

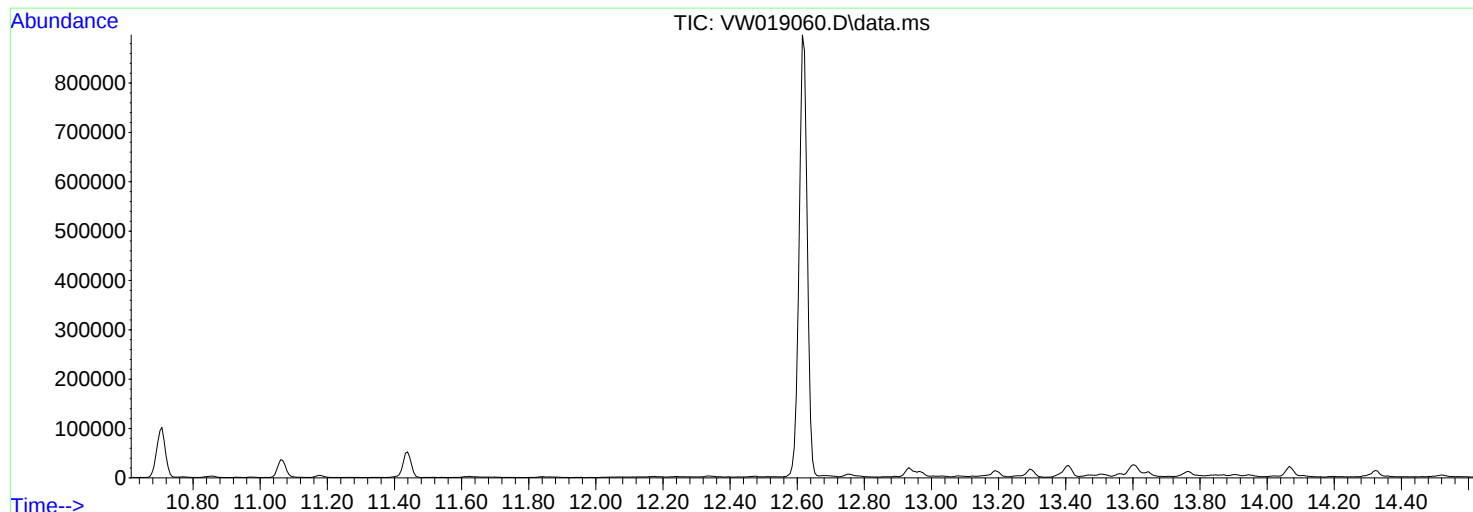

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	33352	PASS
75	95	30	60	52.5	84648	PASS
95	95	100	100	100.0	161387	PASS
96	95	5	9	6.9	11206	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.4	113584	PASS
175	174	5	9	7.9	8957	PASS
176	174	95	101	97.0	110213	PASS
177	176	5	9	6.9	7657	PASS