




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052424\
Data File : VW028737.D
Acq On : 24 May 2024 16:35
Operator : SY/MD
Sample : P2571-06
Misc : 5.35g/10mL/MSVOA_W/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH660

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/25/2024
Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 25 00:04:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 25 00:01:38 2024
Response via : Initial Calibration

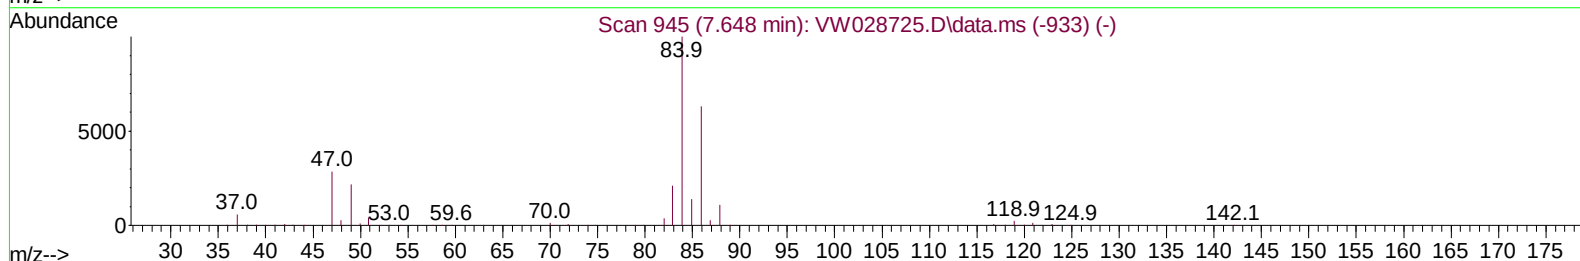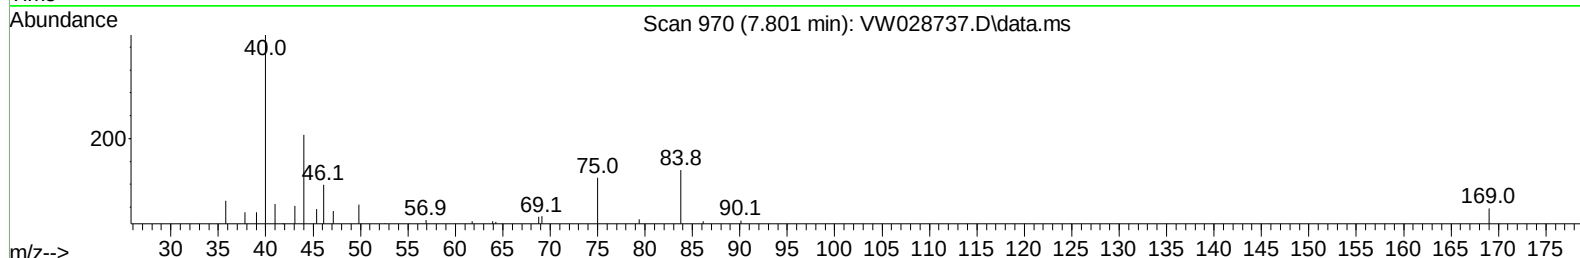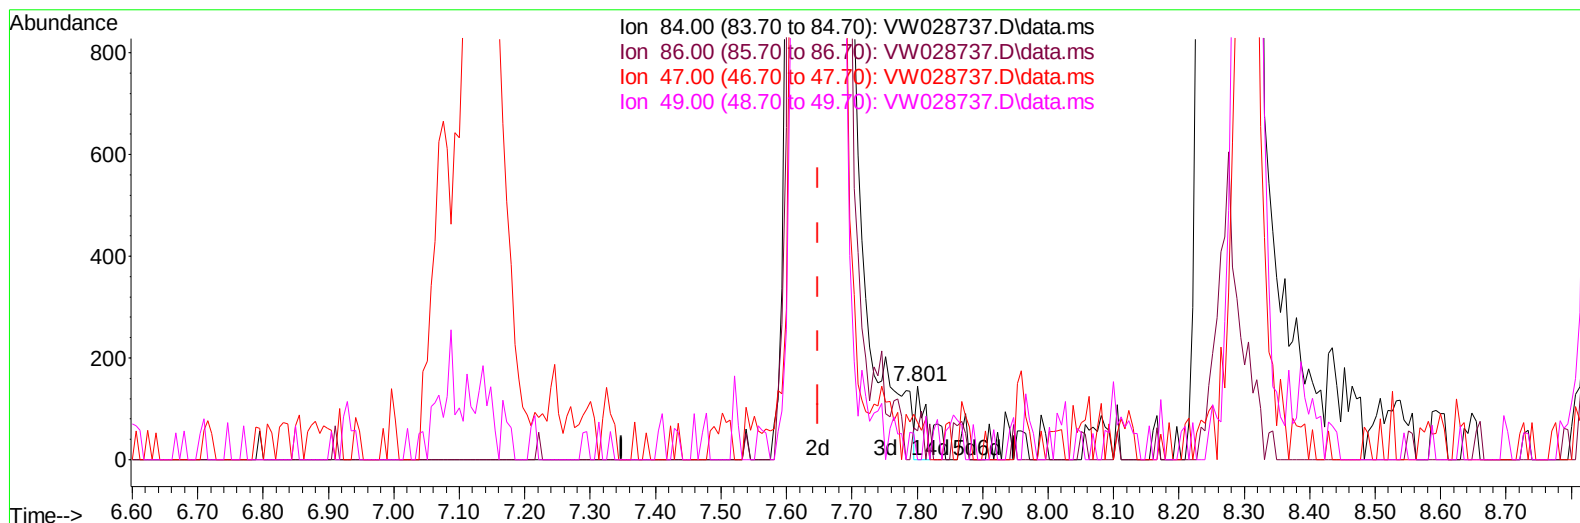

TIC: VW028737.D\data.ms

(24) Chloroform-d (S)

7.801min (+ 0.153) 0.01 ug/L

response 123

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.40	63.41
47.00	49.80	48.78
49.00	28.30	30.89




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052424\
 Data File : VW028737.D
 Acq On : 24 May 2024 16:35
 Operator : SY/MD
 Sample : P2571-06
 Misc : 5.35g/10mL/MSVOA_W/SoIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH660

Manual IntegrationsAPPROVED

Quant Time: May 25 00:04:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 25 00:01:38 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2024
 Supervised By :Mahesh Dadoda 05/28/2024

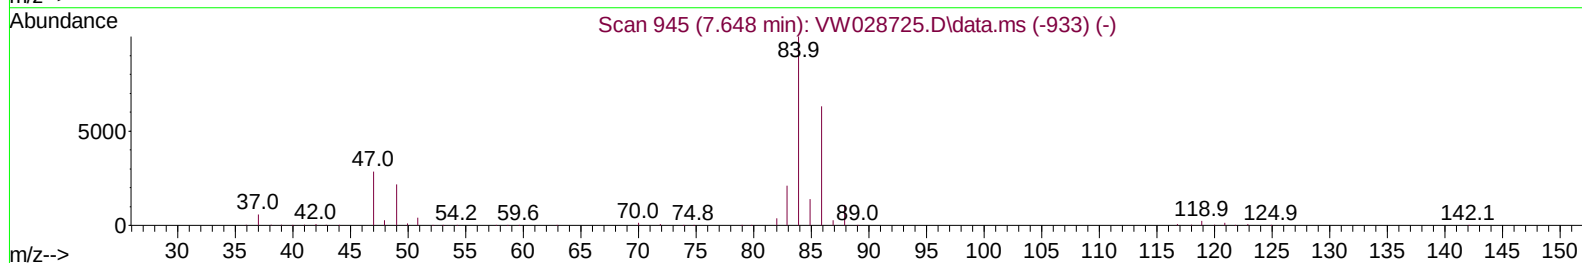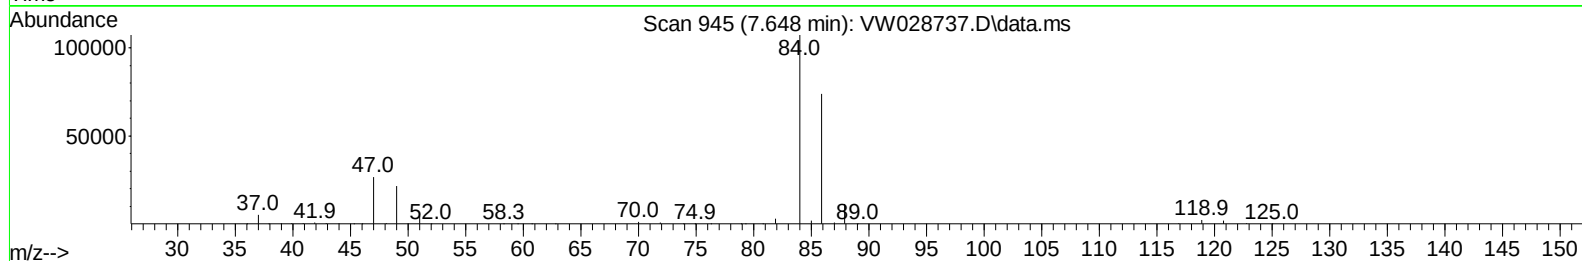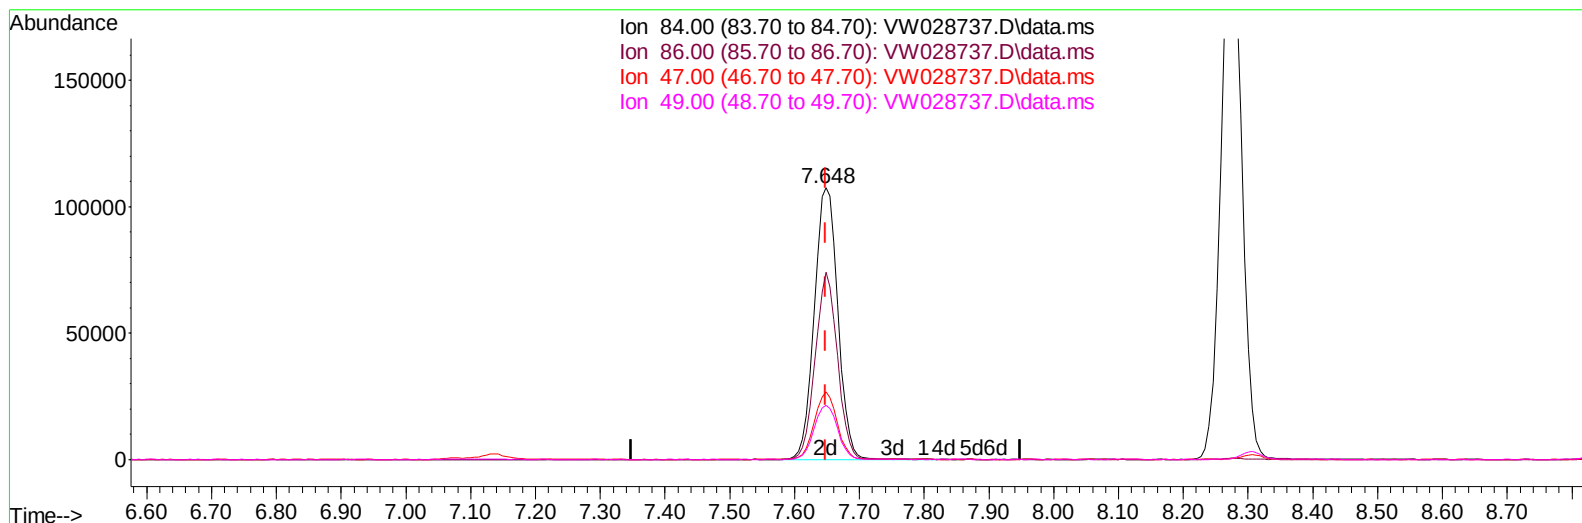

TIC: VW028737.D\data.ms

(24) Chloroform-d (S)

7.648min (+ 0.000) 24.12 ug/L m

response 270913

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.40	0.03#
47.00	49.80	0.02#
49.00	28.30	0.01#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052424\
 Data File : VW028737.D
 Acq On : 24 May 2024 16:35
 Operator : SY/MD
 Sample : P2571-06
 Misc : 5.35g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH660

Manual IntegrationsAPPROVED

Quant Time: May 25 00:04:36 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 25 00:01:38 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2024
 Supervised By :Mahesh Dadoda 05/28/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		359383	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		301988	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		99468	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		92022	13.484	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	53.920%		
7) Chloroethane-d5	2.893	69		90569	17.332	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	69.320%		
11) 1,1-Dichloroethene-d2	4.021	65		44632	15.653	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	62.600%		
21) 2-Butanone-d5	7.075	46		57644	32.376	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	64.760%		
24) Chloroform-d	7.648	84		270913m	24.125	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	96.480%		
26) 1,2-Dichloroethane-d4	8.307	65		163771	25.474	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	101.880%		
32) Benzene-d6	8.276	84		482331	23.939	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	95.760%		
36) 1,2-Dichloropropane-d6	9.276	67		175640	28.970	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	115.880%		
41) Toluene-d8	10.325	98		376503	21.101	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	84.400%		
43) trans-1,3-Dichloroprop...	10.581	79		45856	18.801	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	75.200%		
47) 2-Hexanone-d5	10.922	63		23515	22.488	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	44.980%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		137116	26.970	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	107.880%		
66) 1,2-Dichlorobenzene-d4	13.848	152		95569	25.208	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	100.840%		
Target Compounds							
13) Acetone	4.118	43		6552	4.045	ug/L	96
16) Methylene chloride	4.923	84		45150	8.123	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052424\
Data File : VW028737.D
Acq On : 24 May 2024 16:35
Operator : SY/MD
Sample : P2571-06
Misc : 5.35g/10mL/MSVOA_W/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH660

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/25/2024
Supervised By :Mahesh Dadoda 05/28/2024

Quant Time: May 25 00:04:36 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 25 00:01:38 2024
Response via : Initial Calibration

