




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052424\
Data File : VW028759.D
Acq On : 25 May 2024 01:48
Operator : SY/MD
Sample : P2588-08
Misc : 5.68g/10mL/MSVOA_W/SOIL/A
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH5S7

Manual IntegrationsAPPROVED

Quant Time: May 25 03:57:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 25 01:09:10 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2024
Supervised By :Mahesh Dadoda 05/28/2024

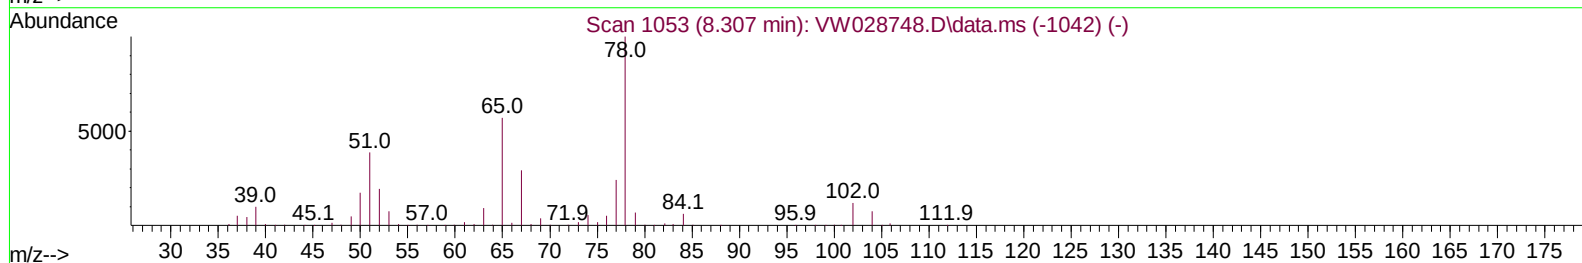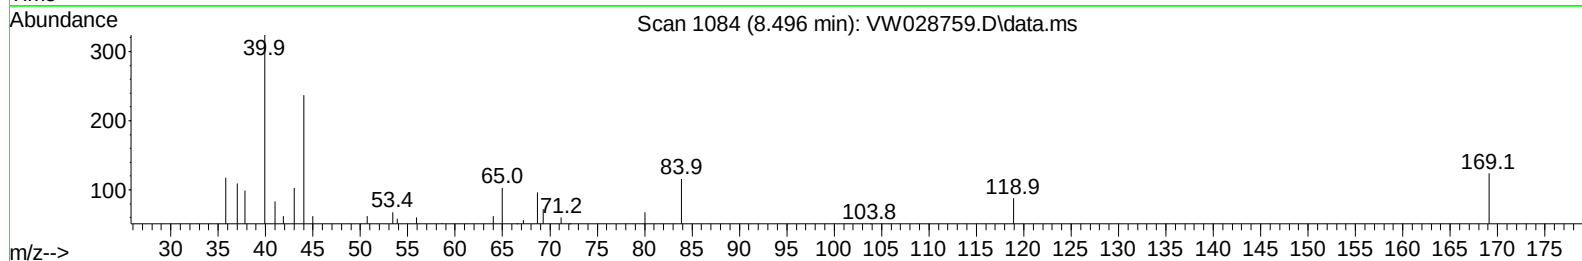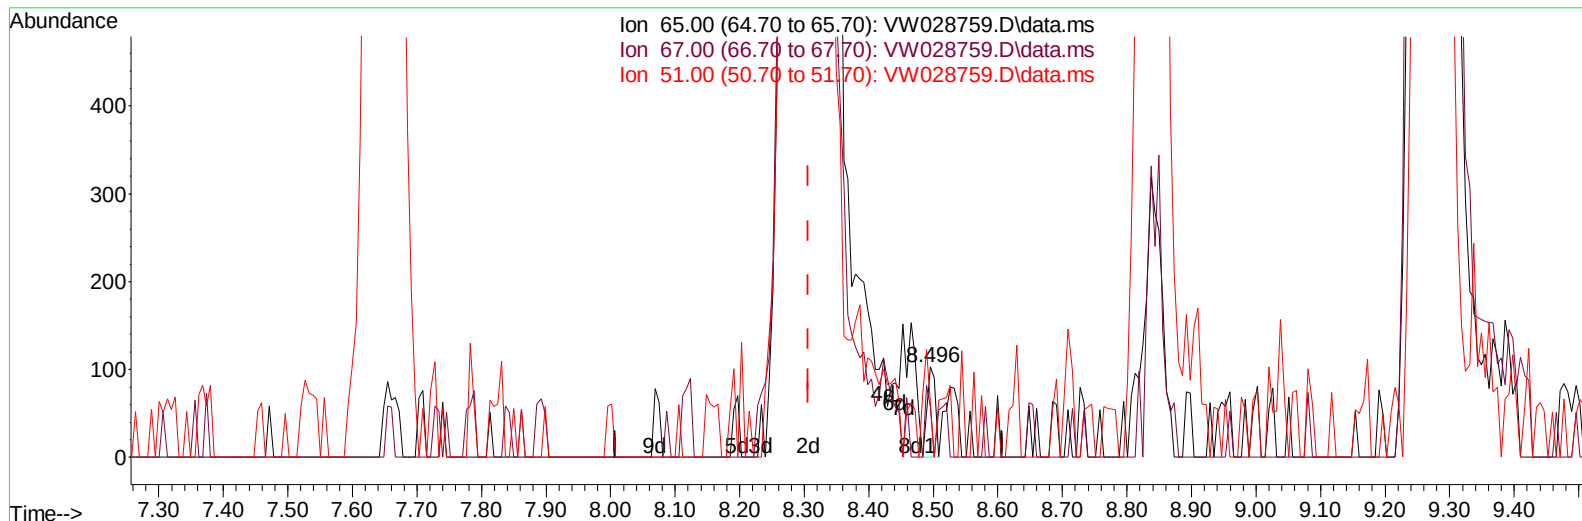

TIC: VW028759.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.496min (+ 0.189) 0.01 ug/L

response 90

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.60	56.67
51.00	101.70	104.44
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052424\
 Data File : VW028759.D
 Acq On : 25 May 2024 01:48
 Operator : SY/MD
 Sample : P2588-08
 Misc : 5.68g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH5S7

Manual IntegrationsAPPROVED

Quant Time: May 25 03:57:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 25 01:09:10 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2024
 Supervised By :Mahesh Dadoda 05/28/2024

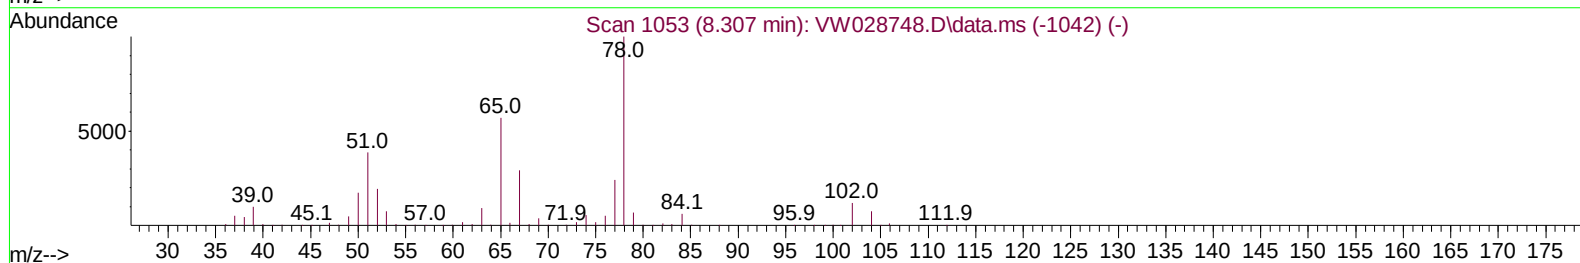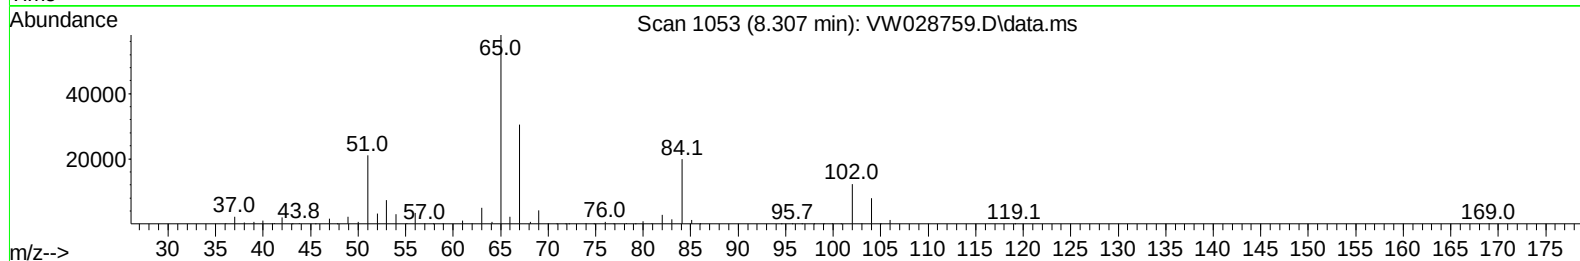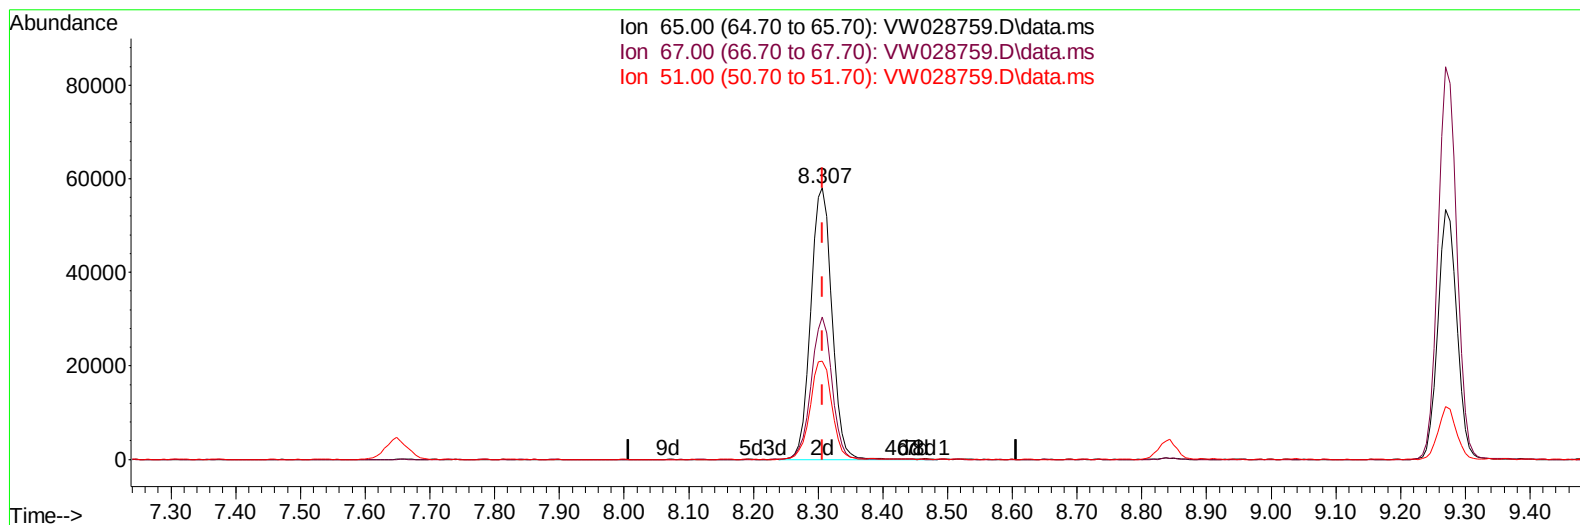

TIC: VW028759.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 19.52 ug/L m

response 131646

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.60	0.04#
51.00	101.70	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052424\
 Data File : VW028759.D
 Acq On : 25 May 2024 01:48
 Operator : SY/MD
 Sample : P2588-08
 Misc : 5.68g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BH5S7

Manual IntegrationsAPPROVED

Quant Time: May 25 03:57:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat May 25 01:09:10 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2024
 Supervised By :Mahesh Dadoda 05/28/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		377036	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		237141	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		39525	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		113944	15.915	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	63.640%		
7) Chloroethane-d5	2.899	69		101569	18.527	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	74.120%		
11) 1,1-Dichloroethene-d2	4.021	65		47571	15.903	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	63.600%		
21) 2-Butanone-d5	7.075	46		65737	35.193	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	70.380%		
24) Chloroform-d	7.648	84		264289	22.433	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	89.720%		
26) 1,2-Dichloroethane-d4	8.307	65		131646m	19.518	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	78.080%		
32) Benzene-d6	8.276	84		495983	31.348	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	125.400%		
36) 1,2-Dichloropropane-d6	9.270	67		169265	35.553	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	142.200%#		
41) Toluene-d8	10.325	98		350505	25.015	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	100.080%		
43) trans-1,3-Dichloroprop...	10.575	79		27194	14.199	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	56.800%		
47) 2-Hexanone-d5	10.922	63		37173	45.270	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	90.540%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		109161	27.343	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	109.360%		
66) 1,2-Dichlorobenzene-d4	13.848	152		44738	29.697	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	118.800%		
Target Compounds							
16) Methylene chloride	4.917	84		15074	2.585	ug/L	Qvalue 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052424\
Data File : VW028759.D
Acq On : 25 May 2024 01:48
Operator : SY/MD
Sample : P2588-08
Misc : 5.68g/10mL/MSVOA_W/SOIL/A
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BH5S7

Manual IntegrationsAPPROVED

Quant Time: May 25 03:57:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Sat May 25 01:09:10 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/25/2024
Supervised By :Mahesh Dadoda 05/28/2024

