


Data Path : W:\HPCHEM1\MSVOA_W\DATA\VW052518\
Data File : VW002856.D
Acq On : 24 May 2018 21:03
Operator : JC/SY
Sample : BFB
Misc : 5.00G/5.0ML/MSVOA_W/SOIL
ALS Vial : 25 Sample Multiplier: 1

Integration File: RTEINT.P

Method : W:\HPCHEM1\MSVOA_W\METHOD\82W051518S.M
Title : SW846 8260
Last Update : Tue May 15 03:32:11 2018

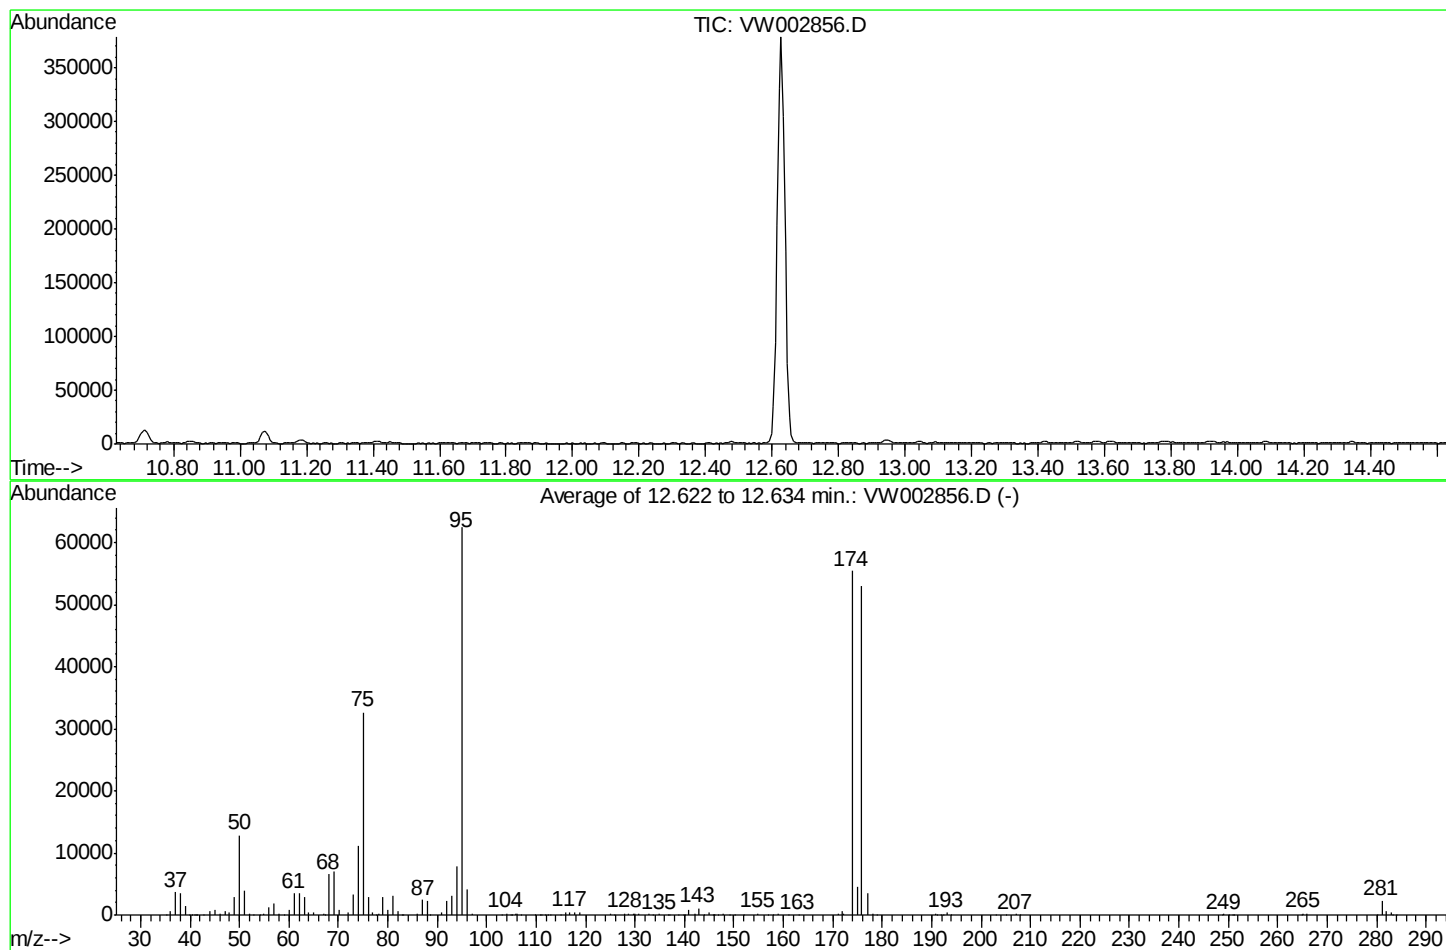

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	12867	PASS
75	95	30	60	52.3	32656	PASS
95	95	100	100	100.0	62442	PASS
96	95	5	9	6.5	4057	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	88.8	55448	PASS
175	174	5	9	8.2	4538	PASS
176	174	95	101	95.7	53037	PASS
177	176	5	9	6.6	3517	PASS