

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023307.D
 Acq On : 25 May 2022 09:35
 Operator : SY/VA
 Sample : VW0525SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK517

Quant Time: May 26 01:28:29 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	338391	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	327102	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	170402	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	117780	16.965	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.840%
7) Chloroethane-d5	2.885	69	78274	17.330	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.320%
11) 1,1-Dichloroethene-d2	4.019	63	133325	14.862	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.440%
21) 2-Butanone-d5	7.074	46	61001	46.213	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.420%
24) Chloroform-d	7.653	84	219505	22.141	ug/L	0.01
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.560%
26) 1,2-Dichloroethane-d4	8.305	65	124081	22.820	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.280%
32) Benzene-d6	8.275	84	430789	22.849	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.400%
36) 1,2-Dichloropropane-d6	9.274	67	125360	23.670	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.680%
41) Toluene-d8	10.323	98	408374	22.422	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.680%
43) trans-1,3-Dichloroprop...	10.579	79	51925	21.293	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.160%
47) 2-Hexanone-d5	10.927	63	47742	47.222	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.440%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	115013	23.299	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.200%
66) 1,2-Dichlorobenzene-d4	13.853	152	144225	24.212	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.840%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4370	0.604	ug/L	# 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023307.D
Acq On : 25 May 2022 09:35
Operator : SY/VA
Sample : VW0525SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK517

Quant Time: May 26 01:28:29 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

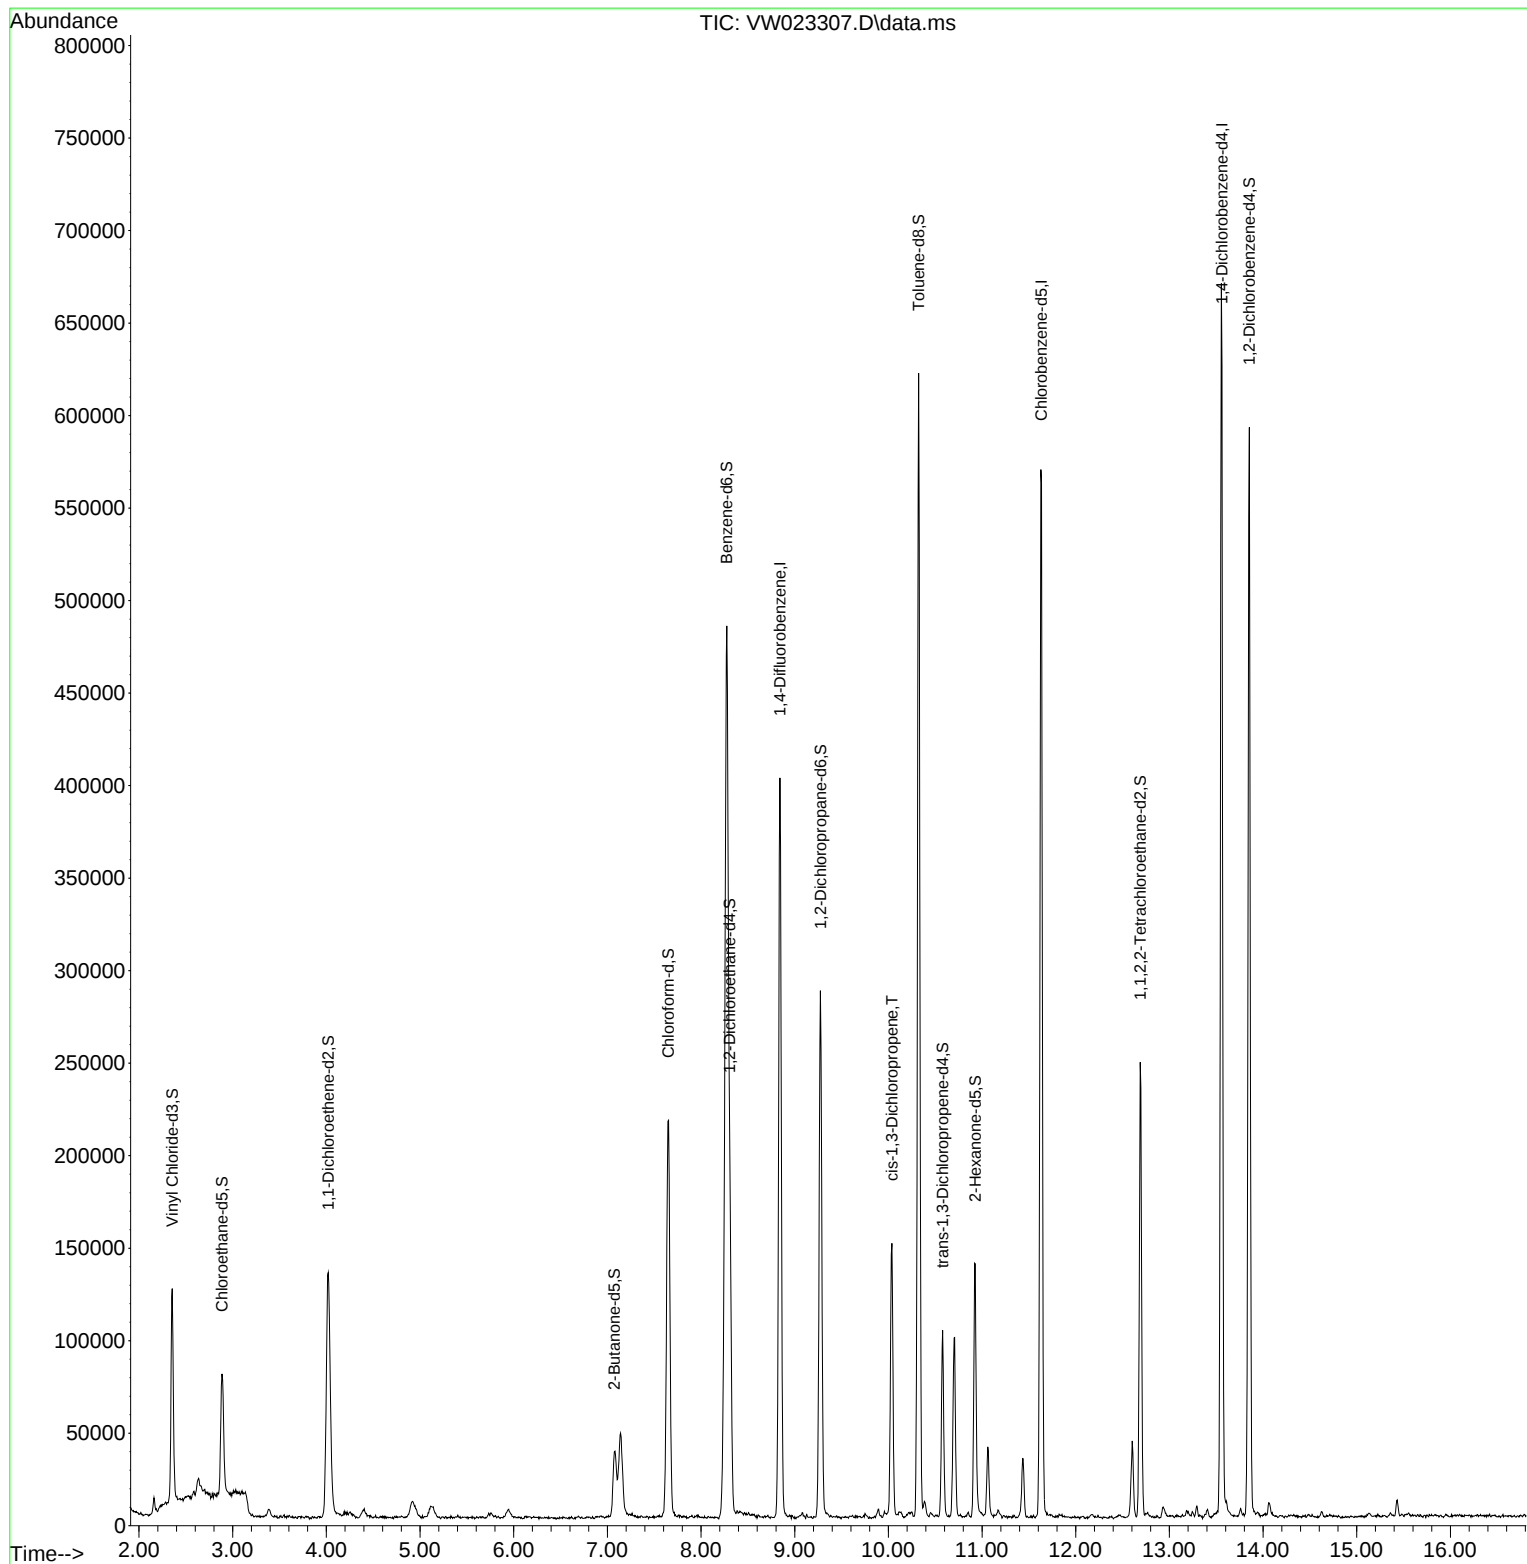

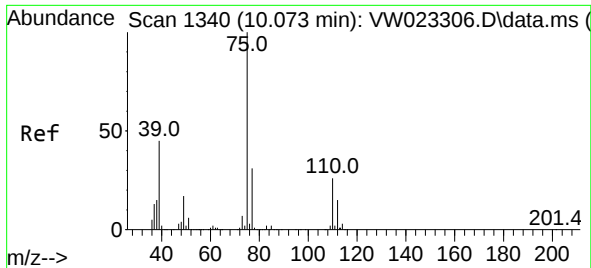

#39
 cis-1,3-Dichloropropene
 Concen: 0.604 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023307.D
 Acq: 25 May 2022 09:35

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK517

Tgt Ion: 75 Resp: 4370
 Ion Ratio Lower Upper
 75 100
 77 46.5 22.1 41.1#

