

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023317.D
 Acq On : 25 May 2022 13:35
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK482

Quant Time: May 26 01:31:26 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	318863	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	321861	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	160949	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	121739	18.609	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.440%
7) Chloroethane-d5	2.879	69	77291	18.160	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.640%
11) 1,1-Dichloroethene-d2	4.019	63	122933	14.543	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	58.160%
21) 2-Butanone-d5	7.080	46	67536	54.297	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.600%
24) Chloroform-d	7.647	84	218715	23.412	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.640%
26) 1,2-Dichloroethane-d4	8.384	65	240	0.047	ug/L	0.08
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.200%#
32) Benzene-d6	8.275	84	419100	22.591	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.360%
36) 1,2-Dichloropropane-d6	9.274	67	124150	23.823	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.280%
41) Toluene-d8	10.323	98	399817	22.310	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.240%
43) trans-1,3-Dichloroprop...	10.579	79	54997	22.920	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.680%
47) 2-Hexanone-d5	10.920	63	54423	54.706	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.420%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	120635	24.836	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.360%
66) 1,2-Dichlorobenzene-d4	13.853	152	140567	24.984	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.920%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	5041	0.709	ug/L	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023317.D
Acq On : 25 May 2022 13:35
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK482

Quant Time: May 26 01:31:26 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

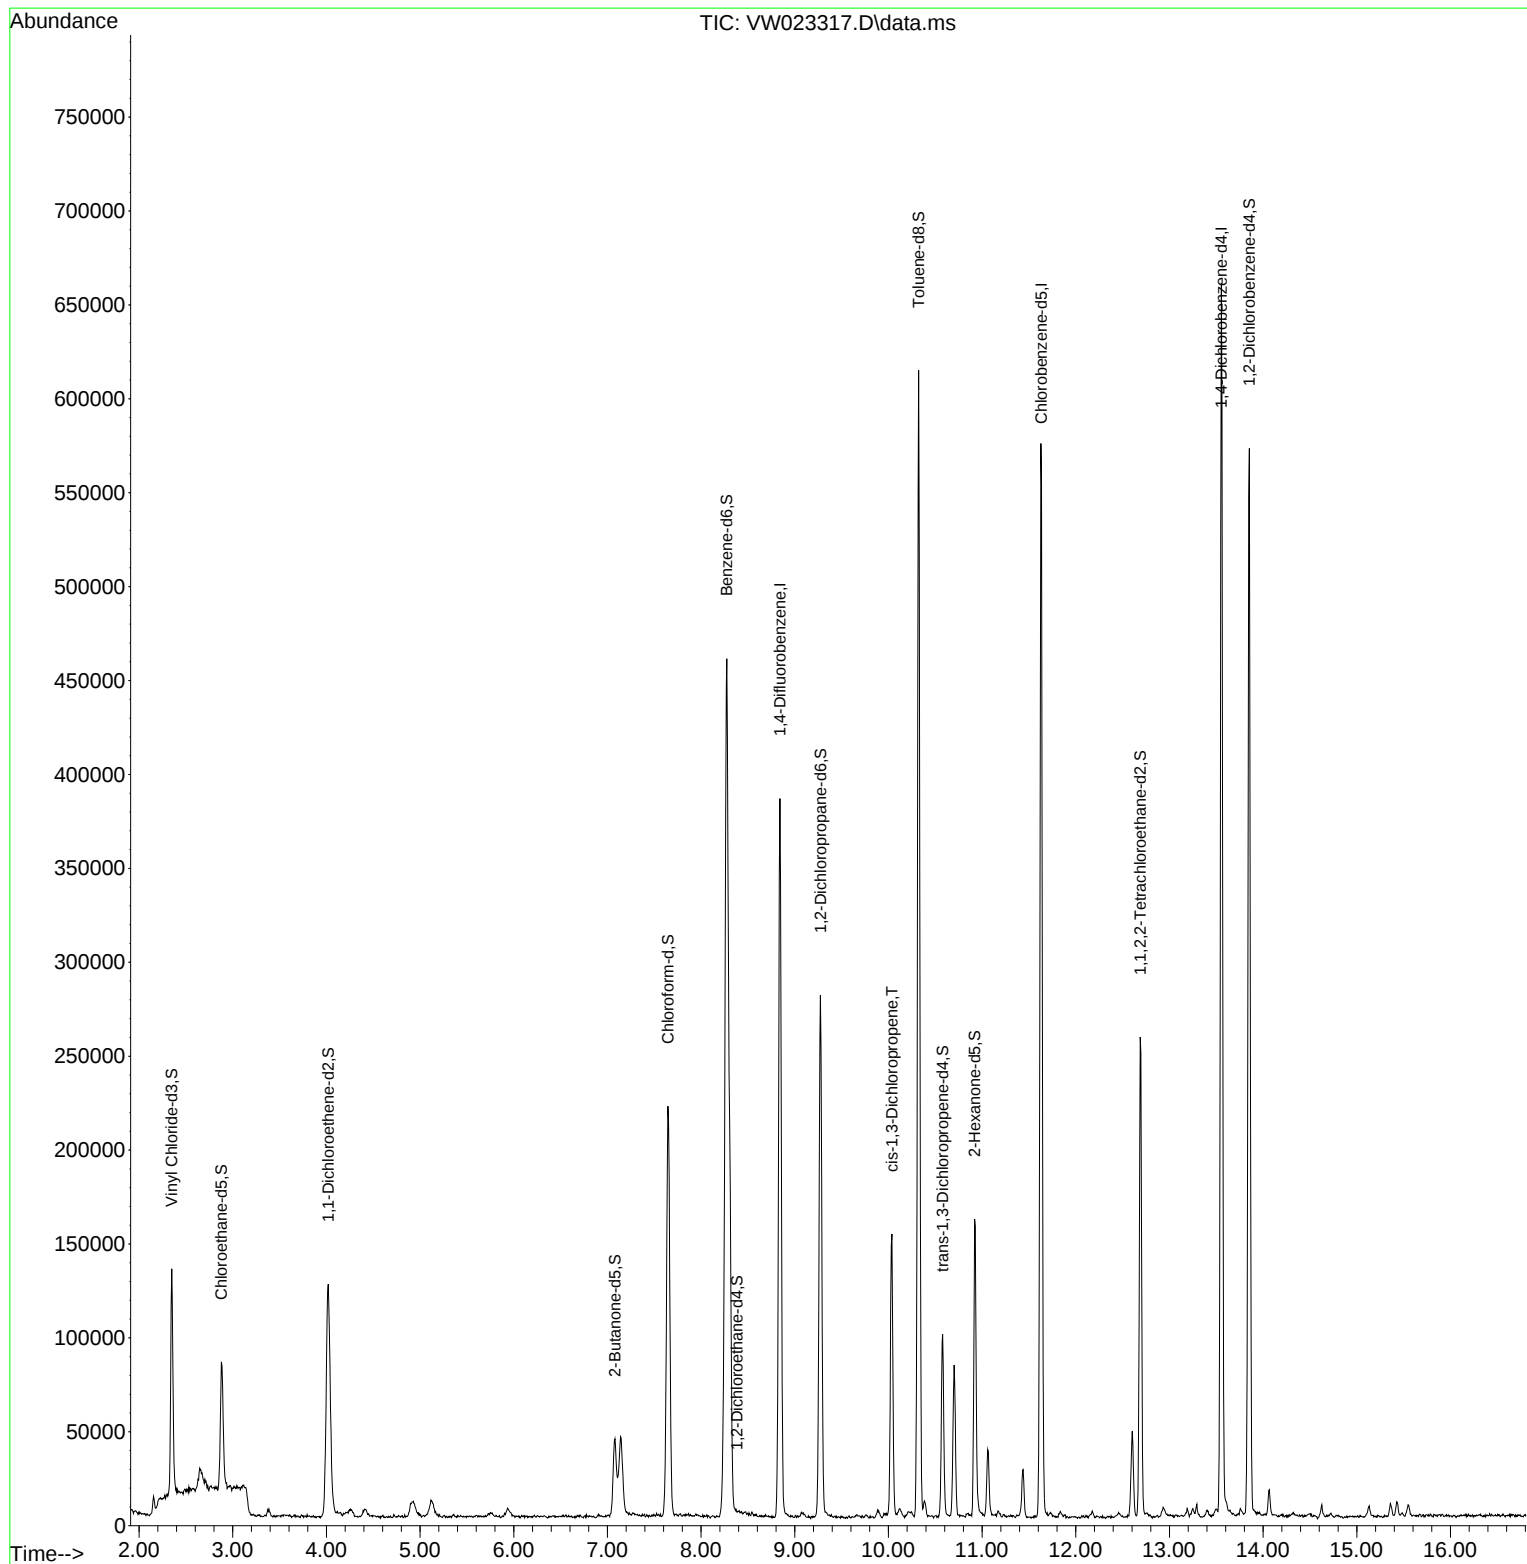

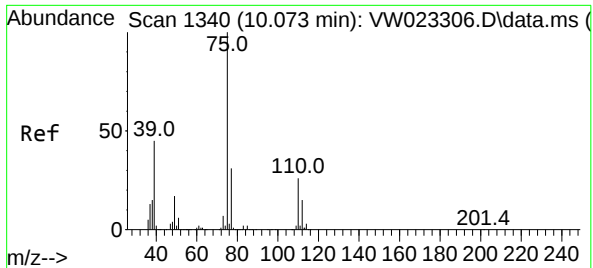

#39
 cis-1,3-Dichloropropene
 Concen: 0.709 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023317.D
 Acq: 25 May 2022 13:35

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK482

Tgt Ion: 75 Resp: 5041
 Ion Ratio Lower Upper
 75 100
 77 38.2 22.1 41.1

