

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023327.D
 Acq On : 25 May 2022 17:36
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK483

Quant Time: May 26 01:33:14 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	291751	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	295044	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	152074	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	114224	19.083	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.320%
7) Chloroethane-d5	2.879	69	75513	19.391	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.560%
11) 1,1-Dichloroethene-d2	4.013	63	114197	14.765	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.080%
21) 2-Butanone-d5	7.074	46	61338	53.896	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.800%
24) Chloroform-d	7.653	84	209692	24.532	ug/L	0.01
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.120%
26) 1,2-Dichloroethane-d4	8.305	65	124407	26.537	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.160%
32) Benzene-d6	8.275	84	407625	23.969	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.880%
36) 1,2-Dichloropropane-d6	9.275	67	120806	25.289	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.160%
41) Toluene-d8	10.323	98	379816	23.120	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.480%
43) trans-1,3-Dichloroprop...	10.579	79	50535	22.975	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.920%
47) 2-Hexanone-d5	10.921	63	52198	57.239	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.480%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	119282	26.790	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	107.160%
66) 1,2-Dichlorobenzene-d4	13.853	152	137653	25.894	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.560%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4560	0.699	ug/L	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023327.D
Acq On : 25 May 2022 17:36
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK483

Quant Time: May 26 01:33:14 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

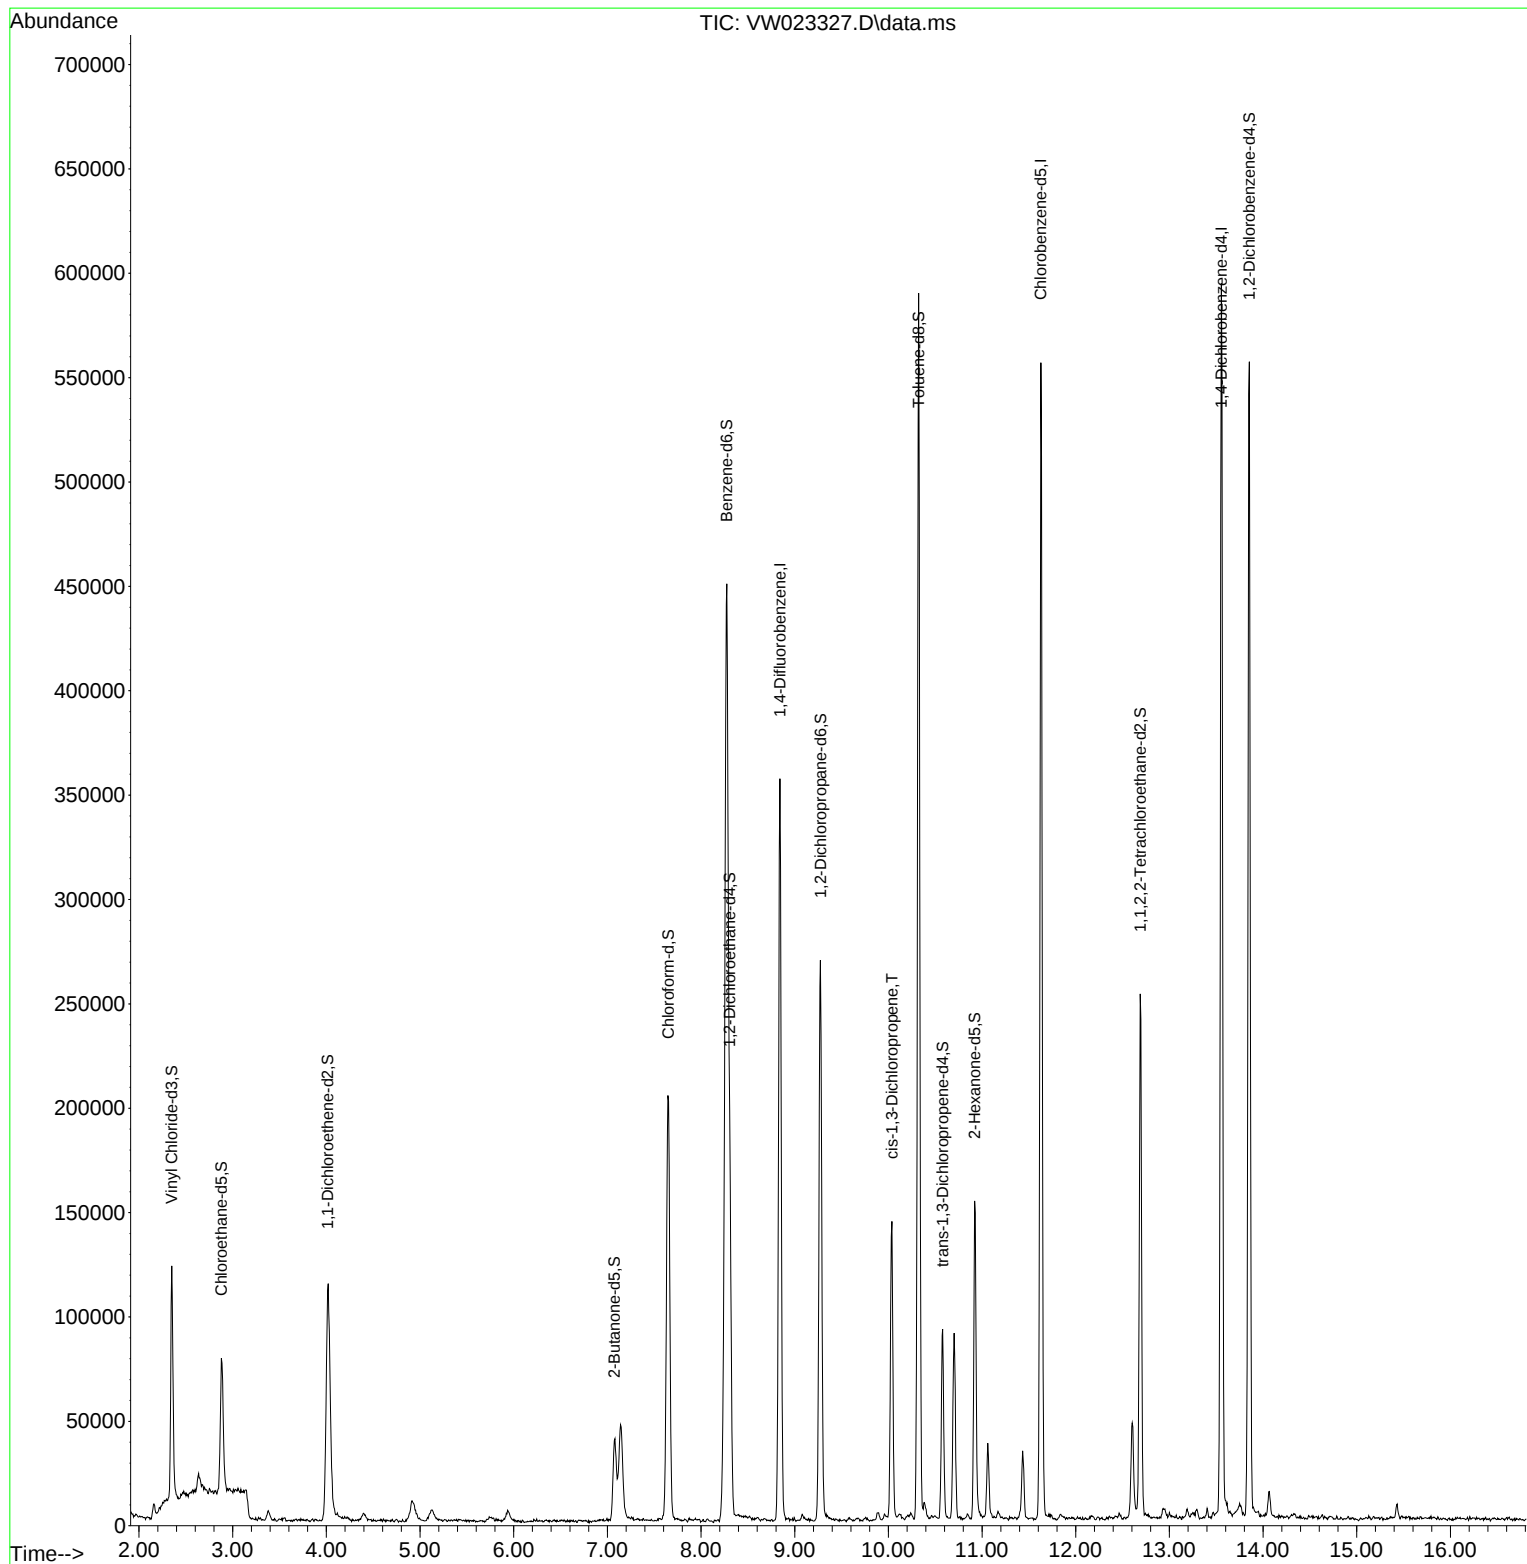

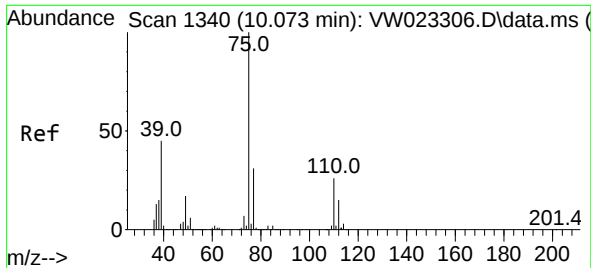

#39
 cis-1,3-Dichloropropene
 Concen: 0.699 ug/L
 RT: 10.037 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023327.D
 Acq: 25 May 2022 17:36

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK483

Tgt Ion: 75 Resp: 4560
 Ion Ratio Lower Upper
 75 100
 77 40.8 22.1 41.1

