

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023334.D
 Acq On : 25 May 2022 21:28
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK484

Quant Time: May 26 05:15:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	286227	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	292499	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	144028	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	115644	19.693	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.760%
7) Chloroethane-d5	2.885	69	72717	19.034	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	76.120%
11) 1,1-Dichloroethene-d2	4.019	63	112361	14.808	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	59.240%
21) 2-Butanone-d5	7.080	46	56573	50.669	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.340%
24) Chloroform-d	7.647	84	206567	24.633	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.520%
26) 1,2-Dichloroethane-d4	8.305	65	119244	25.927	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.720%
32) Benzene-d6	8.275	84	397183	23.558	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.240%
36) 1,2-Dichloropropane-d6	9.268	67	119934	25.325	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.280%
41) Toluene-d8	10.323	98	369060	22.661	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.640%
43) trans-1,3-Dichloroprop...	10.579	79	47661	21.857	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.440%
47) 2-Hexanone-d5	10.927	63	46561	51.502	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.000%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	112785	25.551	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	13.853	152	132246	26.267	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.080%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	4819	0.745	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023334.D
Acq On : 25 May 2022 21:28
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK484

Quant Time: May 26 05:15:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 04:46:06 2022
Response via : Initial Calibration

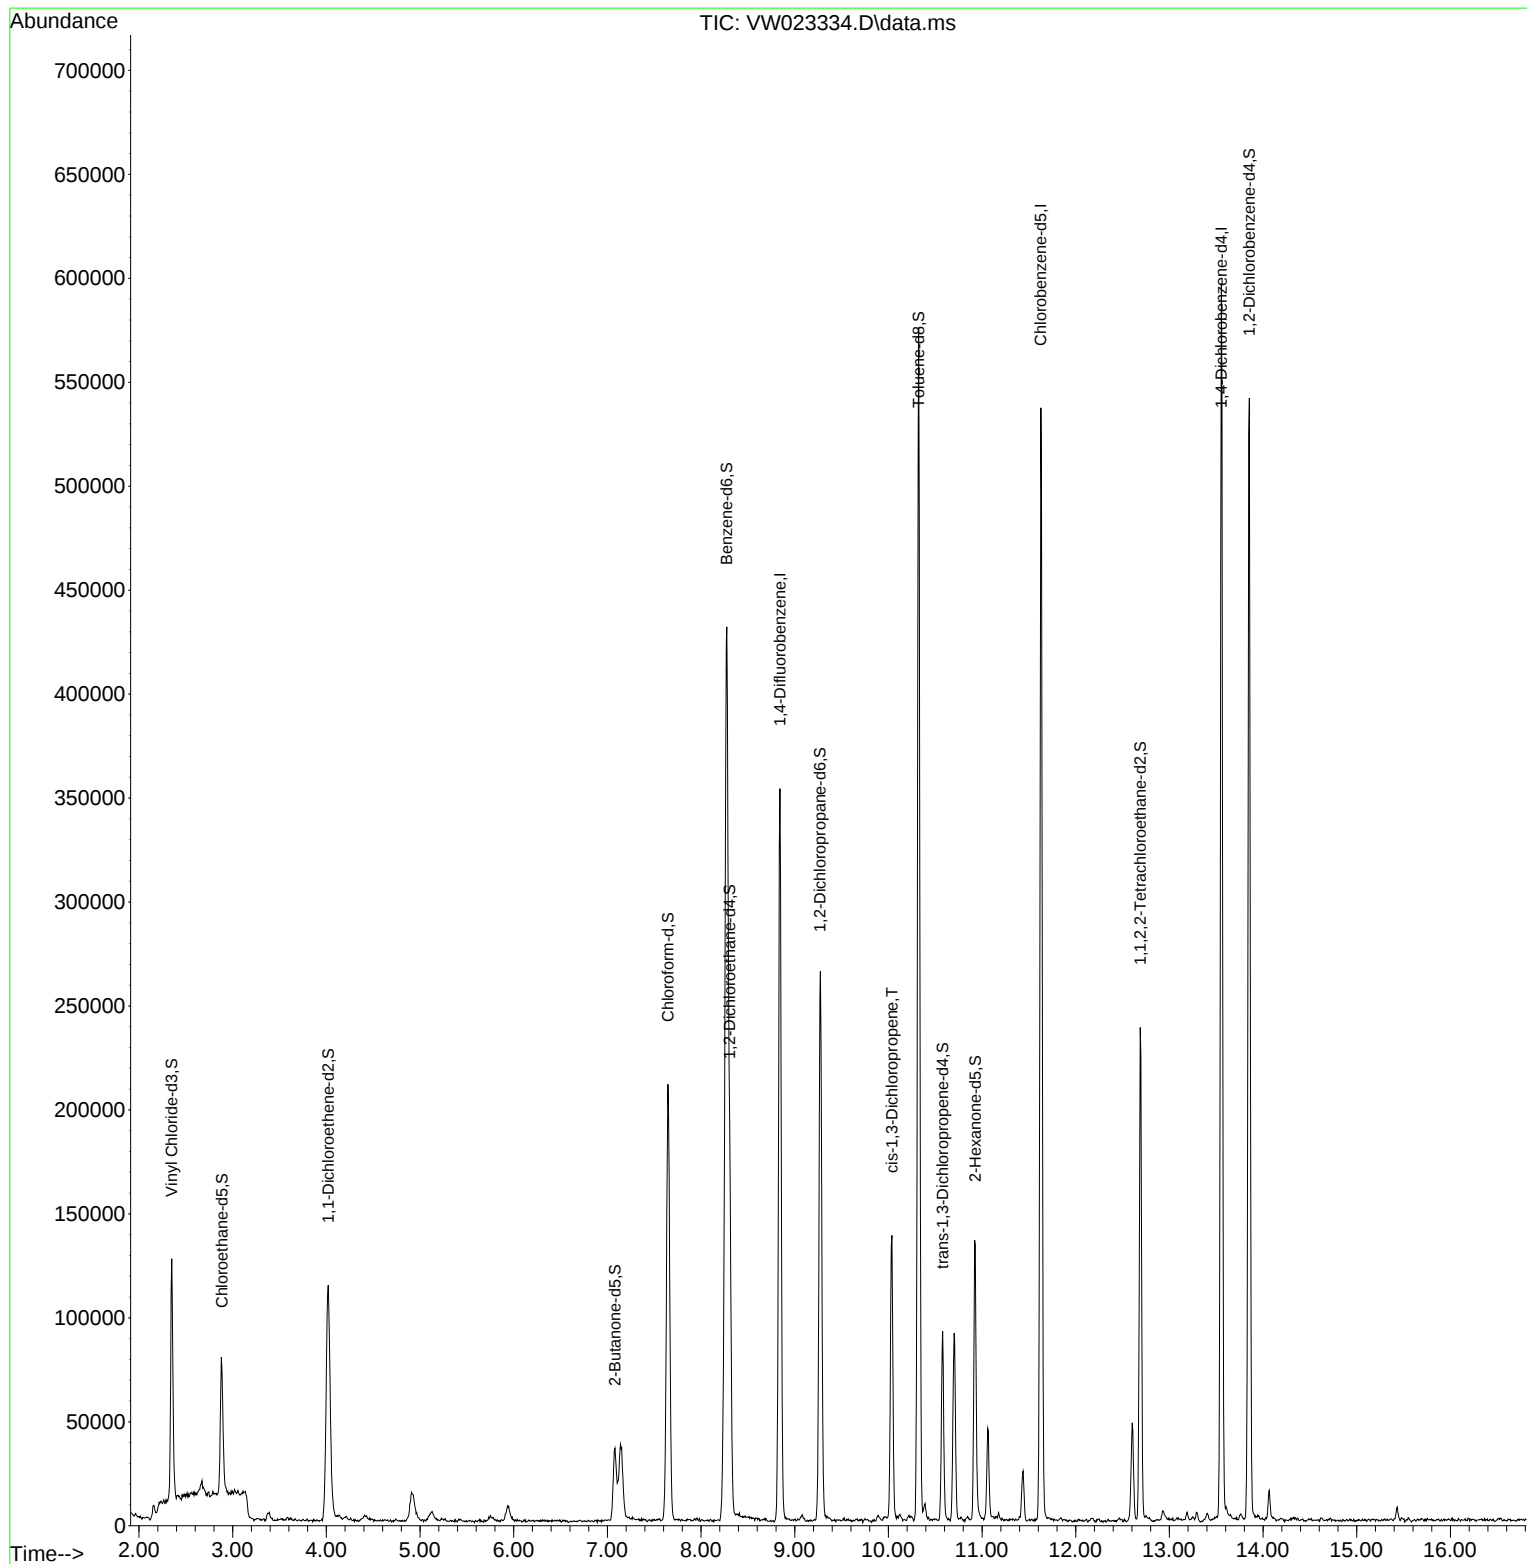

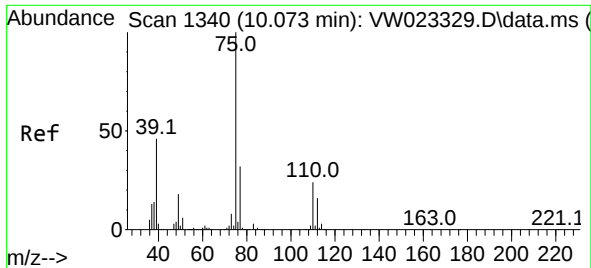

#39
 cis-1,3-Dichloropropene
 Concen: 0.745 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023334.D
 Acq: 25 May 2022 21:28

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK484

Tgt Ion: 75 Resp: 4819
 Ion Ratio Lower Upper
 75 100
 77 37.9 22.1 41.1

