




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023308.D
 Acq On : 25 May 2022 09:59
 Operator : SY/VA
 Sample : N2929-09
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:28:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

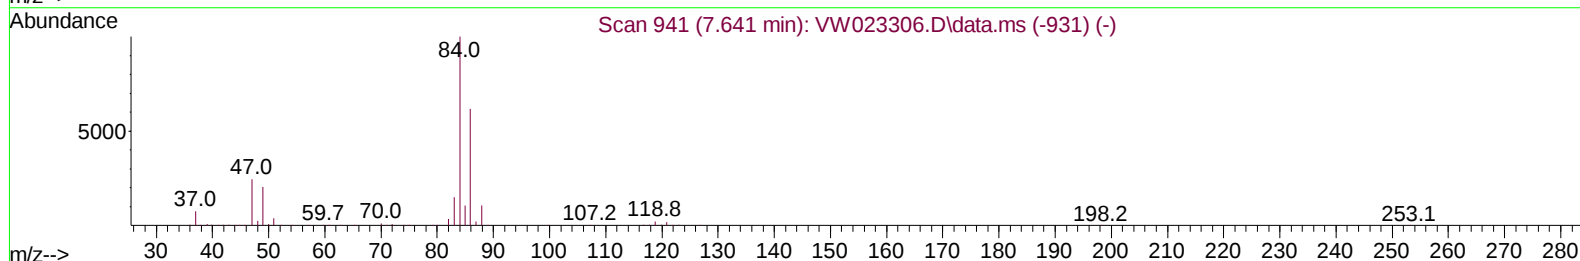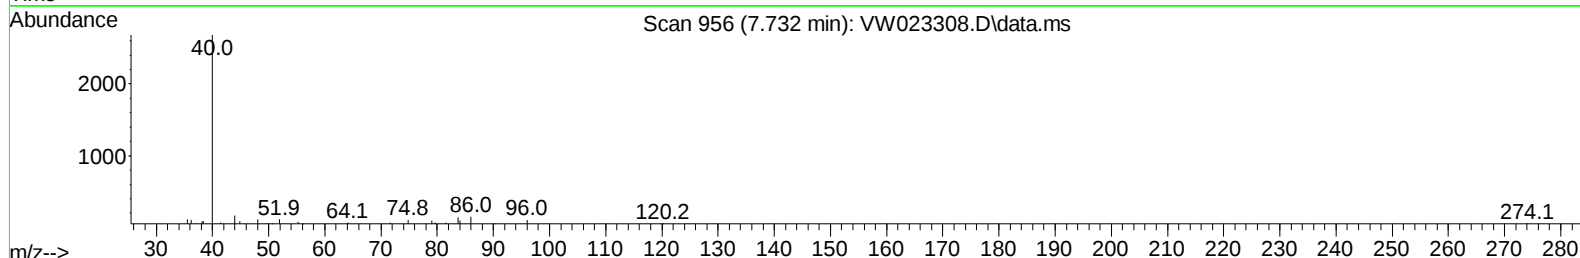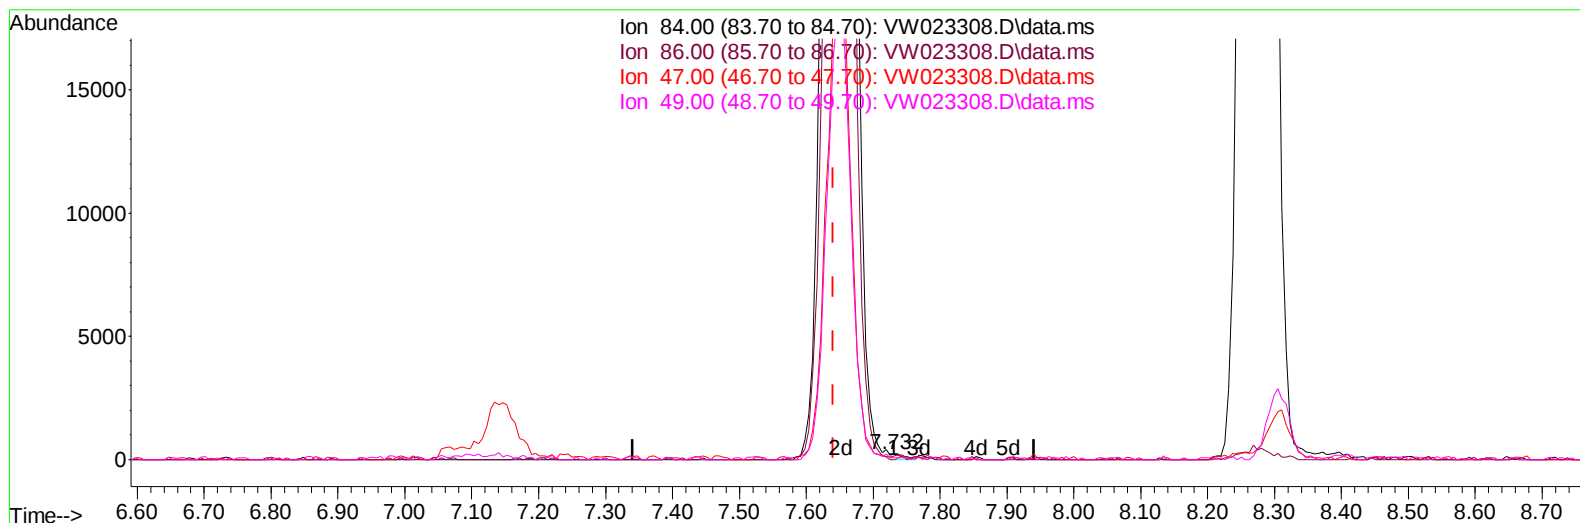

TIC: VW023308.D\data.ms

(24) Chloroform-d (S)

7.732min (+ 0.091) 0.02 ug/L

response 248

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.90	76.61
47.00	43.20	41.53
49.00	26.40	30.65




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023308.D
 Acq On : 25 May 2022 09:59
 Operator : SY/VA
 Sample : N2929-09
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 26 01:28:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

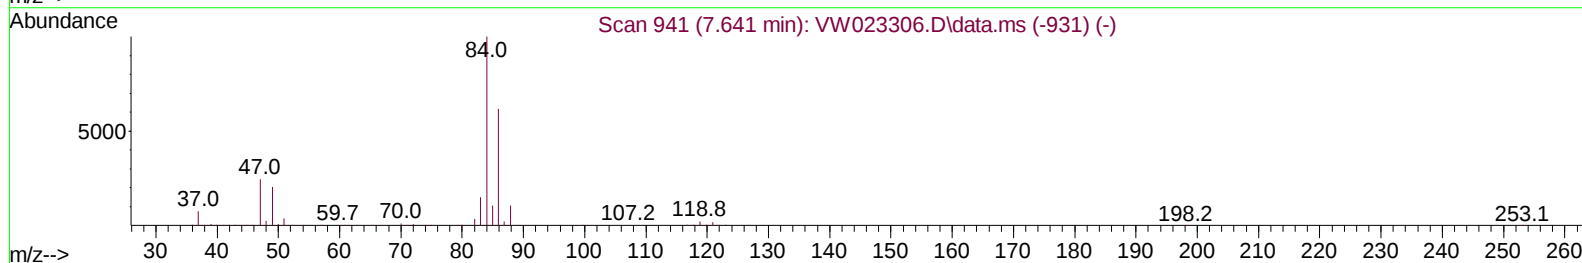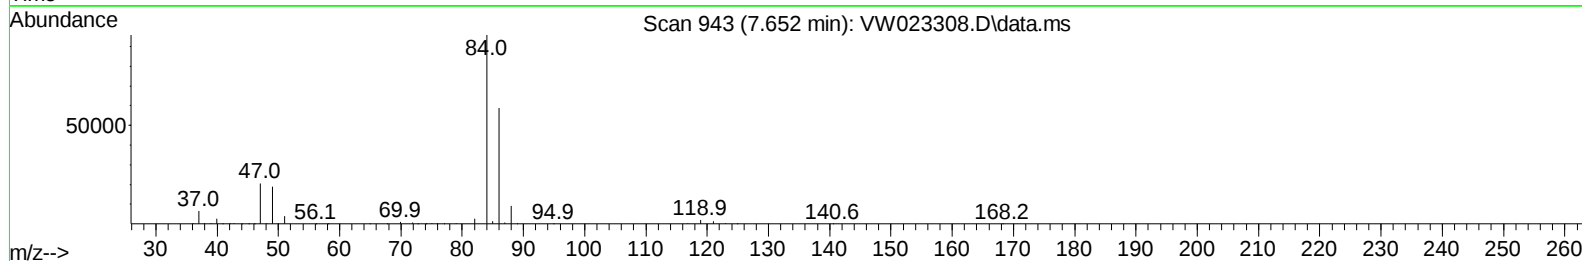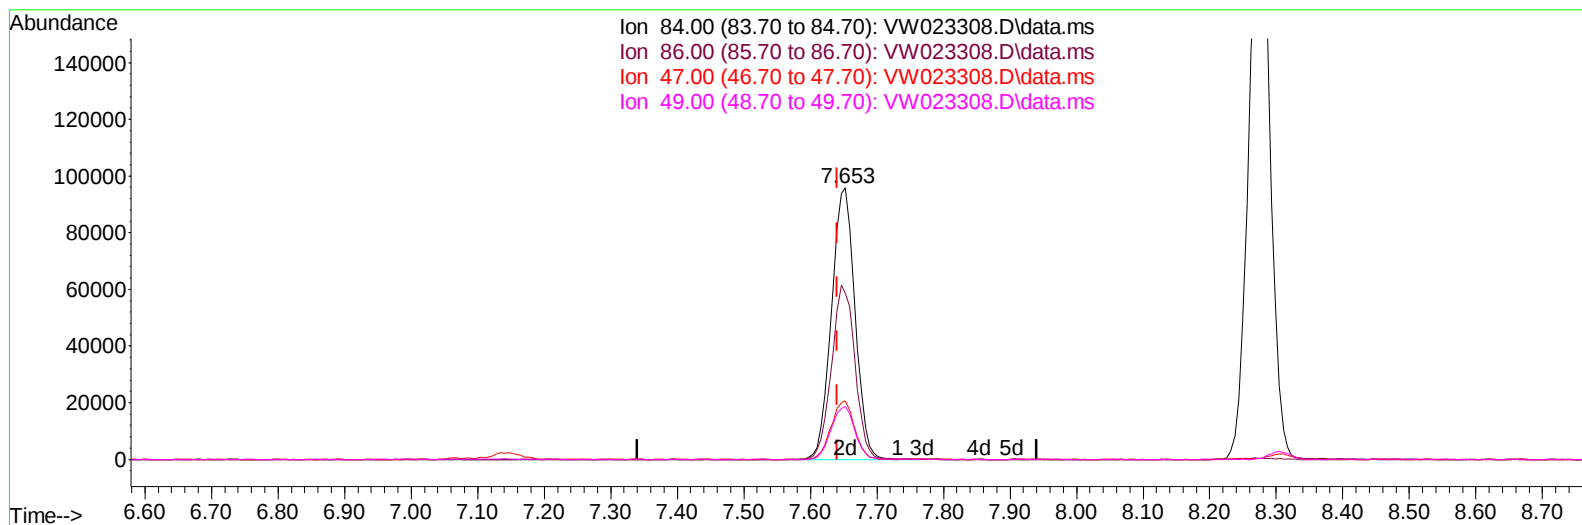

TIC: VW023308.D\data.ms

(24) Chloroform-d (S)

7.652min (+ 0.012) 23.01 ug/L m

response 233600

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.90	0.08#
47.00	43.20	0.04#
49.00	26.40	0.03#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023308.D
 Acq On : 25 May 2022 09:59
 Operator : SY/VA
 Sample : N2929-09
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:28:39 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	346583	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	342375	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	175597	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	131617	18.510	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	74.040%		
7) Chloroethane-d5	2.885	69	81659	17.652	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.600%		
11) 1,1-Dichloroethene-d2	4.019	63	140119	15.251	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.000%		
21) 2-Butanone-d5	7.079	46	56011	41.429	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	82.860%		
24) Chloroform-d	7.652	84	233600m	23.006	ug/L	0.01
Spiked Amount 25.000	Range 40 - 150		Recovery =	92.040%		
26) 1,2-Dichloroethane-d4	8.305	65	126391	22.695	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.760%		
32) Benzene-d6	8.274	84	457788	23.198	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.800%		
36) 1,2-Dichloropropane-d6	9.274	67	130800	23.596	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.400%		
41) Toluene-d8	10.323	98	434047	22.769	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	91.080%		
43) trans-1,3-Dichloroprop...	10.579	79	54290	21.270	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	85.080%		
47) 2-Hexanone-d5	10.926	63	44933	42.461	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	84.920%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	110944	21.472	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.880%		
66) 1,2-Dichlorobenzene-d4	13.853	152	152296	24.811	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.240%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023308.D
Acq On : 25 May 2022 09:59
Operator : SY/VA
Sample : N2929-09
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: May 26 01:28:39 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

