




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023319.D
 Acq On : 25 May 2022 14:23
 Operator : SY/VA
 Sample : N2996-19
 Misc : 4.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGW0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:31:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

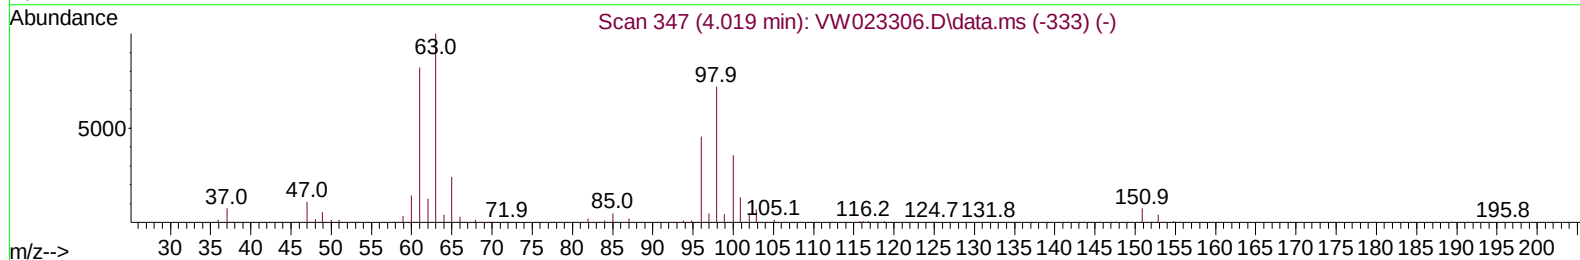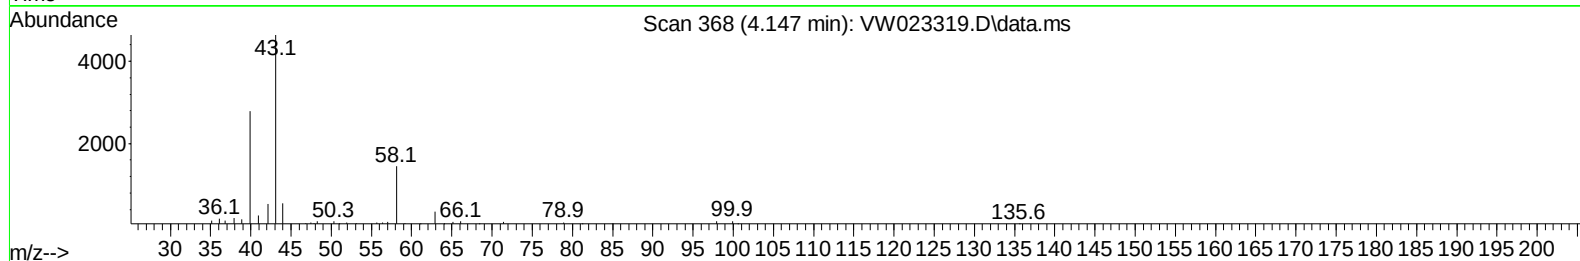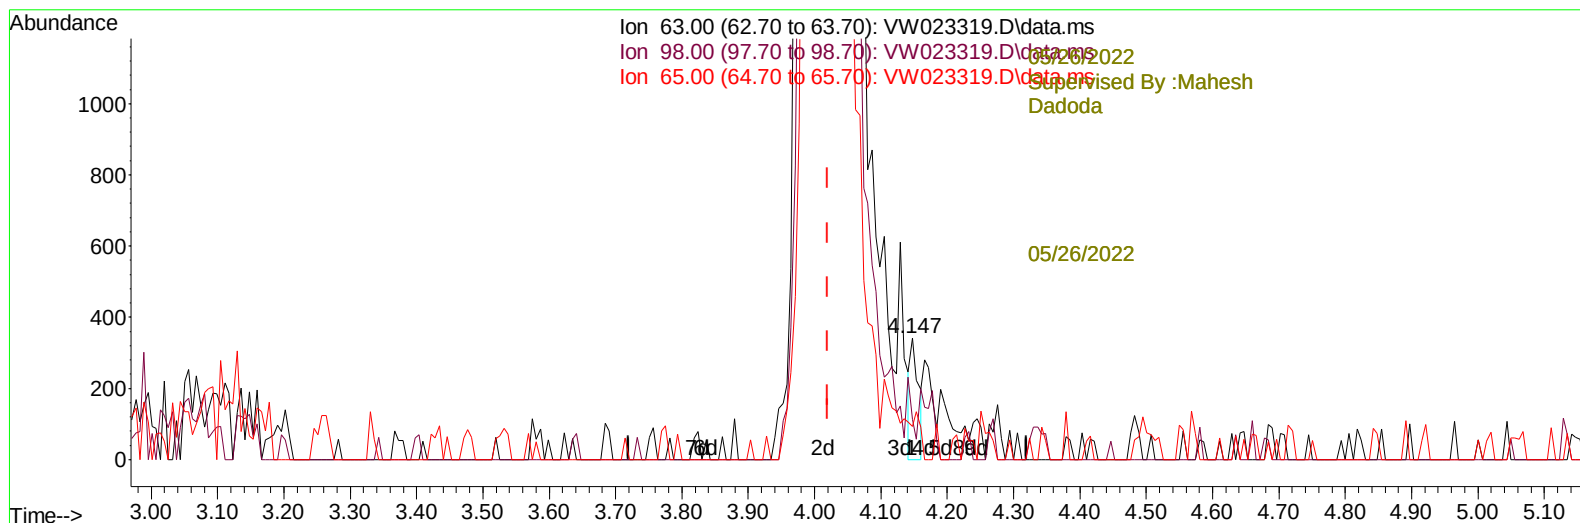

TIC: VW023319.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.147min (+ 0.128) 0.03 ug/L

response 279

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	52.69
65.00	23.30	29.75
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023319.D
 Acq On : 25 May 2022 14:23
 Operator : SY/VA
 Sample : N2996-19
 Misc : 4.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGW0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:31:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

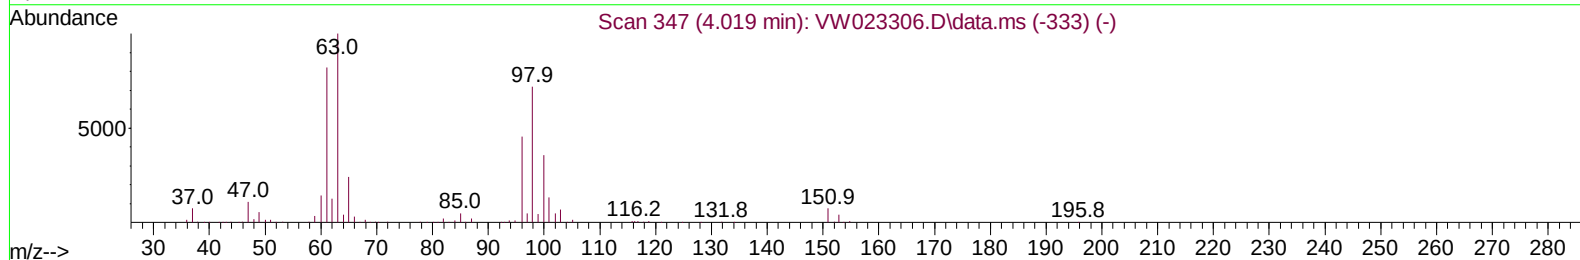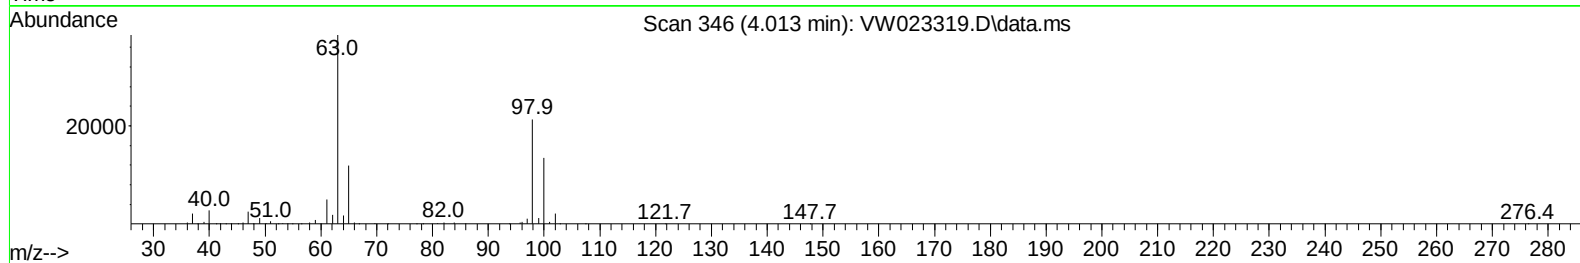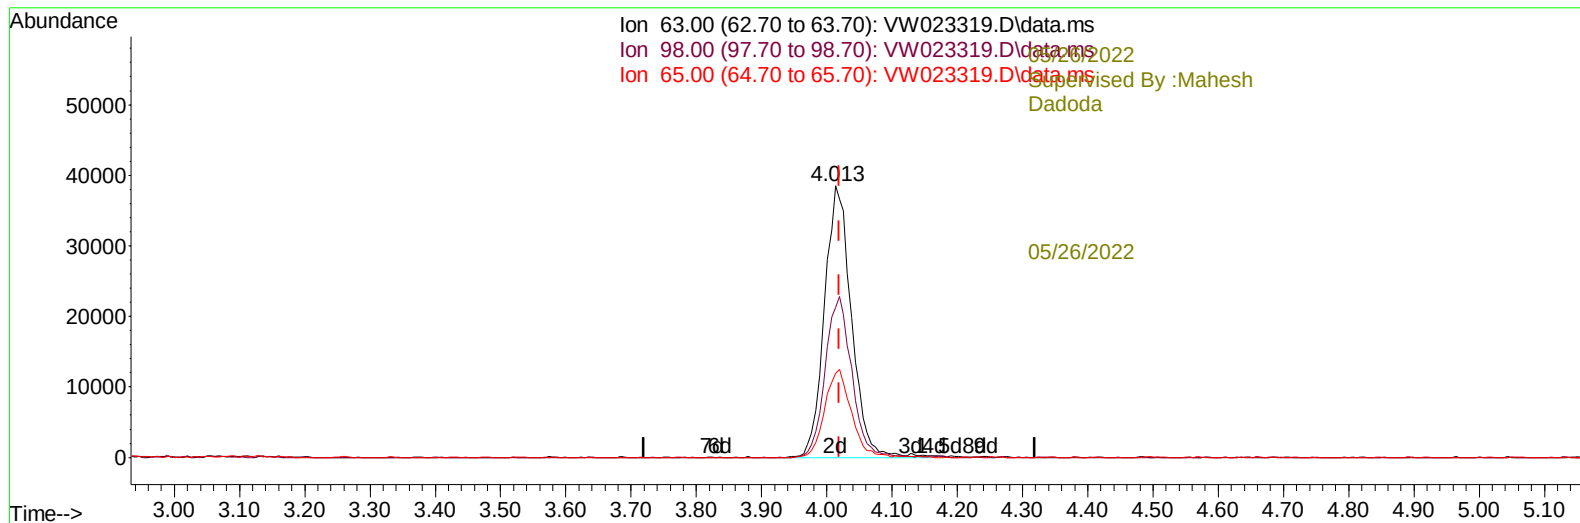

TIC: VW023319.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.013min (-0.006) 11.18 ug/L m

response 110983

Ion	Exp%	Act%
63.00	100.00	100.00
98.00	72.80	0.13#
65.00	23.30	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023319.D
 Acq On : 25 May 2022 14:23
 Operator : SY/VA
 Sample : N2996-19
 Misc : 4.62g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGW0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:31:48 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----05/26/2022							
Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		374445	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117		381830	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		193779	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		106440	13.855	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150		Recovery =	55.440%		
7) Chloroethane-d5	2.879	69		71414	14.289	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150		Recovery =	57.160%		
11) 1,1-Dichloroethene-d2	4.013	63		110983m	11.181	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110		Recovery =	44.720%#		
21) 2-Butanone-d5	7.074	46		88783	60.783	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135		Recovery =	121.560%		
24) Chloroform-d	7.647	84		227323	20.722	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150		Recovery =	82.880%		
26) 1,2-Dichloroethane-d4	8.305	65		138774	23.064	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130		Recovery =	92.240%		
32) Benzene-d6	8.275	84		407860	18.532	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135		Recovery =	74.120%		
36) 1,2-Dichloropropane-d6	9.274	67		130301	21.077	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120		Recovery =	84.320%		
41) Toluene-d8	10.323	98		375401	17.657	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130		Recovery =	70.640%		
43) trans-1,3-Dichloroprop...	10.579	79		58455	20.535	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135		Recovery =	82.160%		
47) 2-Hexanone-d5	10.920	63		78438	66.463	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135		Recovery =	132.920%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		154726	26.852	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120		Recovery =	107.400%		
66) 1,2-Dichlorobenzene-d4	13.853	152		155732	22.990	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120		Recovery =	91.960%		
Target Compounds							
13) Acetone	4.117	43		24837	22.712	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023319.D
Acq On : 25 May 2022 14:23
Operator : SY/VA
Sample : N2996-19
Misc : 4.62g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGW0

Manual IntegrationsAPPROVED

Quant Time: May 26 01:31:48 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

