




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023328.D
Acq On : 25 May 2022 18:01
Operator : SY/VA
Sample : N2848-05
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:33:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

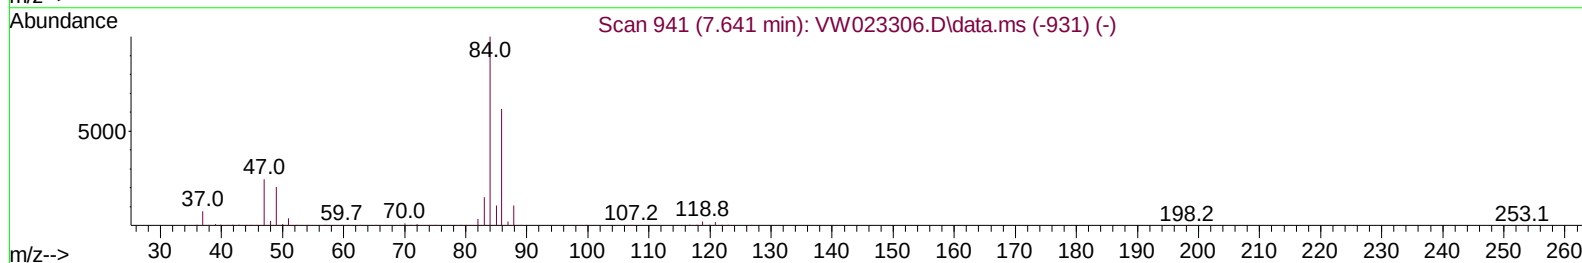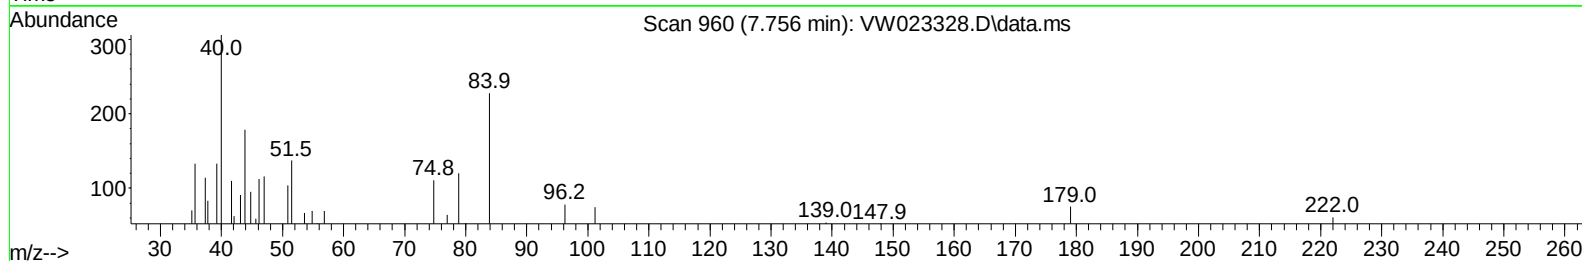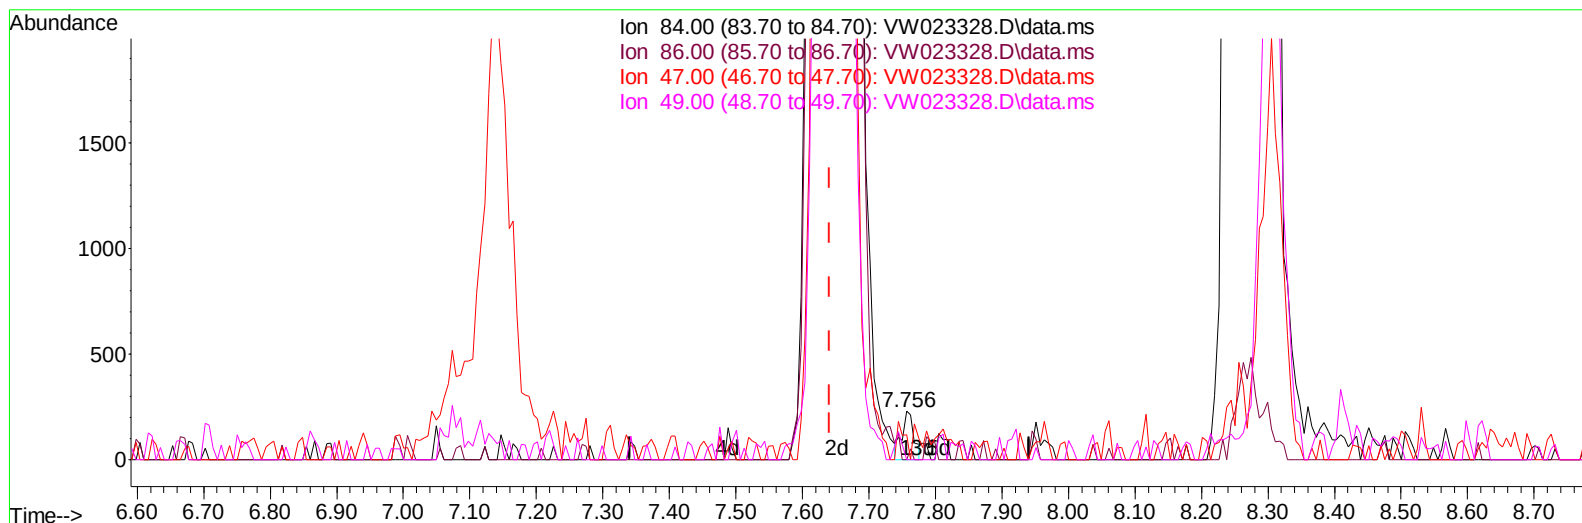

TIC: VW023328.D\data.ms

(24) Chloroform-d (S)

7.756min (+ 0.116) 0.03 ug/L

response 286

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.90	65.38
47.00	43.20	52.45
49.00	26.40	33.92




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023328.D
Acq On : 25 May 2022 18:01
Operator : SY/VA
Sample : N2848-05
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:33:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

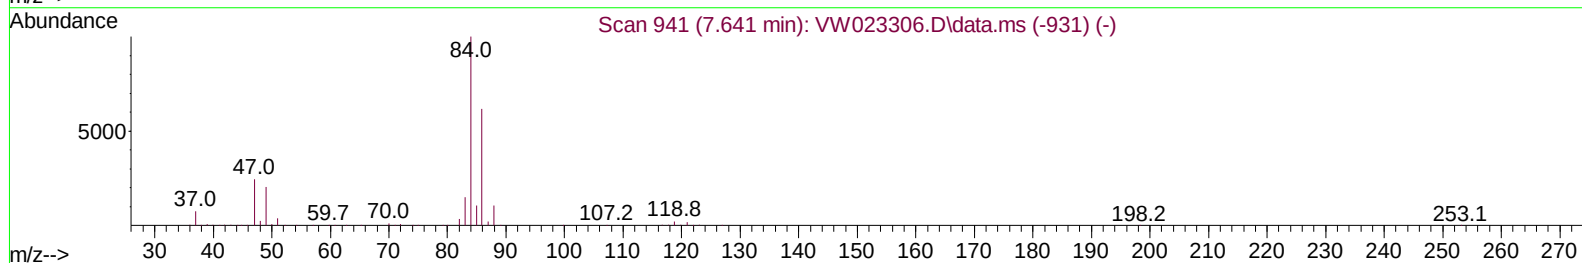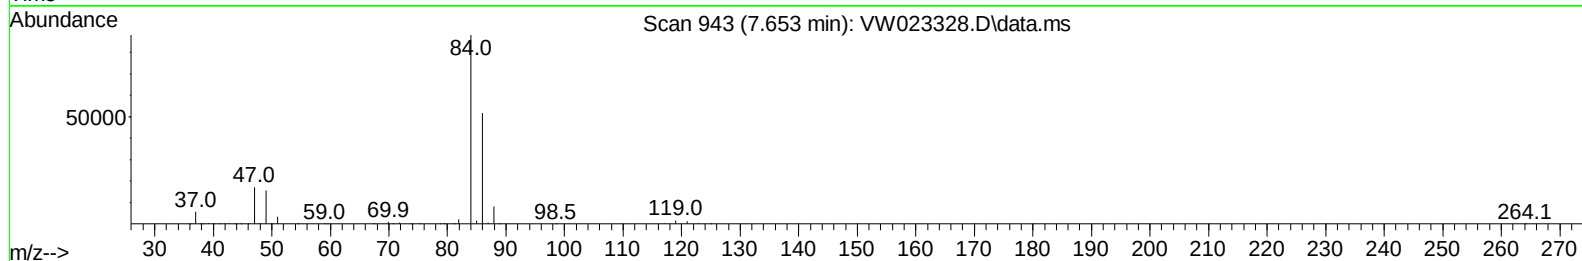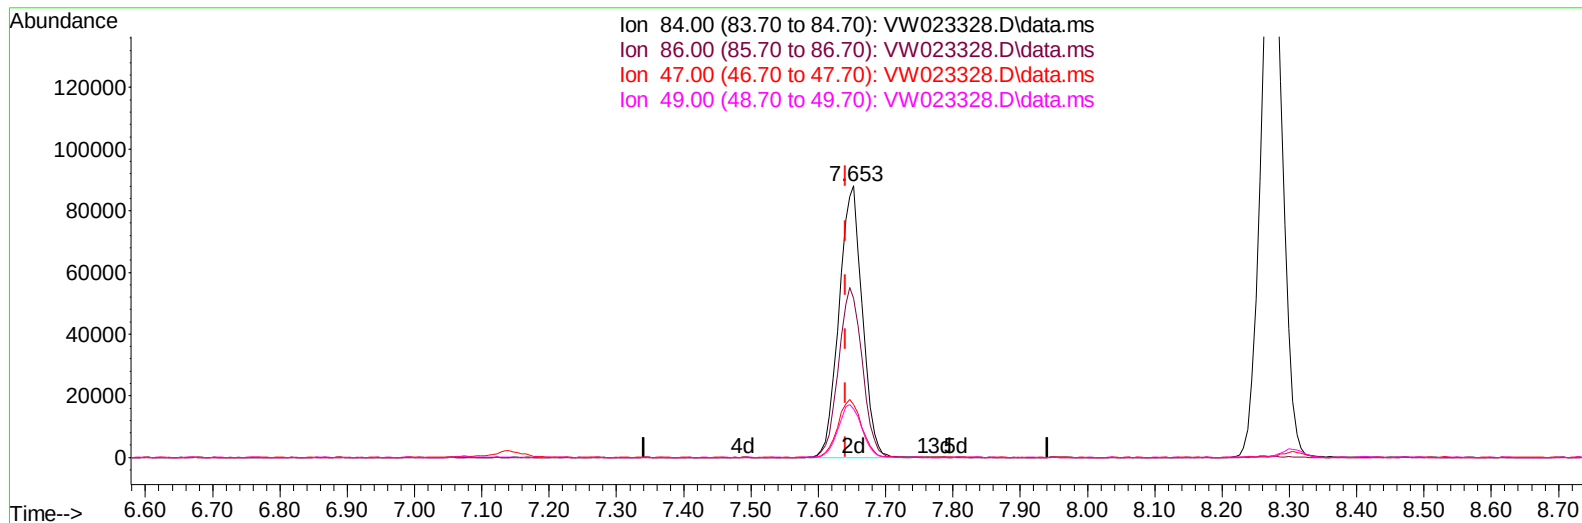

TIC: VW023328.D\data.ms

(24) Chloroform-d (S)

7.653min (+ 0.012) 25.24 ug/L m

response 210829

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	61.90	0.09#
47.00	43.20	0.07#
49.00	26.40	0.05#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023328.D
 Acq On : 25 May 2022 18:01
 Operator : SY/VA
 Sample : N2848-05
 Misc : 5.02g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:33:24 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	285066	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	290347	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	140120	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	122942	21.021	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.080%	
7) Chloroethane-d5	2.879	69	76067	19.992	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	79.960%	
11) 1,1-Dichloroethene-d2	4.013	63	121833	16.122	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	64.480%	
21) 2-Butanone-d5	7.080	46	56136	50.482	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.960%	
24) Chloroform-d	7.653	84	210829m	25.244	ug/L	0.01
Spiked Amount 25.000	Range 40	- 150	Recovery	=	100.960%	
26) 1,2-Dichloroethane-d4	8.305	65	115623	25.242	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	100.960%	
32) Benzene-d6	8.275	84	409085	24.444	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	97.760%	
36) 1,2-Dichloropropane-d6	9.268	67	119447	25.409	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	101.640%	
41) Toluene-d8	10.323	98	387875	23.993	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	95.960%	
43) trans-1,3-Dichloroprop...	10.579	79	48901	22.592	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.360%	
47) 2-Hexanone-d5	10.921	63	44090	49.130	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	98.260%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	106192	24.235	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	96.960%	
66) 1,2-Dichlorobenzene-d4	13.853	152	131041	26.753	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	107.000%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023328.D
Acq On : 25 May 2022 18:01
Operator : SY/VA
Sample : N2848-05
Misc : 5.02g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:33:24 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

