




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023342.D
 Acq On : 26 May 2022 00:40
 Operator : SY/VA
 Sample : N2995-08
 Misc : 4.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR1

Manual IntegrationsAPPROVED

Quant Time: May 26 05:16:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

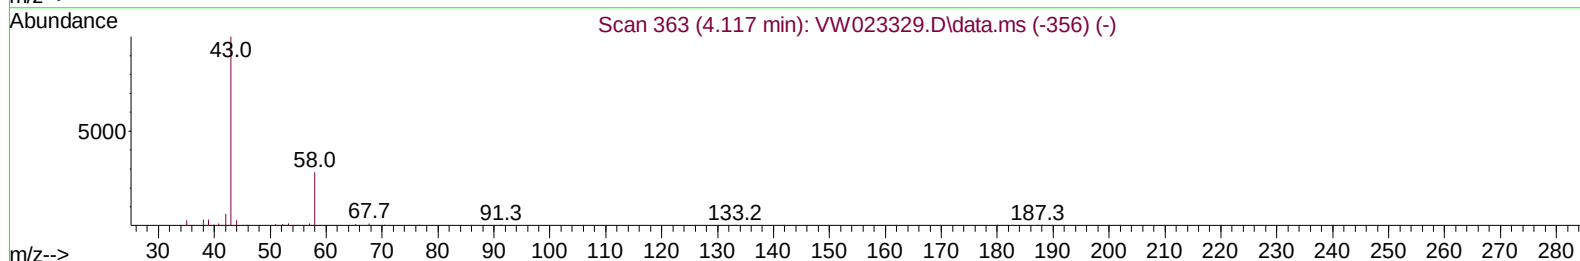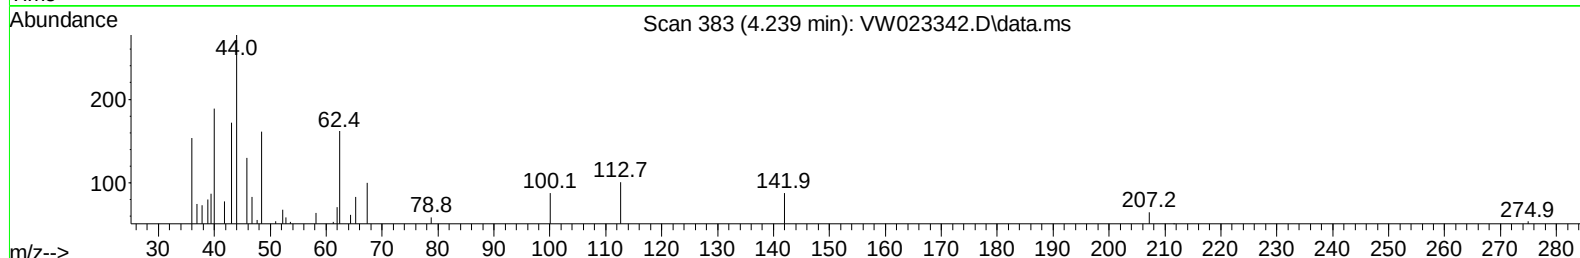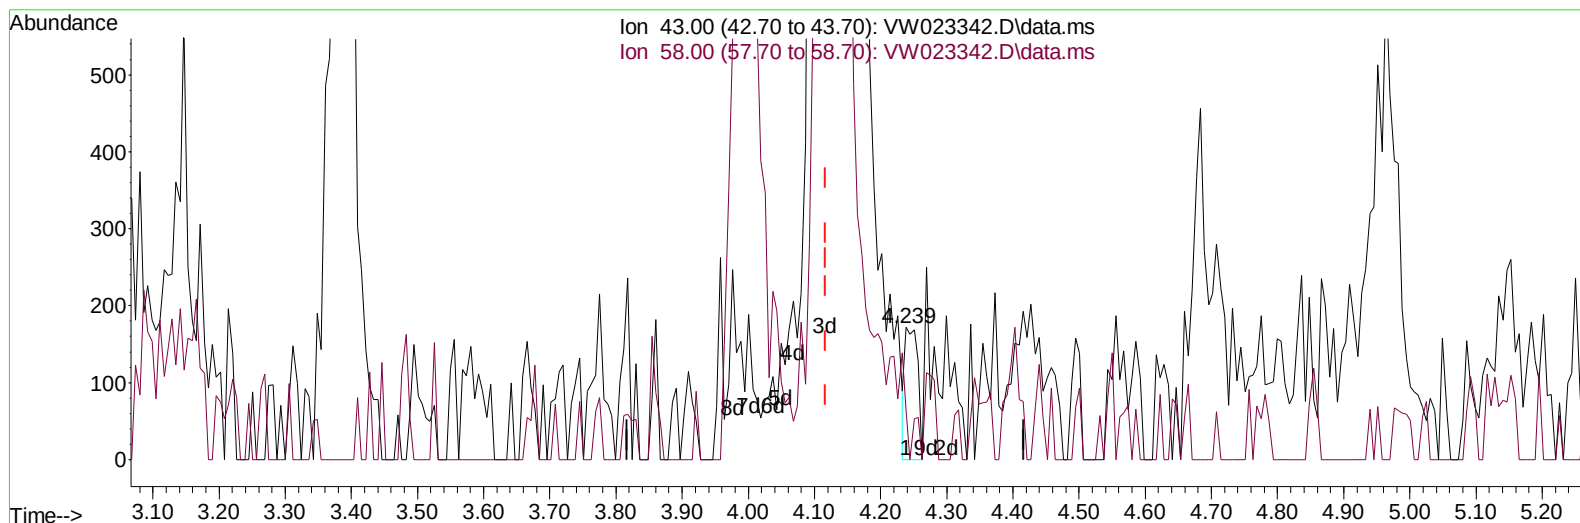

TIC: VW023342.D\data.ms

(13) Acetone (T)

4.239min (+ 0.122) 0.29 ug/L

response 231

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	32.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023342.D
 Acq On : 26 May 2022 00:40
 Operator : SY/VA
 Sample : N2995-08
 Misc : 4.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR1

Manual IntegrationsAPPROVED

Quant Time: May 26 05:16:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

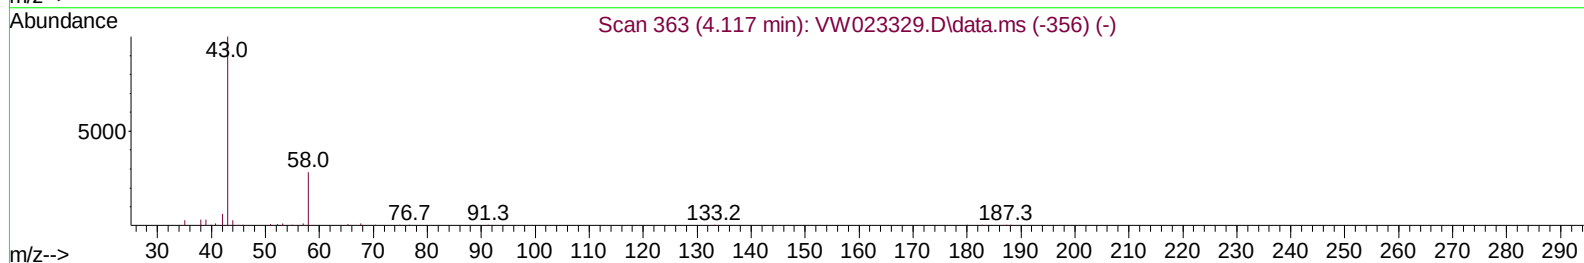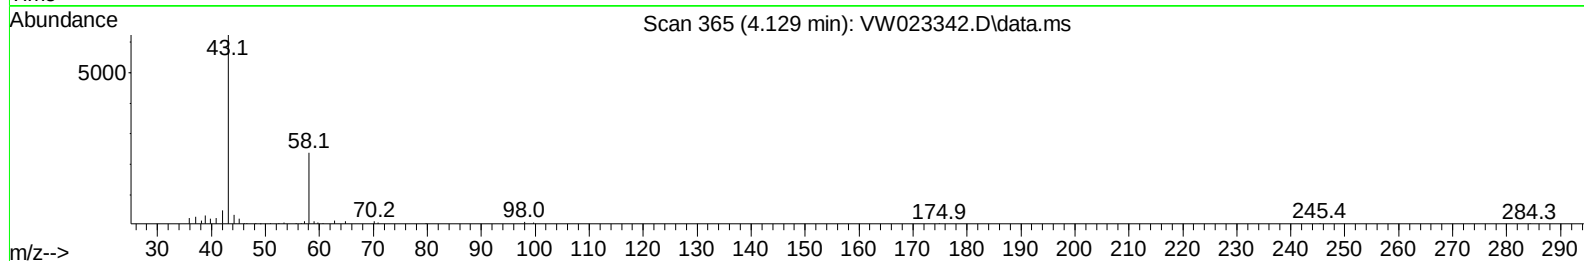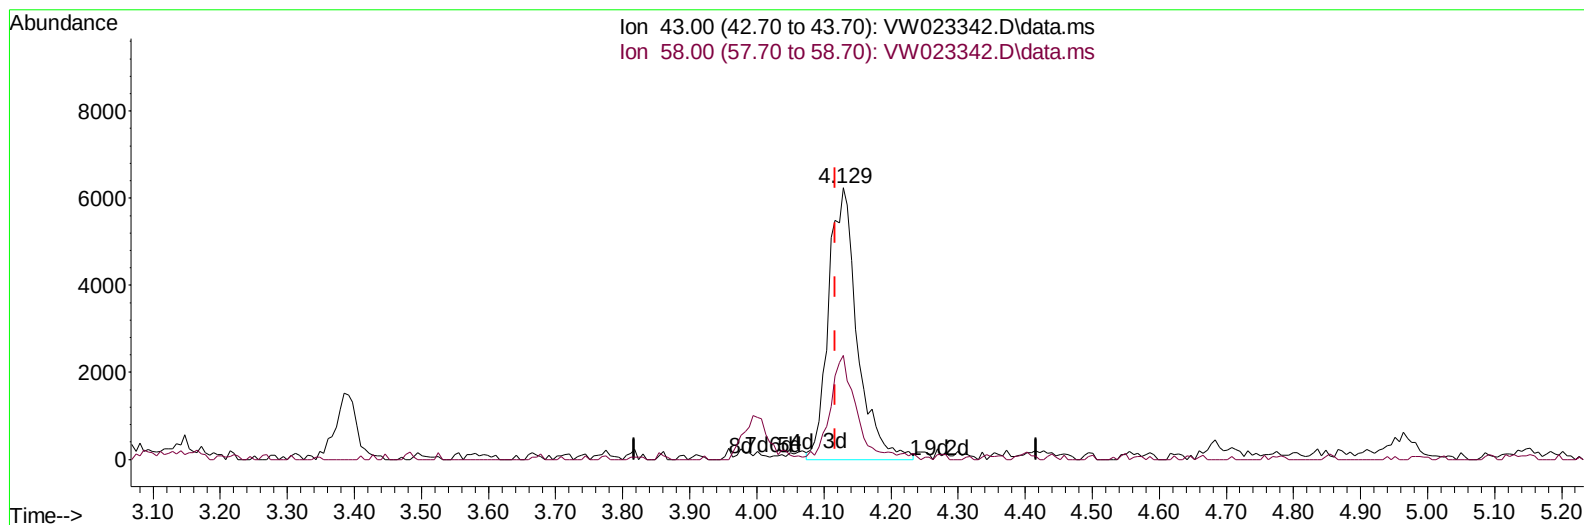

TIC: VW023342.D\data.ms

(13) Acetone (T)

4.129min (+ 0.012) 23.08 ug/L m

response 18505

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	32.00	0.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023342.D
 Acq On : 26 May 2022 00:40
 Operator : SY/VA
 Sample : N2995-08
 Misc : 4.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 05:16:56 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	274528	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	252439	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	93844	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	84677	15.034	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	60.120%	
7) Chloroethane-d5	2.885	69	57910	15.804	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.200%	
11) 1,1-Dichloroethene-d2	4.019	63	91049	12.511	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	50.040%	
21) 2-Butanone-d5	7.080	46	71782	67.030	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	134.060%	
24) Chloroform-d	7.653	84	194623	24.198	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	96.800%	
26) 1,2-Dichloroethane-d4	8.305	65	117884	26.723	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	106.880%	
32) Benzene-d6	8.274	84	328456	22.574	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	90.280%	
36) 1,2-Dichloropropane-d6	9.274	67	108268	26.489	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	105.960%	
41) Toluene-d8	10.323	98	274160	19.505	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	78.040%	
43) trans-1,3-Dichloroprop...	10.579	79	42887	22.789	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	91.160%	
47) 2-Hexanone-d5	10.920	63	55036	70.536	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	141.080%#	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	115914	30.427	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	121.720%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	76555	23.337	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	93.360%	
Target Compounds						
13) Acetone	4.129	43	18505m	23.080	ug/L	
42) Toluene	10.390	91	31758	1.906	ug/L	100
62) 1,3,5-Trimethylbenzene	12.938	105	49406	6.908	ug/L	96
63) 1,2,4-Trimethylbenzene	13.249	105	27600	2.570	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023342.D
Acq On : 26 May 2022 00:40
Operator : SY/VA
Sample : N2995-08
Misc : 4.03g/10mL/MSVOA_W/SoIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGR1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 05:16:56 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 04:46:06 2022
Response via : Initial Calibration

