

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023320.D
 Acq On : 25 May 2022 14:47
 Operator : SY/VA
 Sample : N2996-20
 Misc : 3.48g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGW1

Quant Time: May 26 01:31:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	334002	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	323516	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	137987	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	101261	14.777	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	59.120%
7) Chloroethane-d5	2.885	69	67060	15.042	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.160%
11) 1,1-Dichloroethene-d2	4.019	63	103964	11.742	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.960%
21) 2-Butanone-d5	7.074	46	84117	64.562	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	129.120%
24) Chloroform-d	7.647	84	215402	22.012	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.040%
26) 1,2-Dichloroethane-d4	8.305	65	133287	24.835	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.320%
32) Benzene-d6	8.275	84	376498	20.191	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	80.760%
36) 1,2-Dichloropropane-d6	9.274	67	123153	23.511	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.040%
41) Toluene-d8	10.323	98	348097	19.324	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	77.280%
43) trans-1,3-Dichloroprop...	10.579	79	50135	20.787	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	83.160%
47) 2-Hexanone-d5	10.920	63	68548	68.552	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	137.100%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	137398	28.142	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	112.560%
66) 1,2-Dichlorobenzene-d4	13.853	152	111005	23.013	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.040%
Target Compounds					Qvalue	
13) Acetone	4.129	43	13749	14.095	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023320.D
Acq On : 25 May 2022 14:47
Operator : SY/VA
Sample : N2996-20
Misc : 3.48g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGW1

Quant Time: May 26 01:31:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

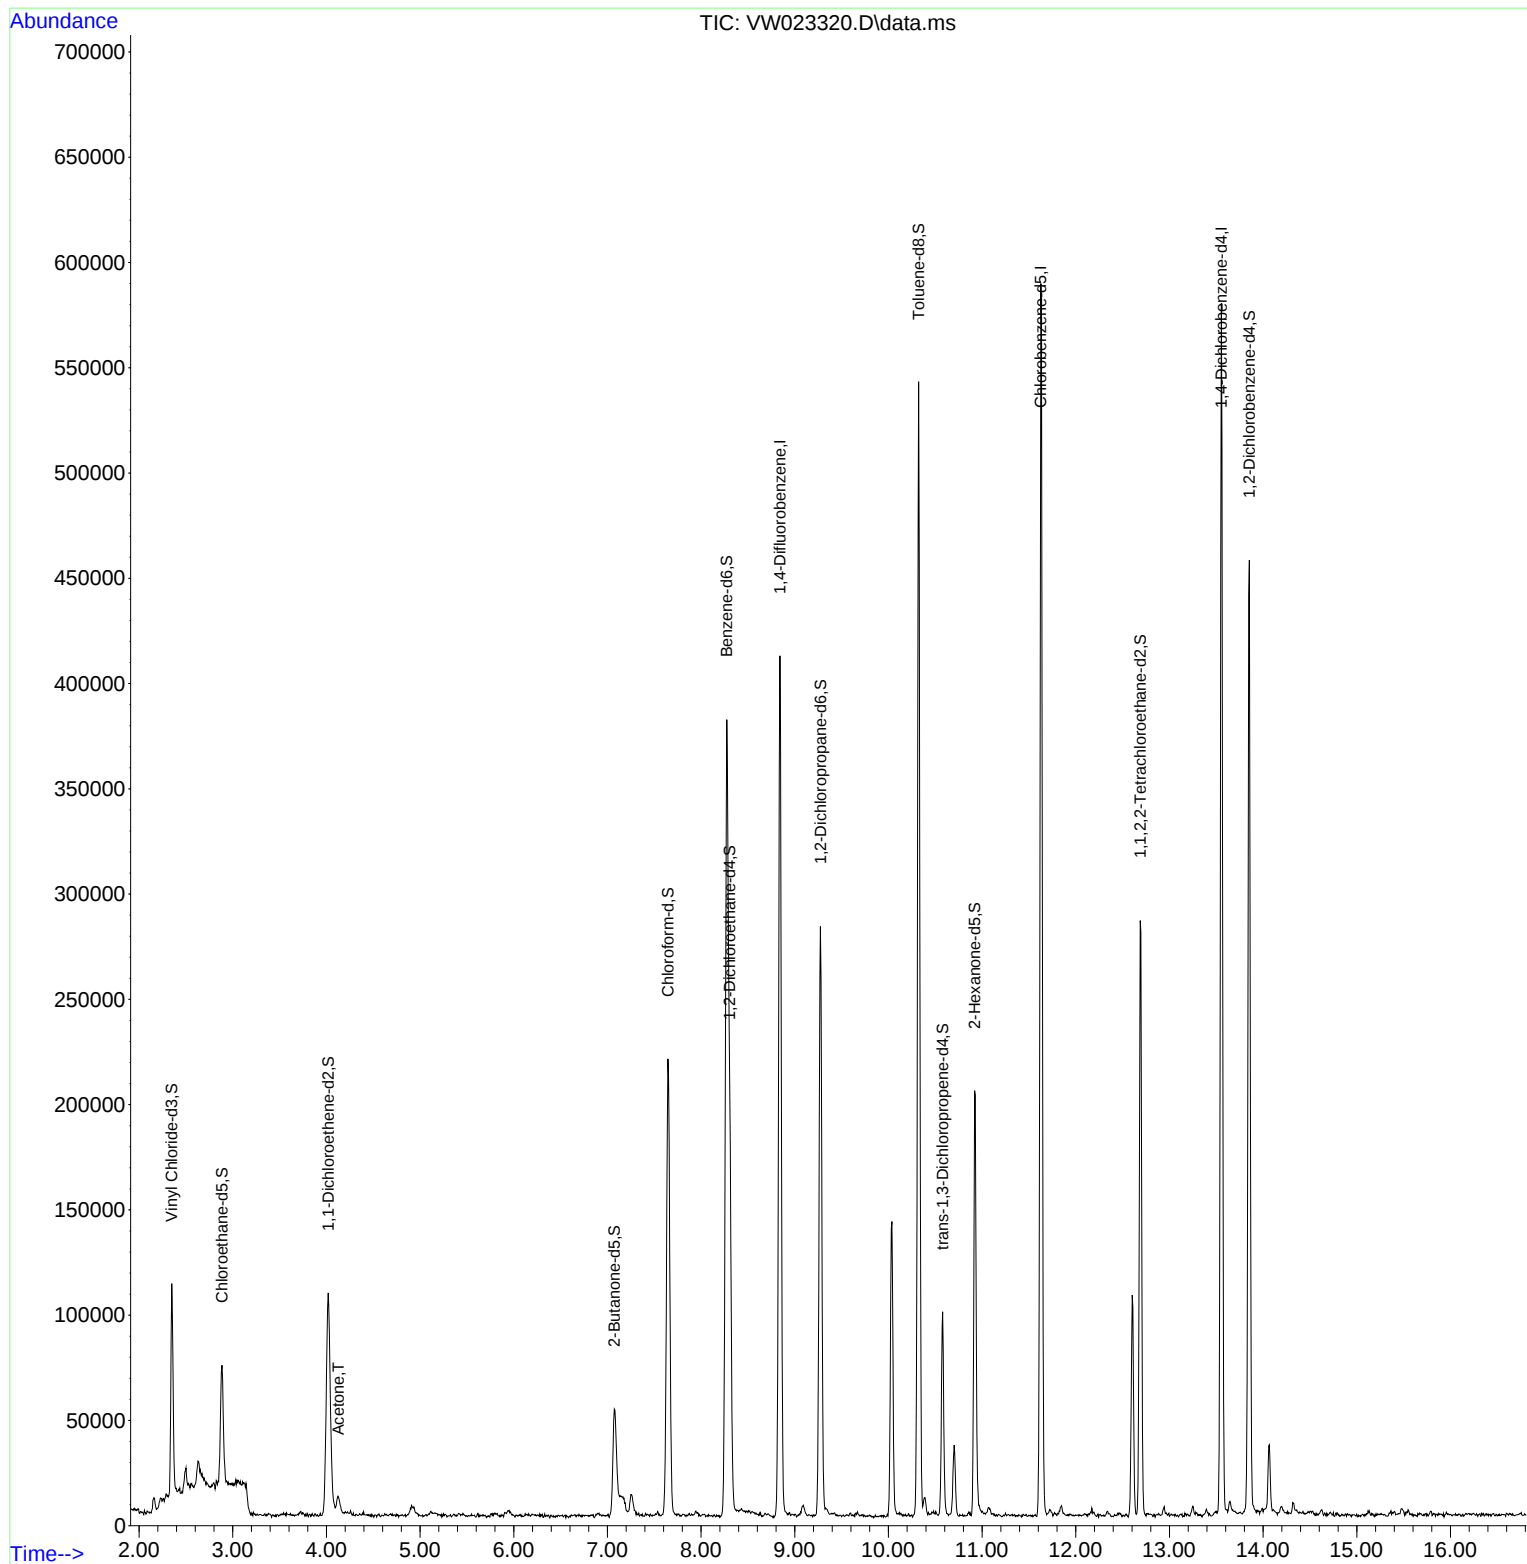

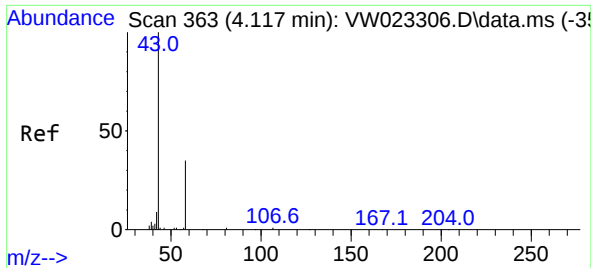

#13
Acetone
Concen: 14.095 ug/L
RT: 4.129 min Scan# 30
Delta R.T. 0.012 min
Lab File: VW023320.D
Acq: 25 May 2022 14:47

Instrument :
MSVOA_W
ClientSampleId :
GBGW1

Tgt Ion: 43 Resp: 13749
Ion Ratio Lower Upper
43 100
58 35.1 0.0 64.0

