

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023325.D
 Acq On : 25 May 2022 16:48
 Operator : SY/VA
 Sample : N2995-20
 Misc : 5.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGS1

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:32:50 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	244015	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	250596	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	123095	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	79322	15.844	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.360%		
7) Chloroethane-d5	2.885	69	59257	18.194	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.760%		
11) 1,1-Dichloroethene-d2	4.019	63	80881	12.503	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	50.000%		
21) 2-Butanone-d5	7.080	46	79619	83.646	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	167.300%#		
24) Chloroform-d	7.647	84	168248	23.534	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	94.120%		
26) 1,2-Dichloroethane-d4	8.305	65	106221m	27.090	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	108.360%		
32) Benzene-d6	8.275	84	294383	20.381	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	81.520%		
36) 1,2-Dichloropropane-d6	9.274	67	95969	23.653	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	94.600%		
41) Toluene-d8	10.323	98	268187	19.221	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	76.880%		
43) trans-1,3-Dichloroprop...	10.579	79	42772	22.895	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.560%		
47) 2-Hexanone-d5	10.927	63	65138	84.098	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	168.200%#		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	130624	34.540	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	138.160%#		
66) 1,2-Dichlorobenzene-d4	13.853	152	109142	25.364	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	101.440%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	10256	14.391	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023325.D
Acq On : 25 May 2022 16:48
Operator : SY/VA
Sample : N2995-20
Misc : 5.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGS1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022


Quant Time: May 26 01:32:50 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

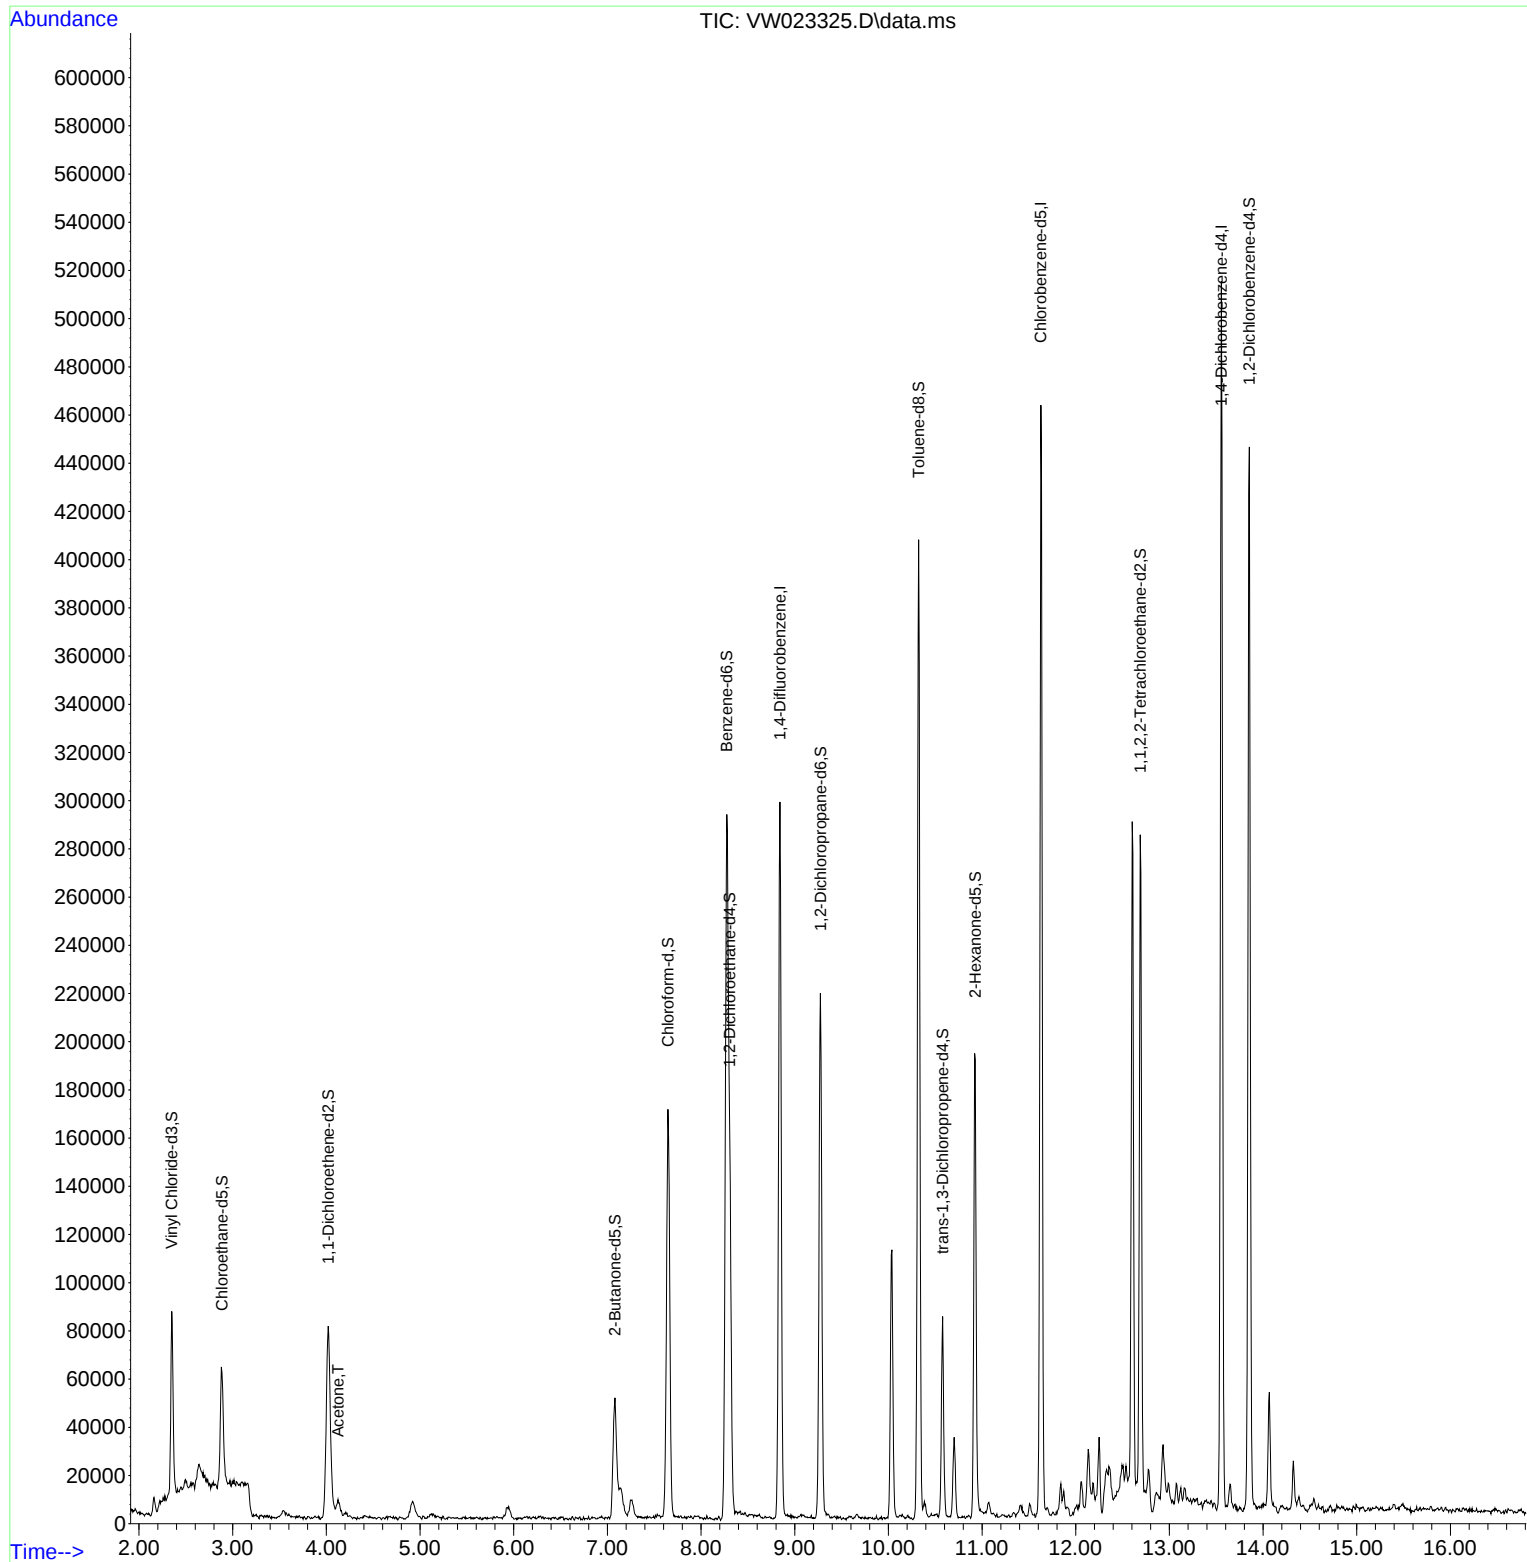

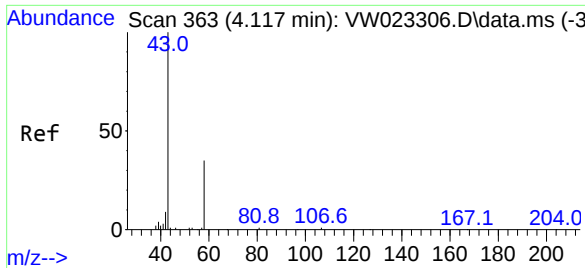

#13
 Acetone
 Concen: 14.391 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW023325.D
 Acq: 25 May 2022 16:48

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGS1

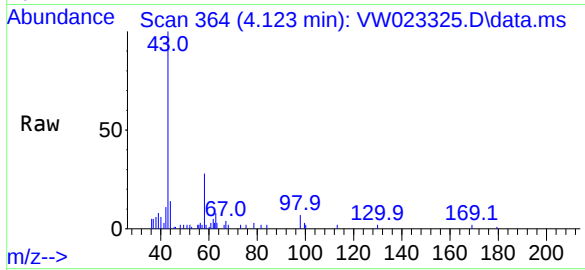

Tgt Ion: 43 Resp: 10250
 Ion Ratio Lower Upper
 43 100
 58 32.1 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

