

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023326.D
 Acq On : 25 May 2022 17:12
 Operator : SY/VA
 Sample : N2995-22
 Misc : 4.76g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGS3

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 01:33:03 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 01:27:55 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	358766	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	365703	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	182612	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	102895	13.979	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.920%
7) Chloroethane-d5	2.879	69	69443	14.502	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.000%
11) 1,1-Dichloroethene-d2	4.019	63	104157	10.952	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	43.800%#
21) 2-Butanone-d5	7.074	46	80438	57.477	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.960%
24) Chloroform-d	7.647	84	217434	20.686	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	82.760%
26) 1,2-Dichloroethane-d4	8.305	65	130450m	22.628	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.520%
32) Benzene-d6	8.275	84	394010	18.692	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	74.760%
36) 1,2-Dichloropropane-d6	9.268	67	126964	21.443	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	85.760%
41) Toluene-d8	10.323	98	354947	17.432	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	69.720%
43) trans-1,3-Dichloroprop...	10.579	79	52903	19.405	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.600%
47) 2-Hexanone-d5	10.921	63	66460	58.797	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.600%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	145241	26.317	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	145231	22.751	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.000%
Target Compounds						Qvalue
13) Acetone	4.123	43	15122	14.432	ug/L	97
20) cis-1,2-Dichloroethene	7.171	96	14618	2.632	ug/L #	95
34) Trichloroethene	9.092	95	4925	0.831	ug/L	88
46) Tetrachloroethene	10.860	164	2568	0.577	ug/L	77

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023326.D
Acq On : 25 May 2022 17:12
Operator : SY/VA
Sample : N2995-22
Misc : 4.76g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGS3

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022


Quant Time: May 26 01:33:03 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 01:27:55 2022
Response via : Initial Calibration

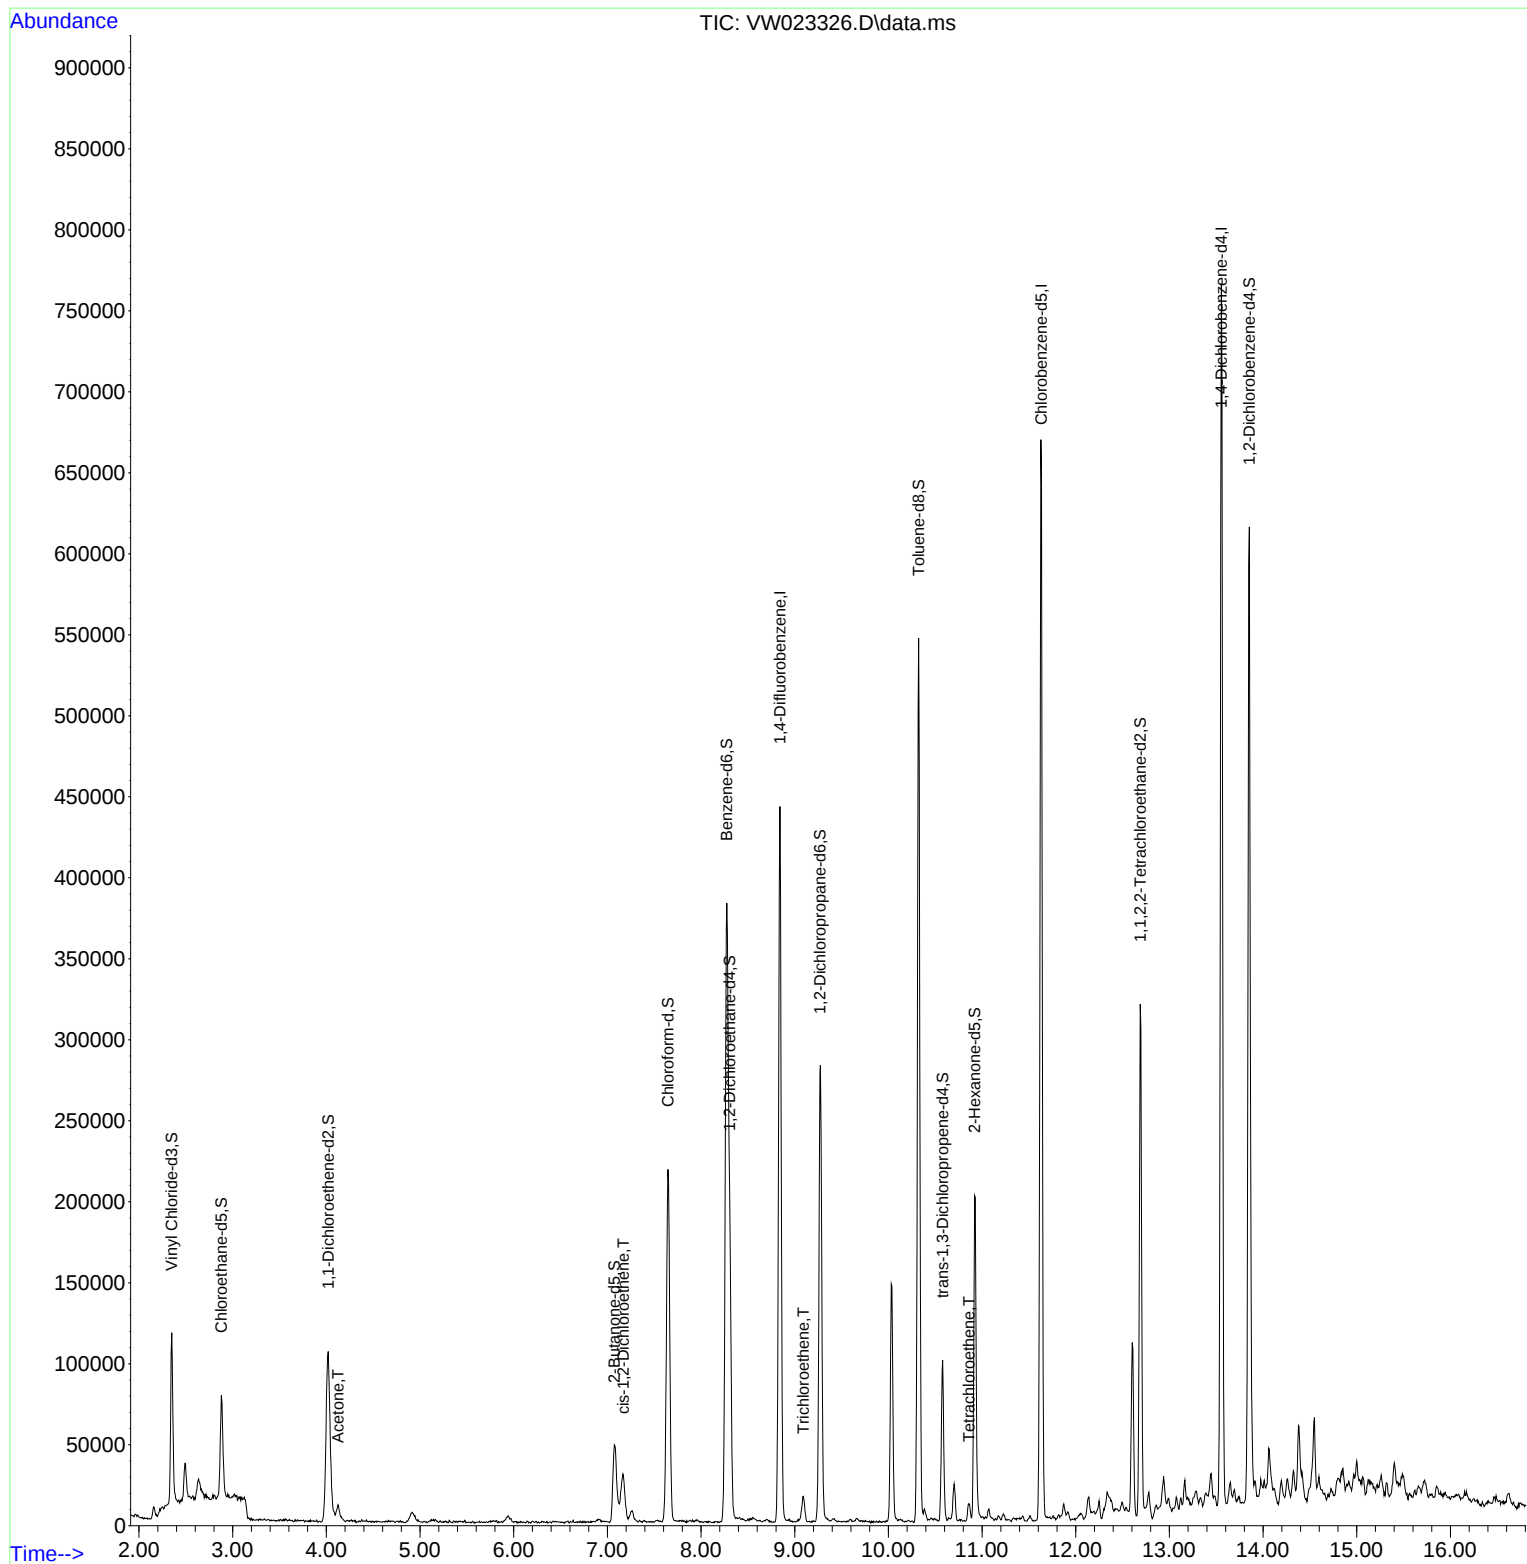

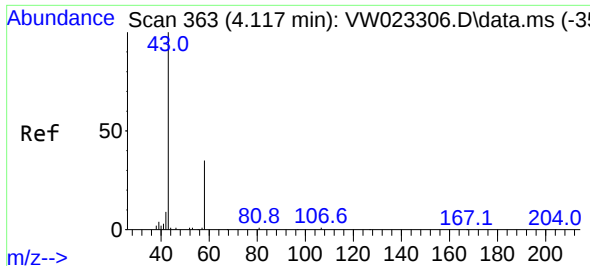

#13
Acetone
Concen: 14.432 ug/L
RT: 4.123 min Scan# 364
Delta R.T. 0.006 min
Lab File: VW023326.D
Acq: 25 May 2022 17:12




Instrument :
MSVOA_W
ClientSampleId :
GBGS3

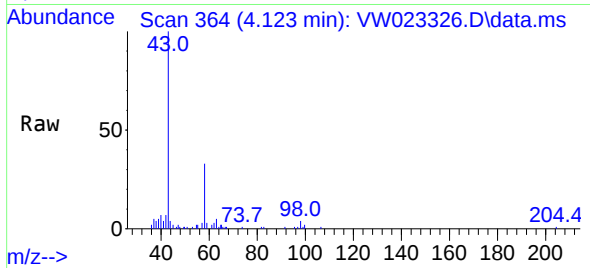


Tgt Ion: 43 Resp: 1512
Ion Ratio Lower Upper
43 100
58 30.3 0.0 64.0

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

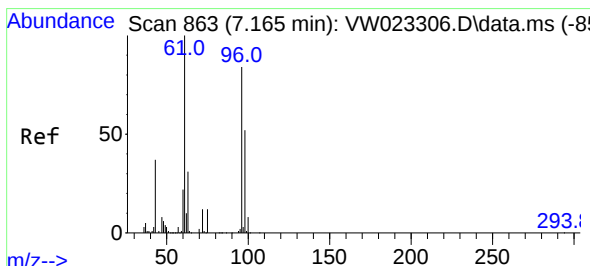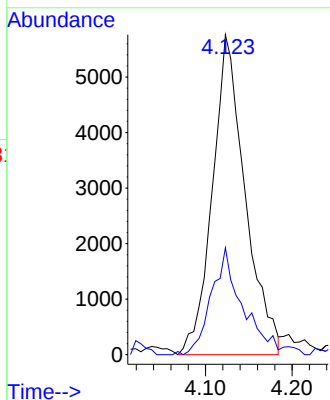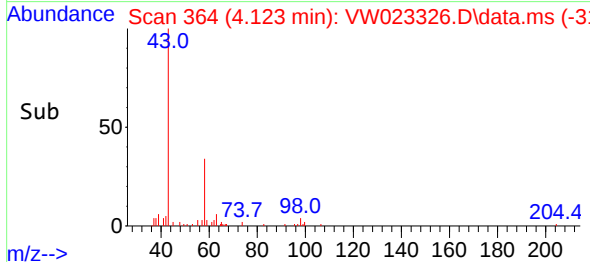


#20
cis-1,2-Dichloroethene
Concen: 2.632 ug/L
RT: 7.171 min Scan# 864
Delta R.T. 0.006 min
Lab File: VW023326.D
Acq: 25 May 2022 17:12

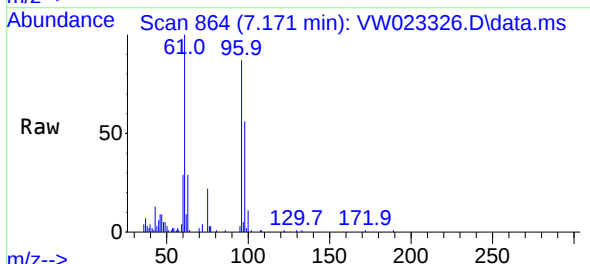


Tgt Ion: 96 Resp: 14618
Ion Ratio Lower Upper
96 100
61 114.8 84.2 156.4
68 0.0 0.1 0.1#

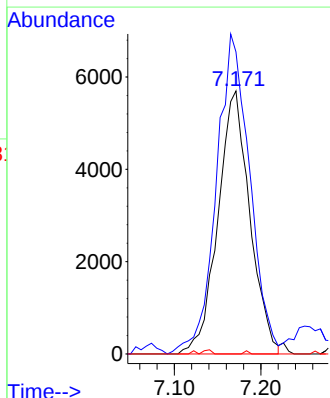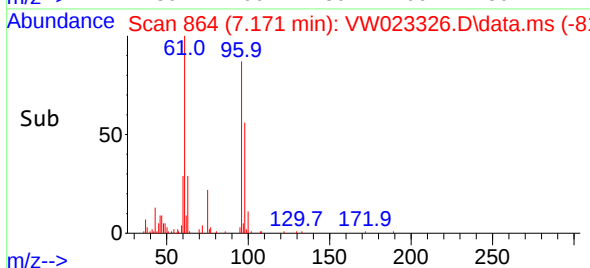

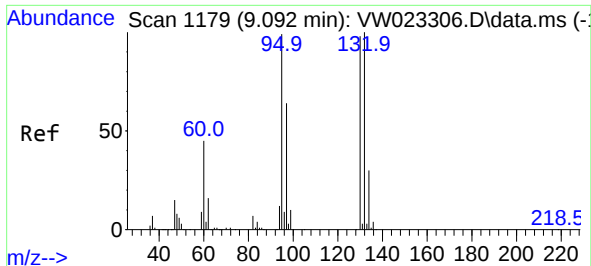

#34
Trichloroethene
Concen: 0.831 ug/L
RT: 9.092 min Scan# 1179
Delta R.T. -0.000 min
Lab File: VW023326.D
Acq: 25 May 2022 17:12

Instrument :
MSVOA_W
ClientSampleId :
GBGS3



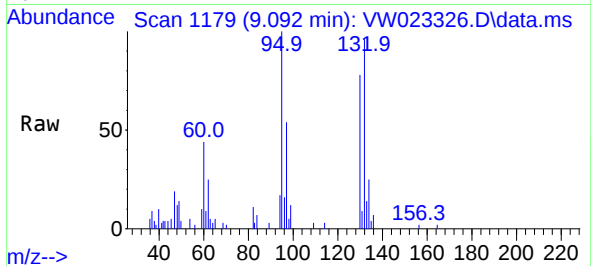


Tgt Ion: 95 Resp: 492


Ion	Ratio	Lower	Upper
95	100		
97	54.2	46.1	85.7
132	95.9	66.9	124.3
130	77.6	69.5	129.1

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

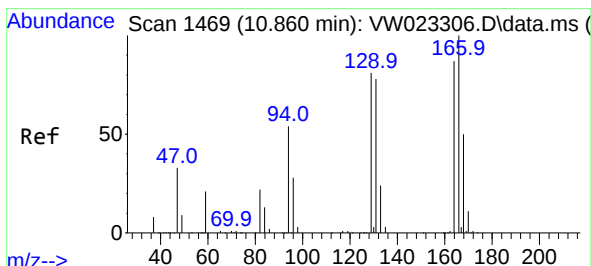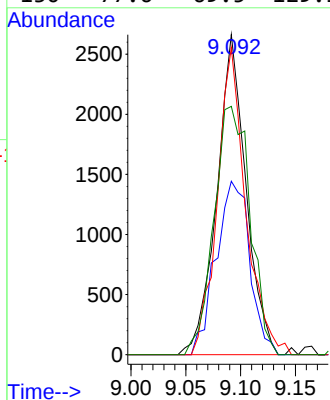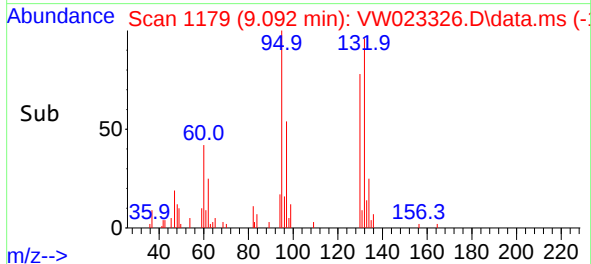

#46
Tetrachloroethene
Concen: 0.577 ug/L
RT: 10.860 min Scan# 1469
Delta R.T. -0.000 min
Lab File: VW023326.D
Acq: 25 May 2022 17:12

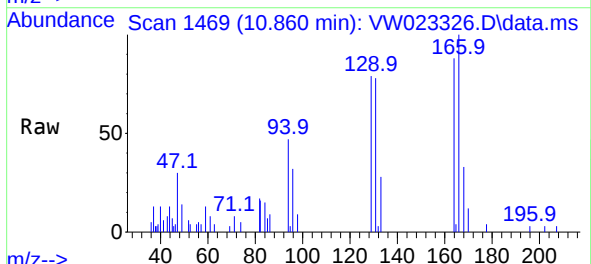

Tgt Ion:164 Resp: 2568

Ion	Ratio	Lower	Upper
164	100		
129	85.0	76.9	142.7
131	84.5	75.1	139.5
166	108.2	96.0	178.2

