

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023331.D
 Acq On : 25 May 2022 20:15
 Operator : SY/VA
 Sample : N2997-01
 Misc : 4.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGW4

Manual Integrations
 APPROVED

Reviewed By : Semsettin Yesilyurt 05/26/2022
 Supervised By : Mahesh Dadoda 05/26/2022

Quant Time: May 26 05:14:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	315109	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	324376	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	169733	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	101429	15.689	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.760%
7) Chloroethane-d5	2.879	69	67388	16.022	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.080%
11) 1,1-Dichloroethene-d2	4.013	63	100349	12.013	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	48.040%
21) 2-Butanone-d5	7.080	46	89433	72.758	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	145.520%#
24) Chloroform-d	7.647	84	217297	23.537	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.160%
26) 1,2-Dichloroethane-d4	8.305	65	134576m	26.578	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	106.320%
32) Benzene-d6	8.275	84	380053	20.327	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.320%
36) 1,2-Dichloropropane-d6	9.275	67	126105	24.011	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.040%
41) Toluene-d8	10.323	98	353677	19.582	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	78.320%
43) trans-1,3-Dichloroprop...	10.579	79	54007	22.333	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.320%
47) 2-Hexanone-d5	10.921	63	72754	72.566	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	145.140%#
56) 1,1,2,2-Tetrachloroeth...	12.689	84	155685	31.804	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	127.200%#
66) 1,2-Dichlorobenzene-d4	13.853	152	144942	24.429	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.720%
Target Compounds					Qvalue	
13) Acetone	4.135	43	7413m	8.055	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023331.D
Acq On : 25 May 2022 20:15
Operator : SY/VA
Sample : N2997-01
Misc : 4.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGW4

Quant Time: May 26 05:14:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 04:46:06 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

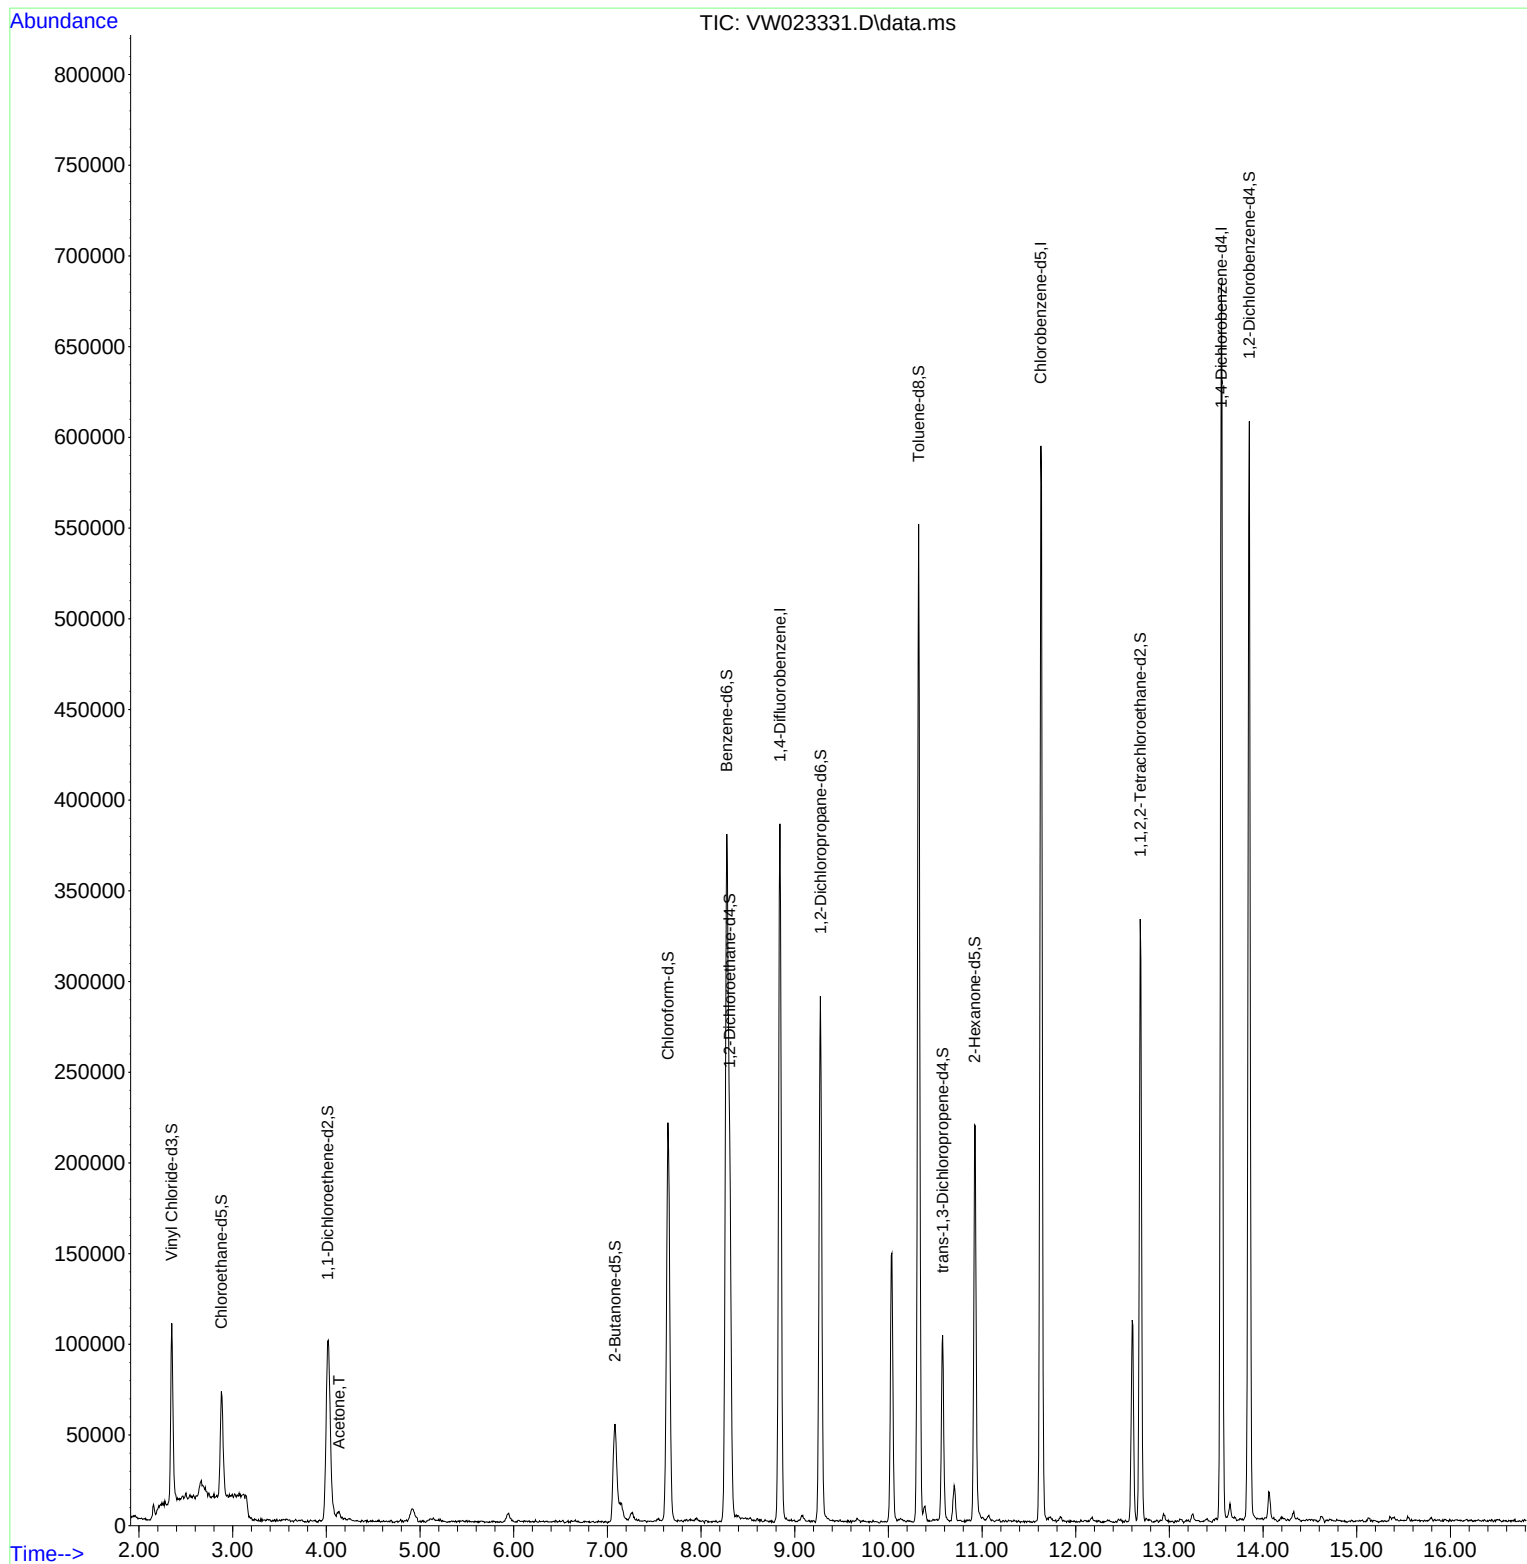

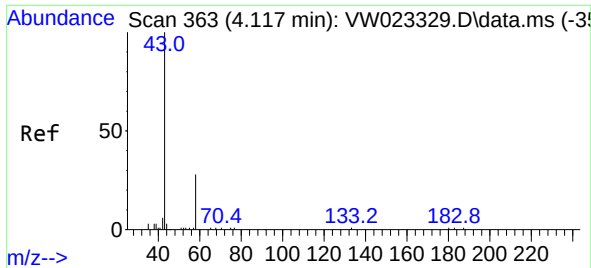

#13
Acetone
Concen: 8.055 ug/L m
RT: 4.135 min Scan# 30
Delta R.T. 0.018 min
Lab File: VW023331.D
Acq: 25 May 2022 20:15

Instrument :
MSVOA_W
ClientSampleId :
GBGW4

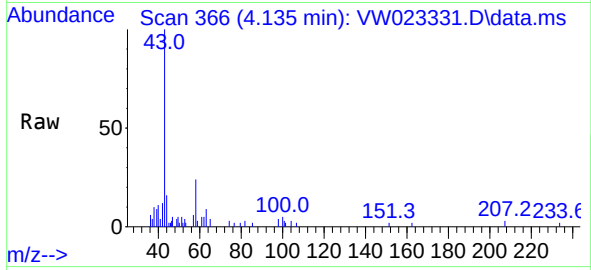

Tgt Ion: 43 Resp: 741
Ion Ratio Lower Upper
43 100
58 5.9 0.0 64.0

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

