

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023332.D
 Acq On : 25 May 2022 20:39
 Operator : SY/VA
 Sample : N2997-02
 Misc : 4.90g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGW5

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 05:14:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	309368	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	308589	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	157849	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	96392	15.187	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.760%		
7) Chloroethane-d5	2.879	69	61074	14.790	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	59.160%		
11) 1,1-Dichloroethene-d2	4.019	63	94705	11.548	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	46.200%		
21) 2-Butanone-d5	7.080	46	76615	63.486	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	126.980%		
24) Chloroform-d	7.647	84	200229	22.091	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	88.360%		
26) 1,2-Dichloroethane-d4	8.305	65	120100m	24.160	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	96.640%		
32) Benzene-d6	8.275	84	350064	19.681	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	78.720%		
36) 1,2-Dichloropropane-d6	9.274	67	114250	22.867	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.480%		
41) Toluene-d8	10.323	98	325266	18.930	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	75.720%		
43) trans-1,3-Dichloroprop...	10.579	79	46107	20.042	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.160%		
47) 2-Hexanone-d5	10.920	63	63703	66.789	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	133.580%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	135017	28.992	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	115.960%		
66) 1,2-Dichlorobenzene-d4	13.853	152	127722	23.147	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.600%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	9064	10.032	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023332.D
Acq On : 25 May 2022 20:39
Operator : SY/VA
Sample : N2997-02
Misc : 4.90g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGW5

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/26/2022
Supervised By : Mahesh Dadoda 05/26/2022


Quant Time: May 26 05:14:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 04:46:06 2022
Response via : Initial Calibration

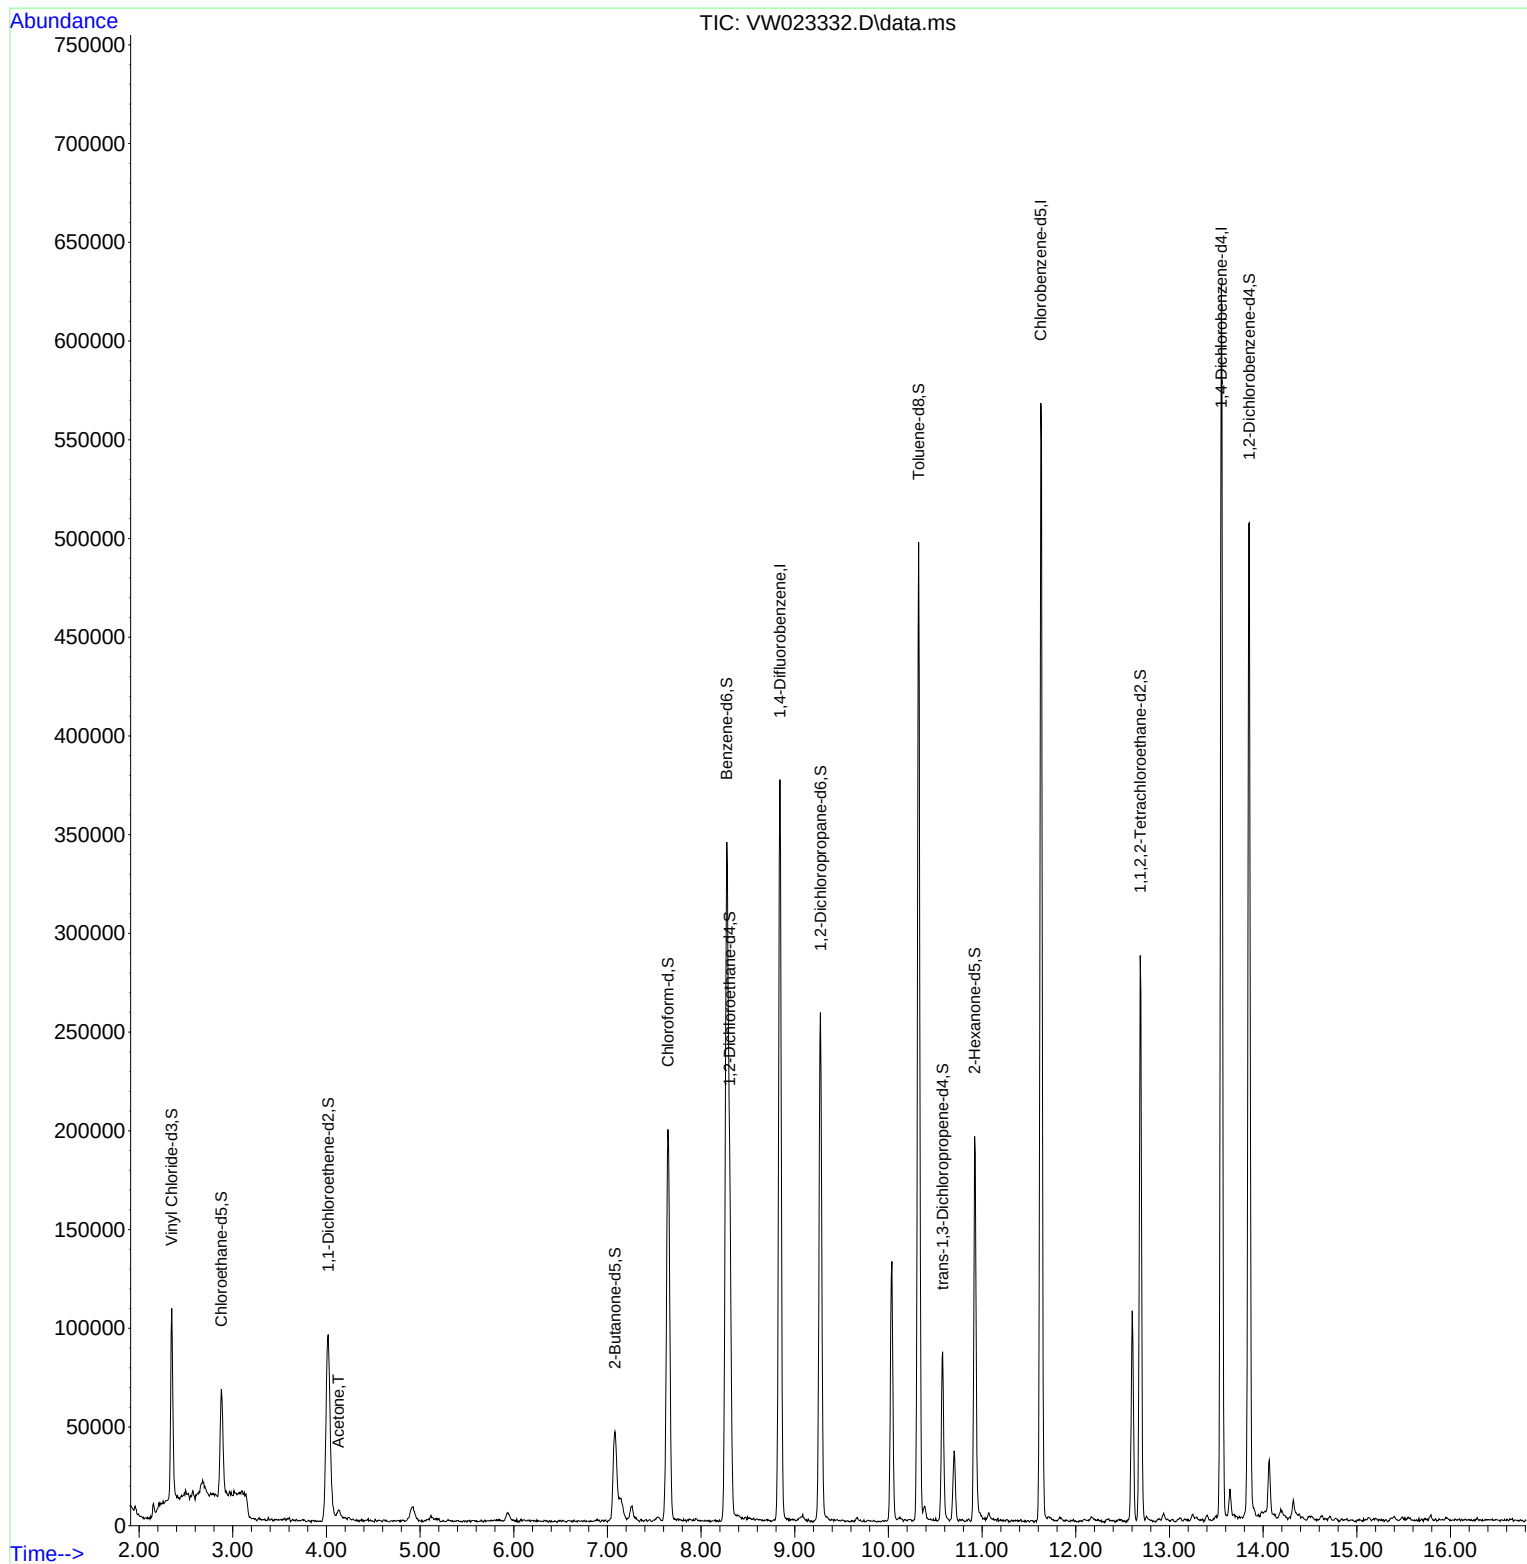

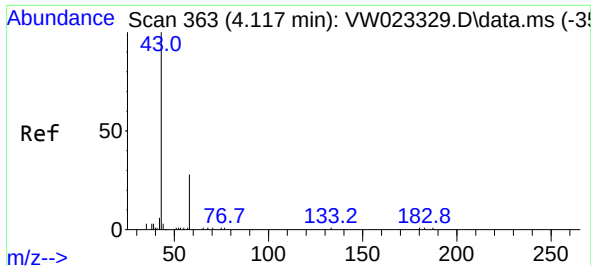

#13
 Acetone
 Concen: 10.032 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW023332.D
 Acq: 25 May 2022 20:39

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGW5

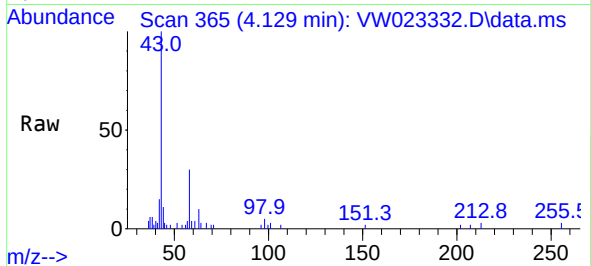

Tgt Ion: 43 Resp: 9064
 Ion Ratio Lower Upper
 43 100
 58 28.4 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

