

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023335.D
 Acq On : 25 May 2022 21:52
 Operator : SY/VA
 Sample : N2995-01RE
 Misc : 2.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ4

Quant Time: May 26 05:15:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	317711	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	320053	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	155261	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	98349	15.088	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	60.360%
7) Chloroethane-d5	2.885	69	66584	15.701	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	62.800%
11) 1,1-Dichloroethene-d2	4.019	63	99113	11.768	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	47.080%
21) 2-Butanone-d5	7.074	46	71234	57.477	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.960%
24) Chloroform-d	7.647	84	209174	22.472	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.880%
26) 1,2-Dichloroethane-d4	8.305	65	122303	23.957	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.840%
32) Benzene-d6	8.275	84	363403	19.699	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.800%
36) 1,2-Dichloropropane-d6	9.274	67	120600	23.273	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.080%
41) Toluene-d8	10.323	98	333736	18.728	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.920%
43) trans-1,3-Dichloroprop...	10.579	79	47853	20.056	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.240%
47) 2-Hexanone-d5	10.927	63	56825	57.443	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.880%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	131537	27.233	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.920%
66) 1,2-Dichlorobenzene-d4	13.853	152	123449	22.746	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.000%
Target Compounds						
13) Acetone	4.123	43	11153	12.020	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023335.D
Acq On : 25 May 2022 21:52
Operator : SY/VA
Sample : N2995-01RE
Misc : 2.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GBGQ4

Quant Time: May 26 05:15:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 04:46:06 2022
Response via : Initial Calibration

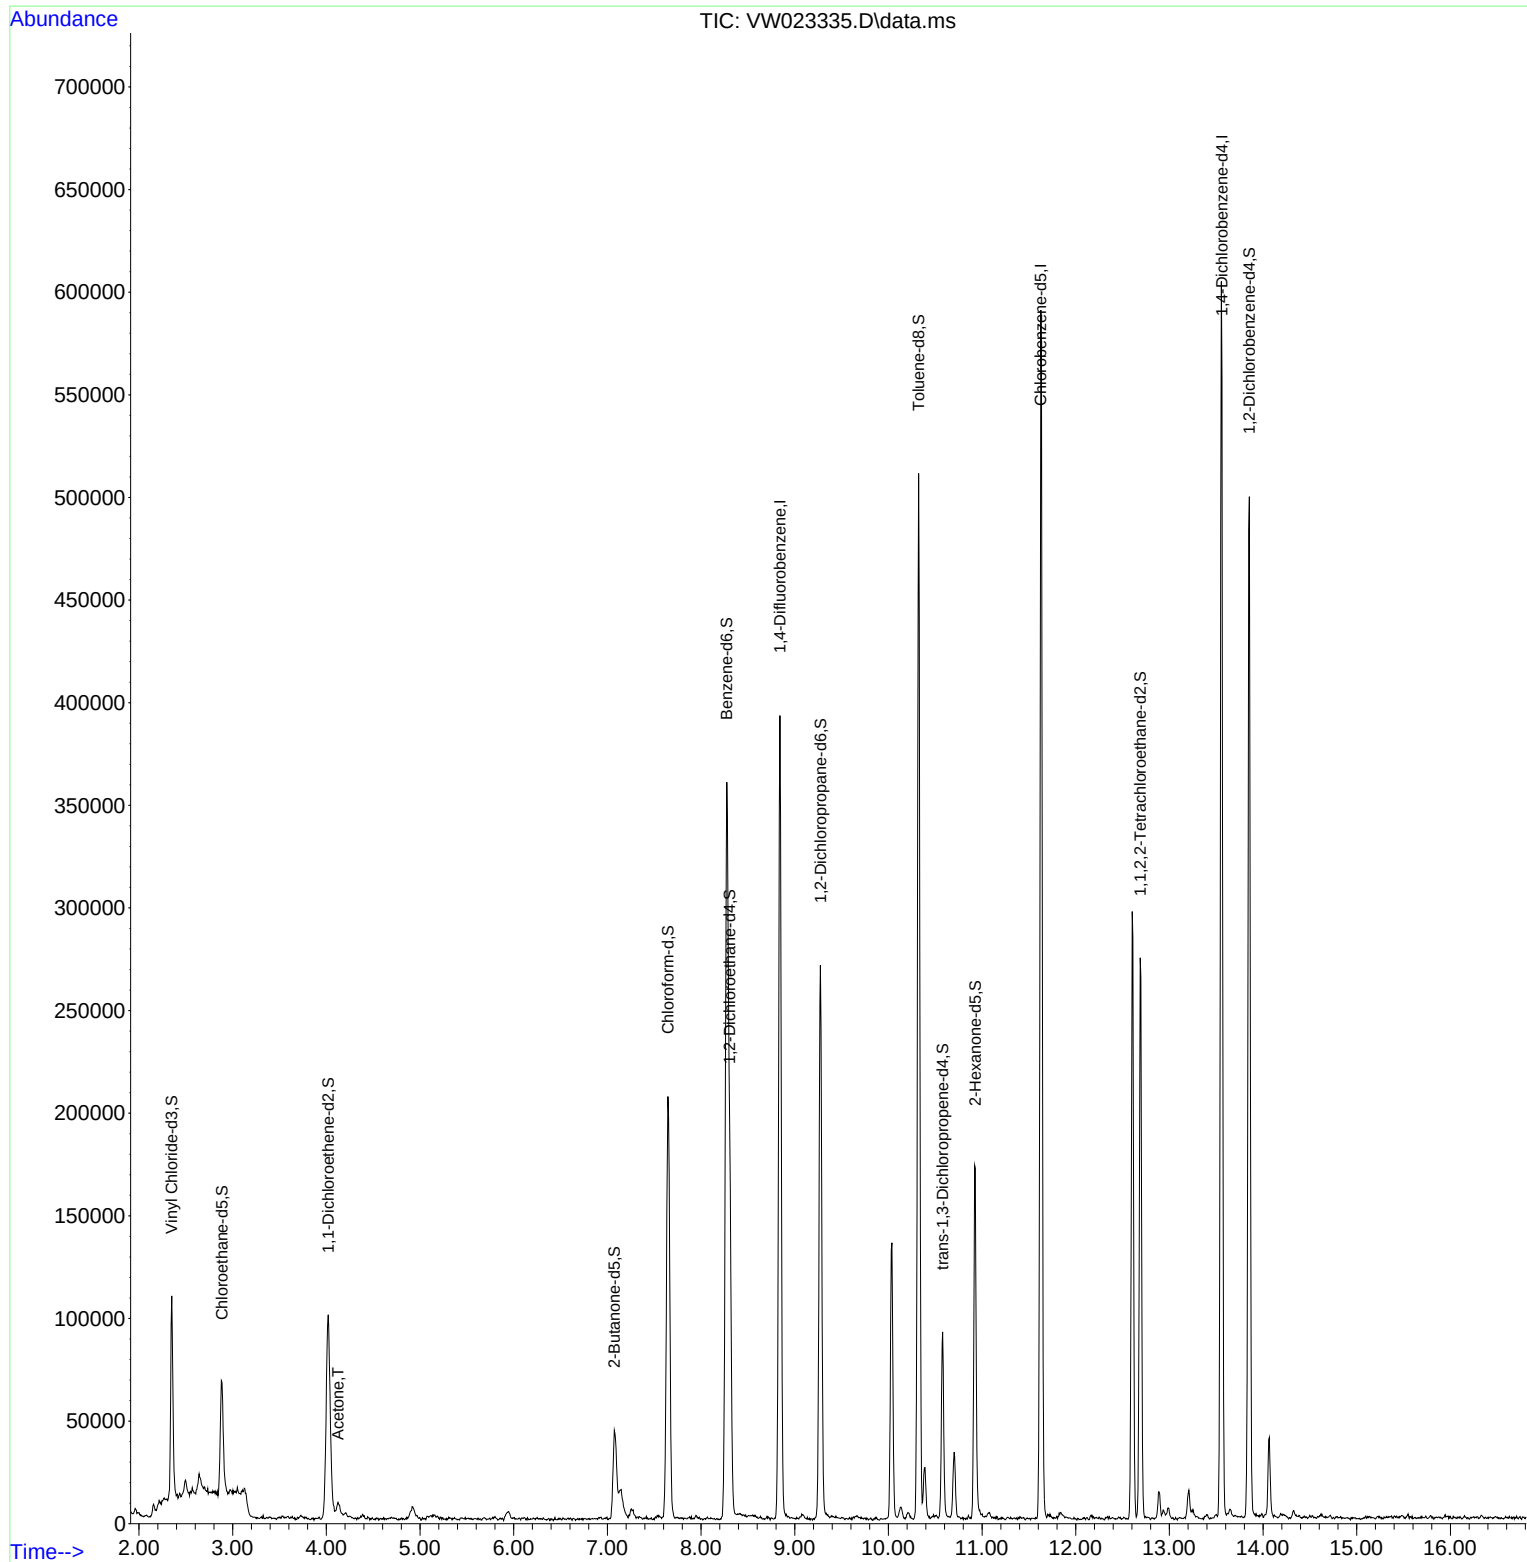

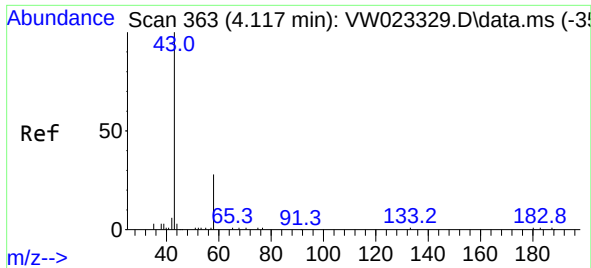

#13
 Acetone
 Concen: 12.020 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW023335.D
 Acq: 25 May 2022 21:52

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGQ4

Tgt Ion: 43 Resp: 11153
 Ion Ratio Lower Upper
 43 100
 58 32.1 0.0 64.0

