

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023338.D
 Acq On : 25 May 2022 23:04
 Operator : SY/VA
 Sample : N2995-11
 Misc : 5.22g/10mL/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR4

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 05:16:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	265388	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	271553	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	135342	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	82055	15.070	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.280%		
7) Chloroethane-d5	2.879	69	53262	15.036	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	60.160%		
11) 1,1-Dichloroethene-d2	4.019	63	80185	11.397	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	45.600%		
21) 2-Butanone-d5	7.074	46	70338m	67.944	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	135.880%#		
24) Chloroform-d	7.653	84	169686	21.824	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.280%		
26) 1,2-Dichloroethane-d4	8.305	65	105185m	24.666	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	98.680%		
32) Benzene-d6	8.275	84	299147	19.112	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.440%		
36) 1,2-Dichloropropane-d6	9.274	67	99369	22.601	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	90.400%		
41) Toluene-d8	10.323	98	275610	18.228	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	72.920%		
43) trans-1,3-Dichloroprop...	10.579	79	40963	20.234	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	80.920%		
47) 2-Hexanone-d5	10.927	63	55228	65.800	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	131.600%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	118877	29.008	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	116.040%		
66) 1,2-Dichlorobenzene-d4	13.847	152	108013	22.830	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.320%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	24765	31.952	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023338.D
Acq On : 25 May 2022 23:04
Operator : SY/VA
Sample : N2995-11
Misc : 5.22g/10mL/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGR4

Quant Time: May 26 05:16:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 04:46:06 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 05/26/2022
Supervised By :Mahesh Dadoda 05/26/2022

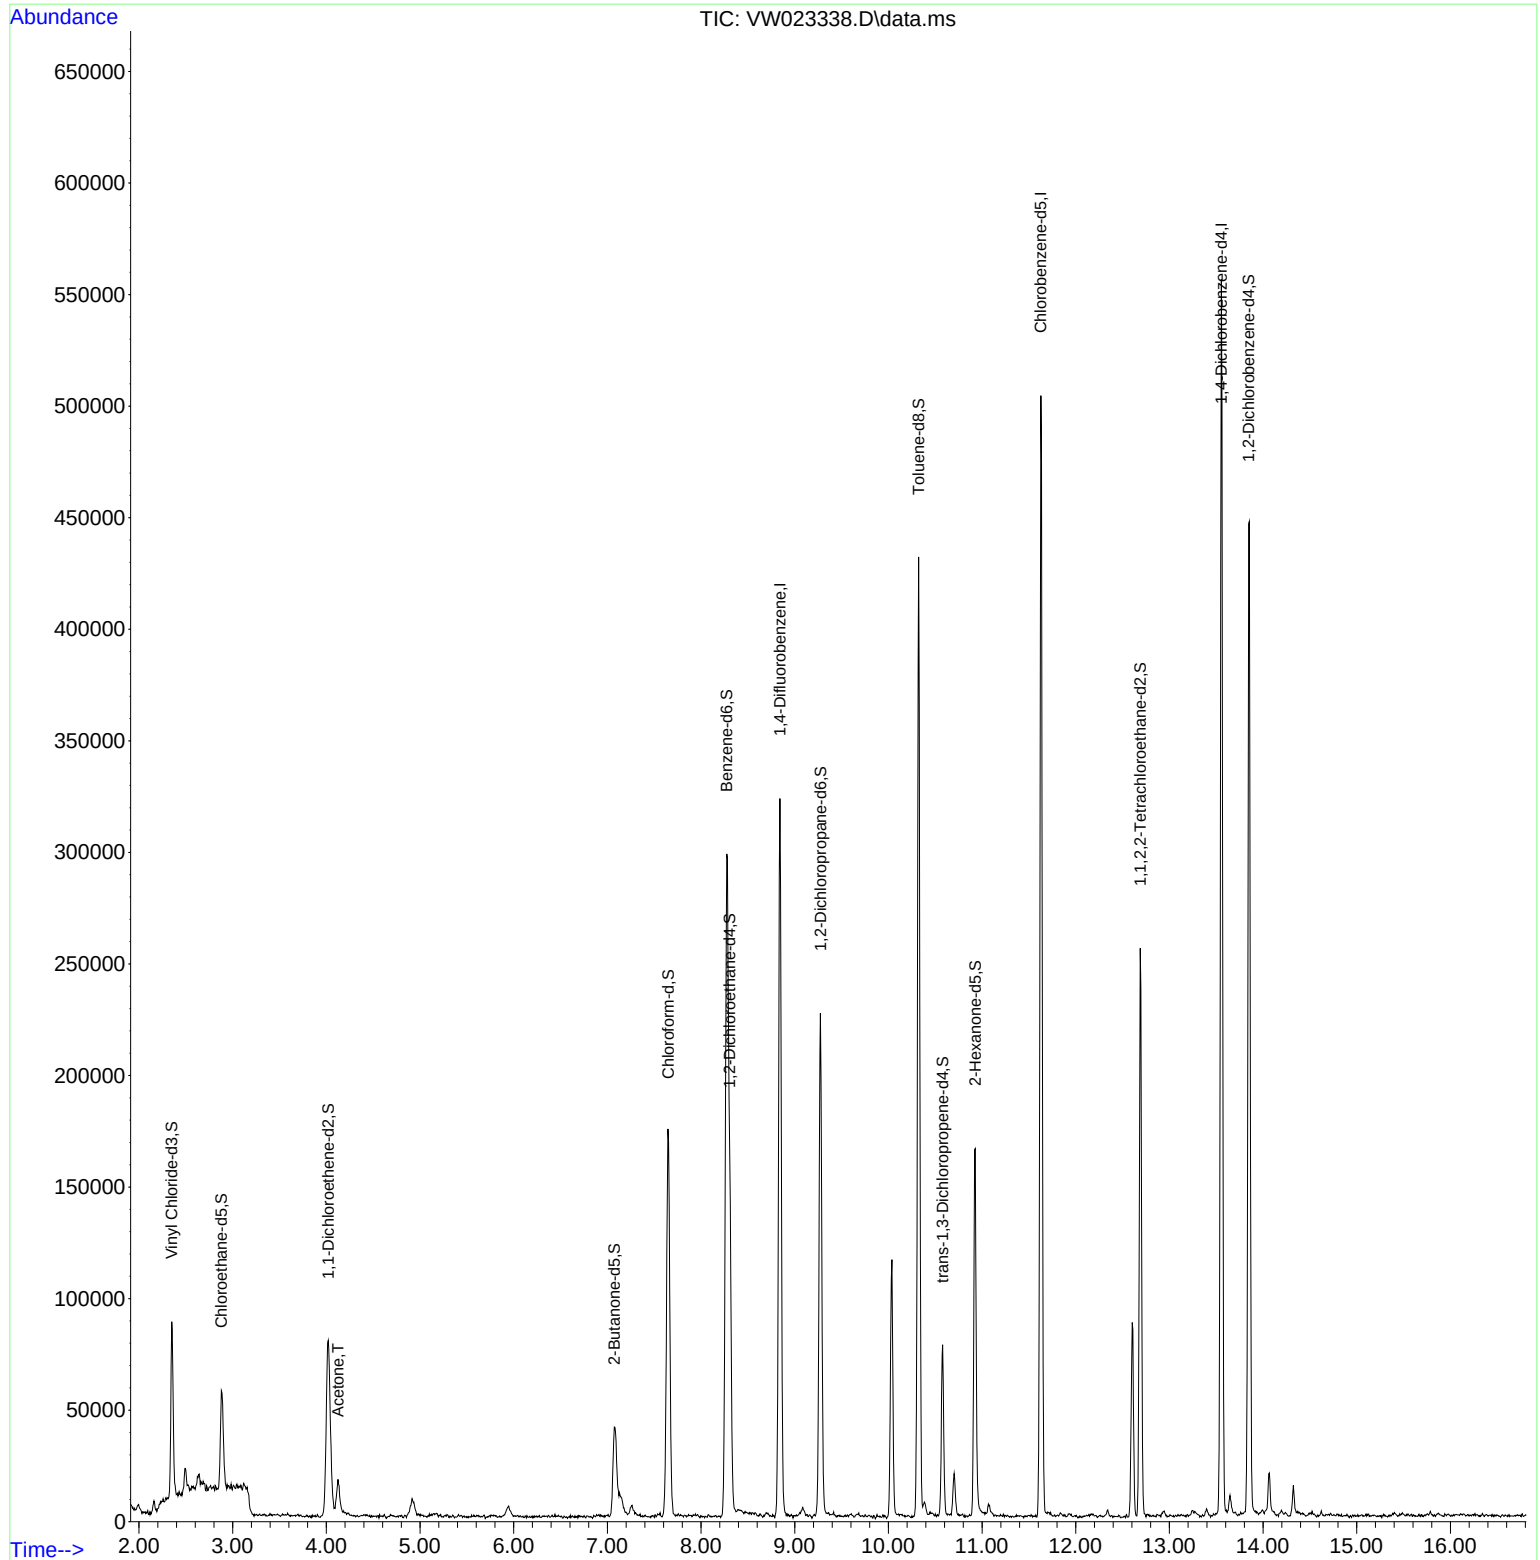

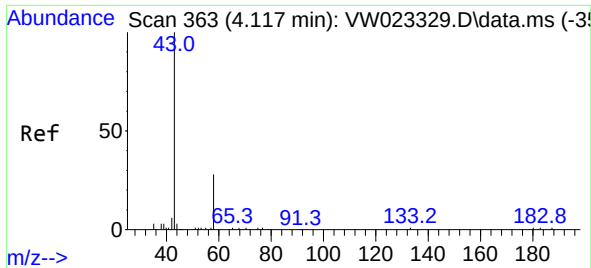

#13
 Acetone
 Concen: 31.952 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW023338.D
 Acq: 25 May 2022 23:04

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR4

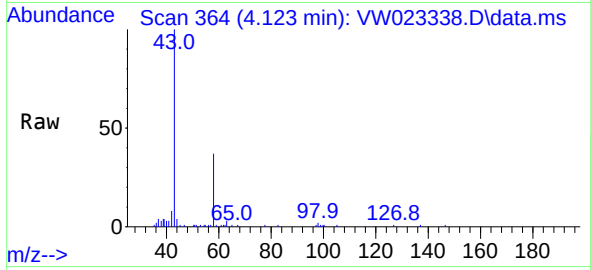

Tgt Ion: 43 Resp: 2476
 Ion Ratio Lower Upper
 43 100
 58 33.2 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

