

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023341.D
 Acq On : 26 May 2022 00:16
 Operator : SY/VA
 Sample : N2995-07
 Misc : 5.39g/10mL/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 05:16:45 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	332134	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	337562	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	172454	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	94645	13.889	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	55.560%
7) Chloroethane-d5	2.885	69	65188	14.705	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.800%
11) 1,1-Dichloroethene-d2	4.013	63	97335	11.055	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	44.200%#
21) 2-Butanone-d5	7.074	46	75122	57.982	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.960%
24) Chloroform-d	7.647	84	216111	22.209	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.840%
26) 1,2-Dichloroethane-d4	8.305	65	128537m	24.084	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.320%
32) Benzene-d6	8.275	84	384305	19.752	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.000%
36) 1,2-Dichloropropane-d6	9.274	67	122504	22.414	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.640%
41) Toluene-d8	10.323	98	349358	18.587	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.360%
43) trans-1,3-Dichloroprop...	10.579	79	50982	20.259	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.040%
47) 2-Hexanone-d5	10.927	63	62568	59.968	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.940%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	141019	27.682	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	110.720%
66) 1,2-Dichlorobenzene-d4	13.853	152	140052	23.232	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.920%
Target Compounds					Qvalue	
13) Acetone	4.129	43	12698	13.091	ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023341.D
Acq On : 26 May 2022 00:16
Operator : SY/VA
Sample : N2995-07
Misc : 5.39g/10mL/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGR0

Quant Time: May 26 05:16:45 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 04:46:06 2022
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/26/2022
Supervised By : Mahesh Dadoda 05/26/2022

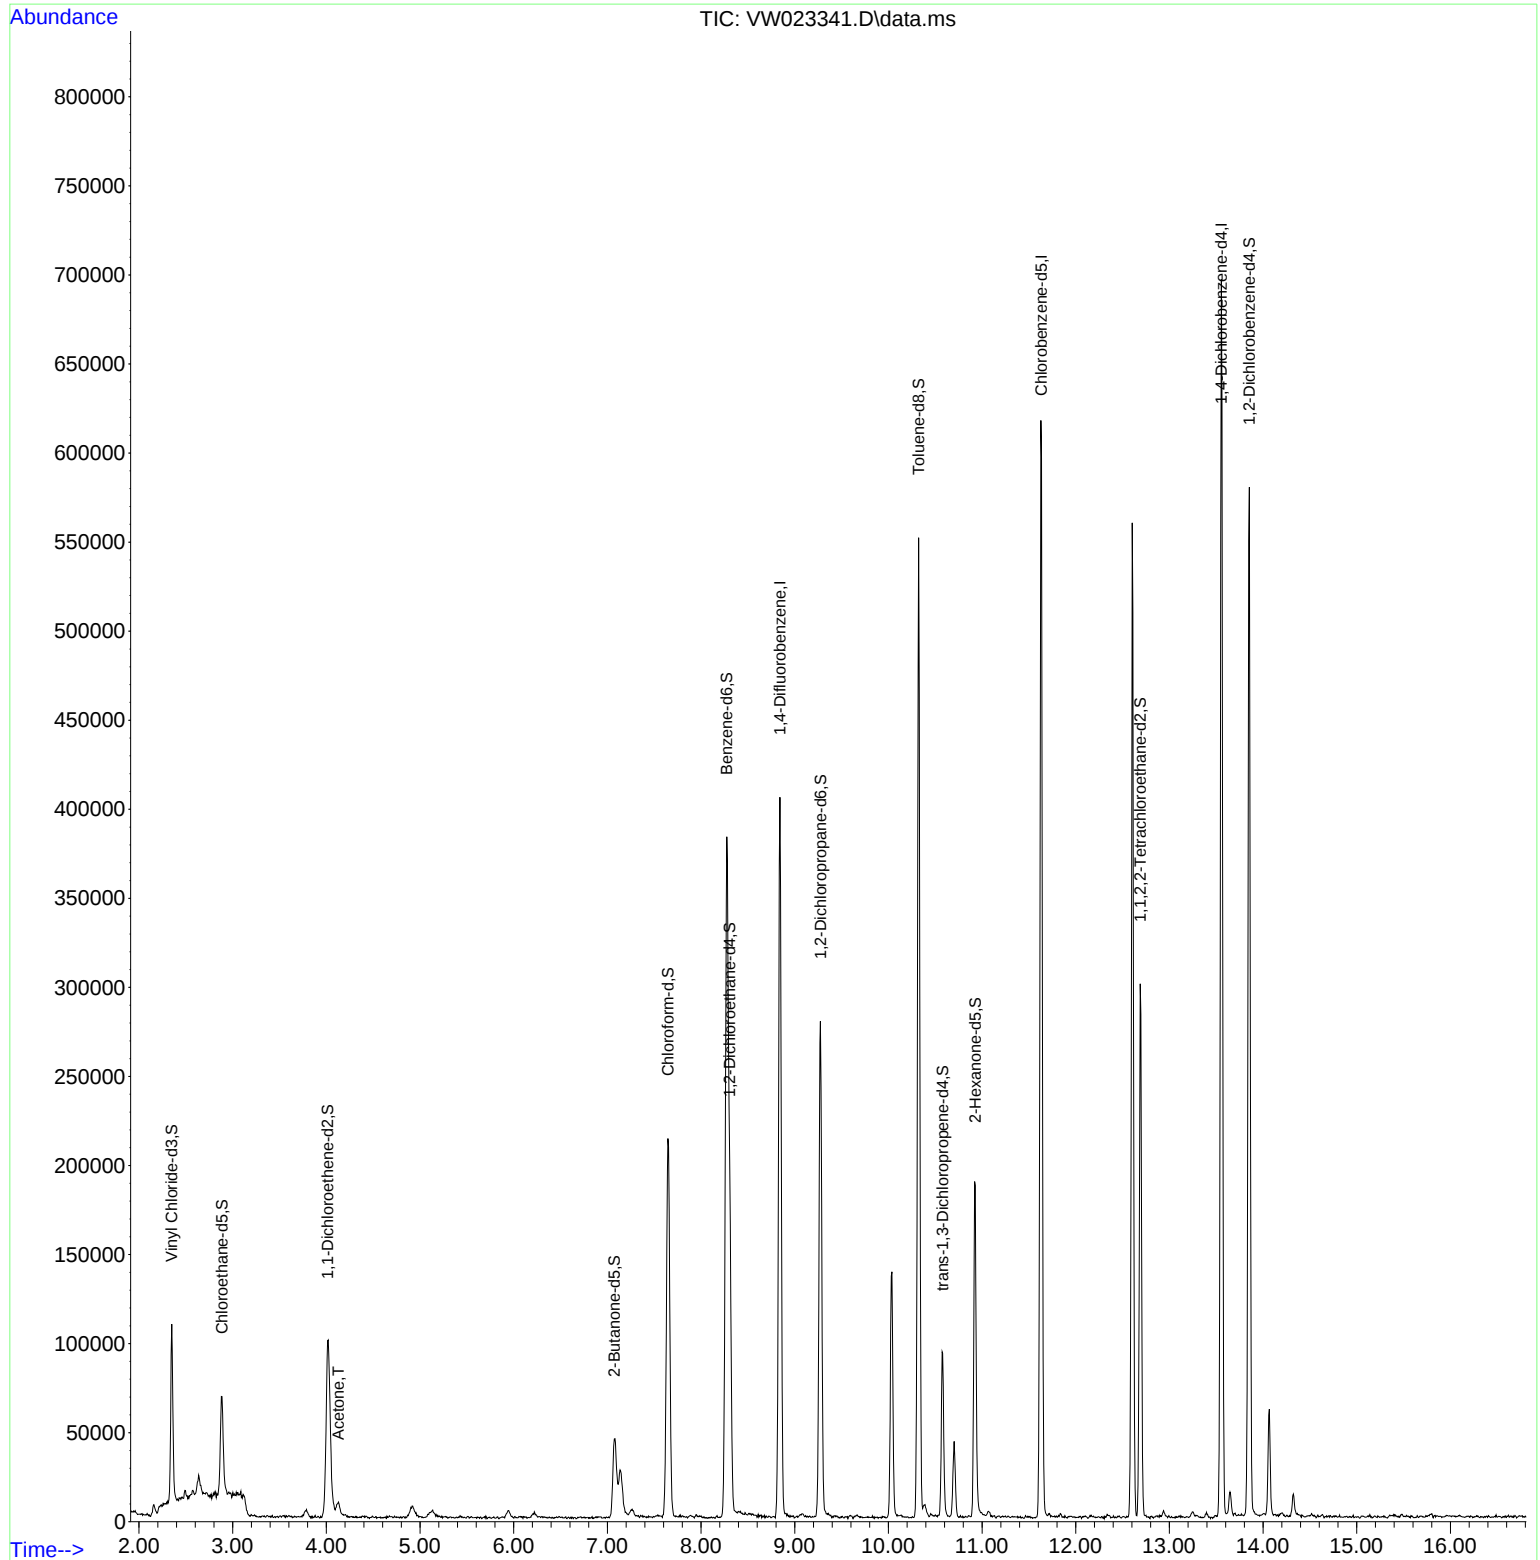

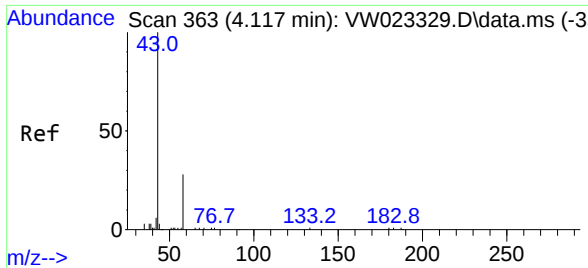

#13
 Acetone
 Concen: 13.091 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW023341.D
 Acq: 26 May 2022 00:16

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR0

Tgt Ion: 43 Resp: 12698
 Ion Ratio Lower Upper
 43 100
 58 32.2 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

