

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
 Data File : VW023343.D
 Acq On : 26 May 2022 01:04
 Operator : SY/VA
 Sample : N2995-17
 Misc : 3.92g/10mL/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

Quant Time: May 26 05:17:09 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu May 26 04:46:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	350721	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	364723	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	193665	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	97918	13.608	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	54.440%		
7) Chloroethane-d5	2.885	69	63809	13.631	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	54.520%		
11) 1,1-Dichloroethene-d2	4.019	63	105147	11.309	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	45.240%		
21) 2-Butanone-d5	7.074	46	70763	51.723	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	103.440%		
24) Chloroform-d	7.647	84	225591	21.955	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.800%		
26) 1,2-Dichloroethane-d4	8.305	65	129770m	23.027	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.120%		
32) Benzene-d6	8.275	84	391956	18.645	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	74.560%		
36) 1,2-Dichloropropane-d6	9.274	67	128834	21.817	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	87.280%		
41) Toluene-d8	10.323	98	372052	18.321	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	73.280%		
43) trans-1,3-Dichloroprop...	10.579	79	50608	18.613	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	74.440%		
47) 2-Hexanone-d5	10.921	63	55719	49.427	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.860%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	140599	25.544	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.160%		
66) 1,2-Dichlorobenzene-d4	13.853	152	154003	22.748	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	91.000%		
Target Compounds					Qvalue	
13) Acetone	4.123	43	12915	12.609	ug/L	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052522\
Data File : VW023343.D
Acq On : 26 May 2022 01:04
Operator : SY/VA
Sample : N2995-17
Misc : 3.92g/10mL/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GBGR8

Manual Integrations
APPROVED

Reviewed By : Semsettin Yesilyurt 05/26/2022
Supervised By : Mahesh Dadoda 05/26/2022


Quant Time: May 26 05:17:09 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Thu May 26 04:46:06 2022
Response via : Initial Calibration

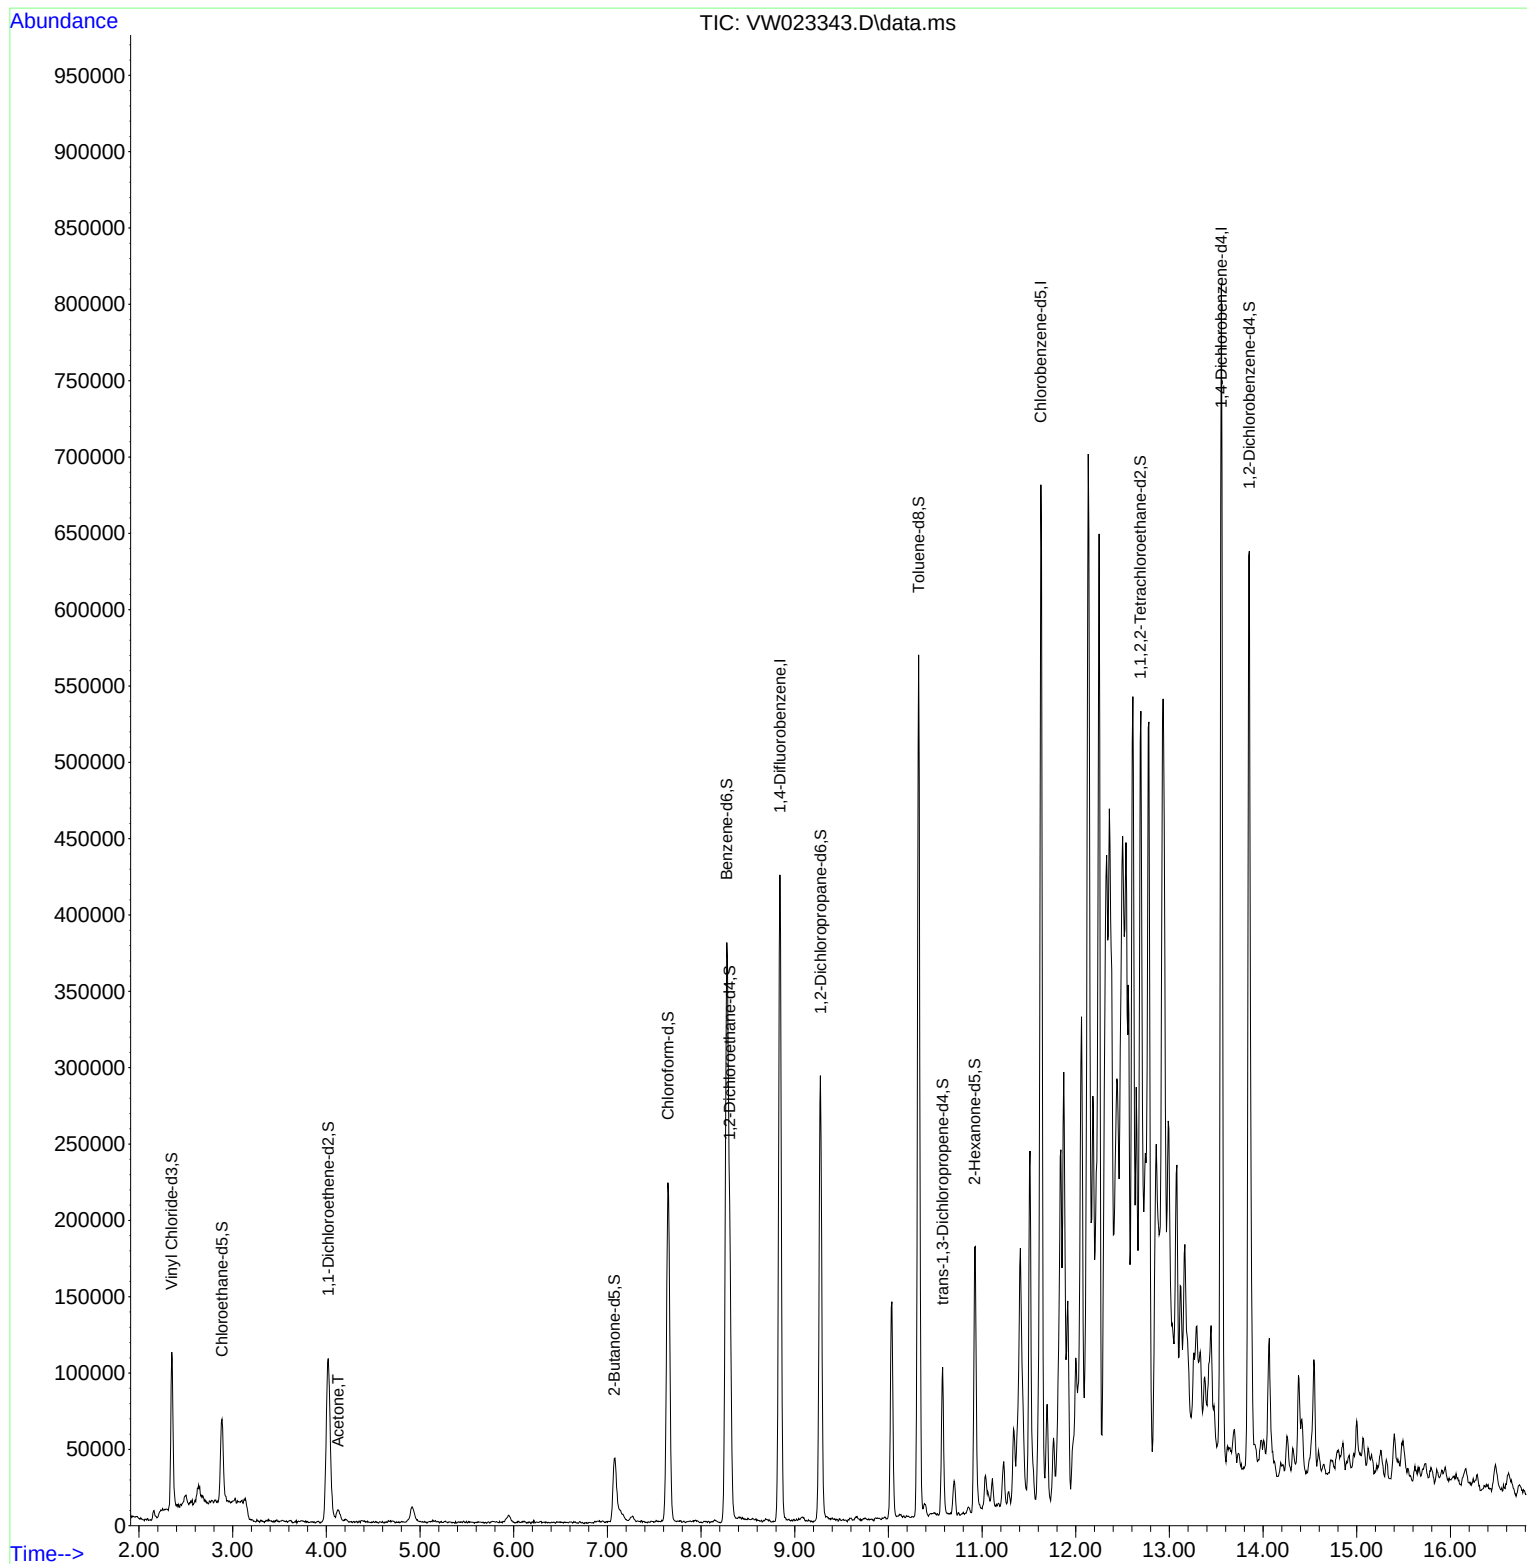

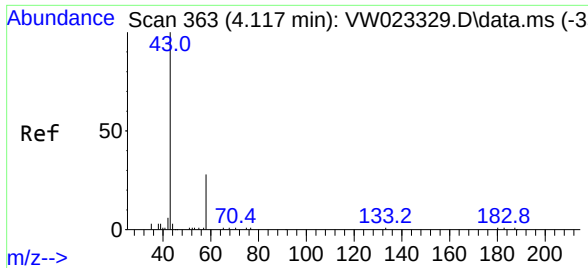

#13
 Acetone
 Concen: 12.609 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW023343.D
 Acq: 26 May 2022 01:04

Instrument :
 MSVOA_W
 ClientSampleId :
 GBGR8

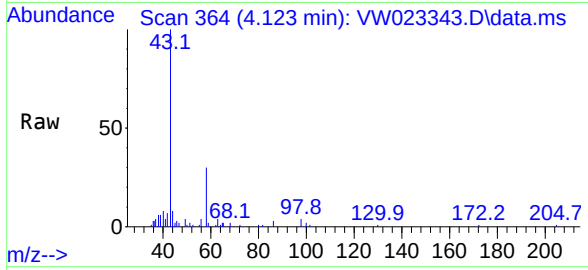

Tgt Ion: 43 Resp: 12915
 Ion Ratio Lower Upper
 43 100
 58 35.4 0.0 64.0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 05/26/2022
 Supervised By :Mahesh Dadoda 05/26/2022

