

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052622\
 Data File : VW023349.D
 Acq On : 26 May 2022 10:38
 Operator : SY/VA
 Sample : VW0526SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 27 00:23:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 27 00:22:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	369575	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	350955	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	187863	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	131779	17.380	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.520%
7) Chloroethane-d5	2.885	69	91676	18.584	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.320%
11) 1,1-Dichloroethene-d2	4.019	63	151157	15.428	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.720%
21) 2-Butanone-d5	7.080	46	76162	52.830	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.660%
24) Chloroform-d	7.653	84	256208	23.662	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.640%
26) 1,2-Dichloroethane-d4	8.305	65	143313	24.133	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.520%
32) Benzene-d6	8.274	84	503363	24.883	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.520%
36) 1,2-Dichloropropane-d6	9.274	67	145826	25.663	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.640%
41) Toluene-d8	10.323	98	477594	24.440	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.760%
43) trans-1,3-Dichloroprop...	10.579	79	64064	24.486	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.960%
47) 2-Hexanone-d5	10.920	63	61037	56.268	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.540%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	140385	26.506	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	106.040%
66) 1,2-Dichlorobenzene-d4	13.853	152	179646	27.356	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	109.440%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	5610	0.723	ug/L	# 60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052622\
Data File : VW023349.D
Acq On : 26 May 2022 10:38
Operator : SY/VA
Sample : VW0526SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 27 00:23:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 27 00:22:20 2022
Response via : Initial Calibration

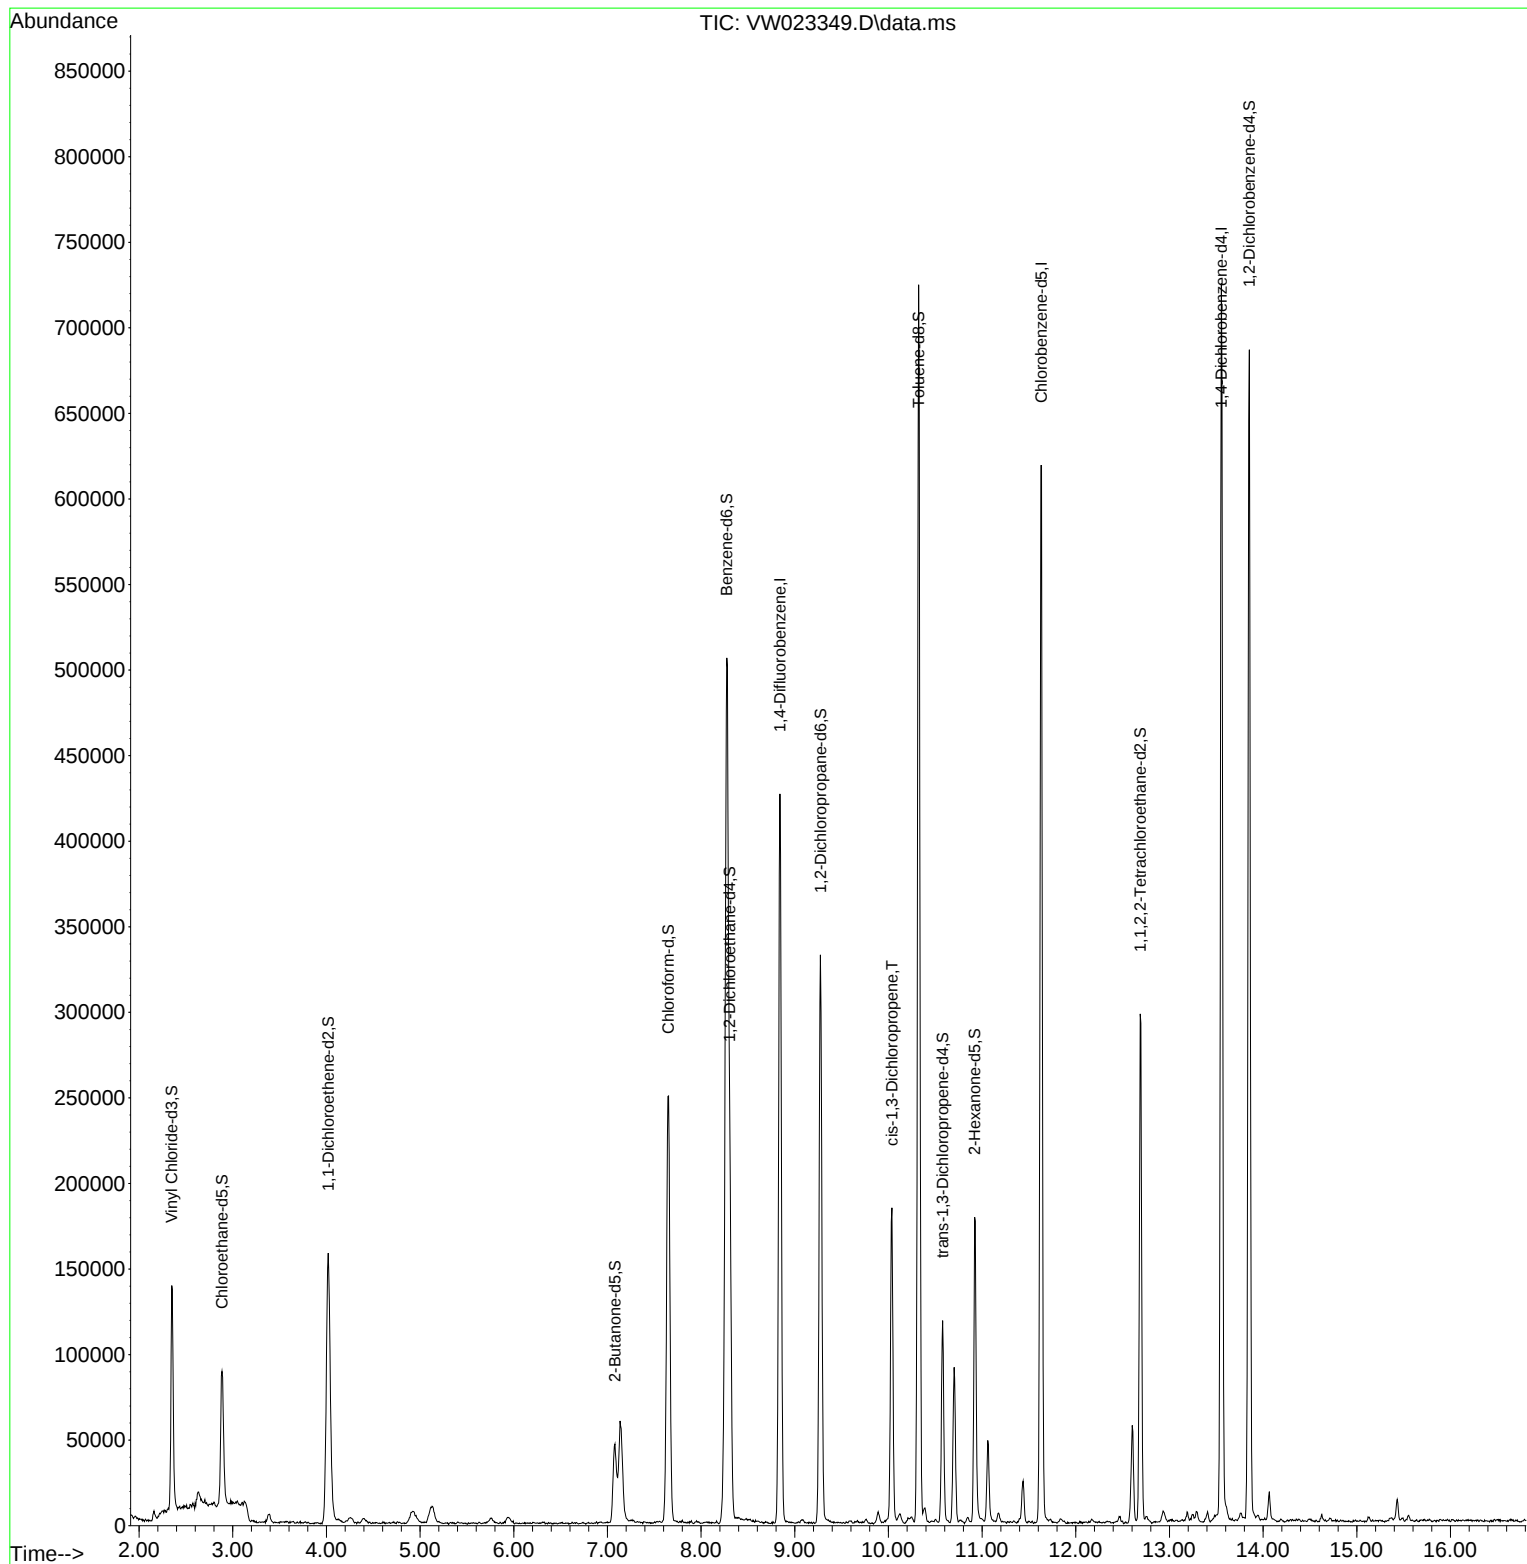

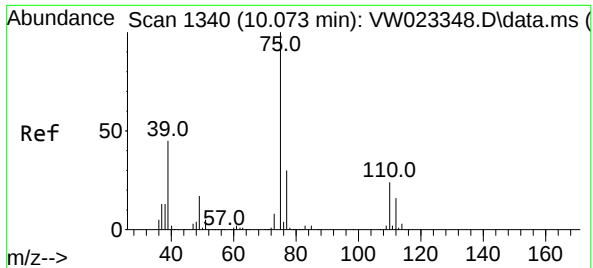

#39

cis-1,3-Dichloropropene

Concen: 0.723 ug/L

RT: 10.036 min Scan# 11

Delta R.T. -0.037 min


Lab File: VW023349.D

Acq: 26 May 2022 10:38

Instrument :

MSVOA_W

ClientSampleId :

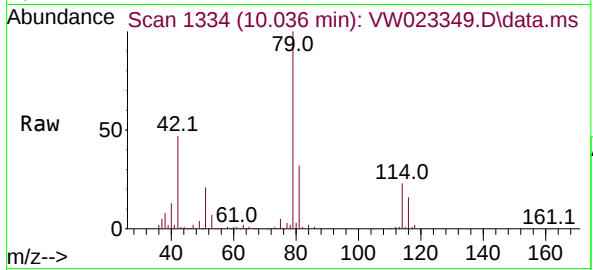

Tgt Ion: 75 Resp: 5610

Ion Ratio Lower Upper

75 100

77 53.9 22.1 41.1#

