

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052622\
 Data File : VW023350.D
 Acq On : 26 May 2022 11:02
 Operator : SY/VA
 Sample : N2925-23
 Misc : 5.06g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 27 00:23:19 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 27 00:22:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	364448	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.627	117	361460	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	188441	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	123819	16.560	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.240%
7) Chloroethane-d5	2.885	69	85348	17.545	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.200%
11) 1,1-Dichloroethene-d2	4.013	63	139773	14.467	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	57.880%
21) 2-Butanone-d5	7.080	46	78798	55.427	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.860%
24) Chloroform-d	7.646	84	245434	22.986	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.960%
26) 1,2-Dichloroethane-d4	8.305	65	143552	24.513	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	98.040%
32) Benzene-d6	8.274	84	472378	22.673	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.680%
36) 1,2-Dichloropropane-d6	9.274	67	140257	23.966	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.880%
41) Toluene-d8	10.323	98	457646	22.739	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.960%
43) trans-1,3-Dichloroprop...	10.579	79	62819	23.312	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.240%
47) 2-Hexanone-d5	10.920	63	64467	57.703	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	115.400%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	139388	25.553	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.200%
66) 1,2-Dichlorobenzene-d4	13.853	152	168508	25.581	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	102.320%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.036	75	5355	0.670	ug/L	# 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052622\
Data File : VW023350.D
Acq On : 26 May 2022 11:02
Operator : SY/VA
Sample : N2925-23
Misc : 5.06g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 27 00:23:19 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 27 00:22:20 2022
Response via : Initial Calibration

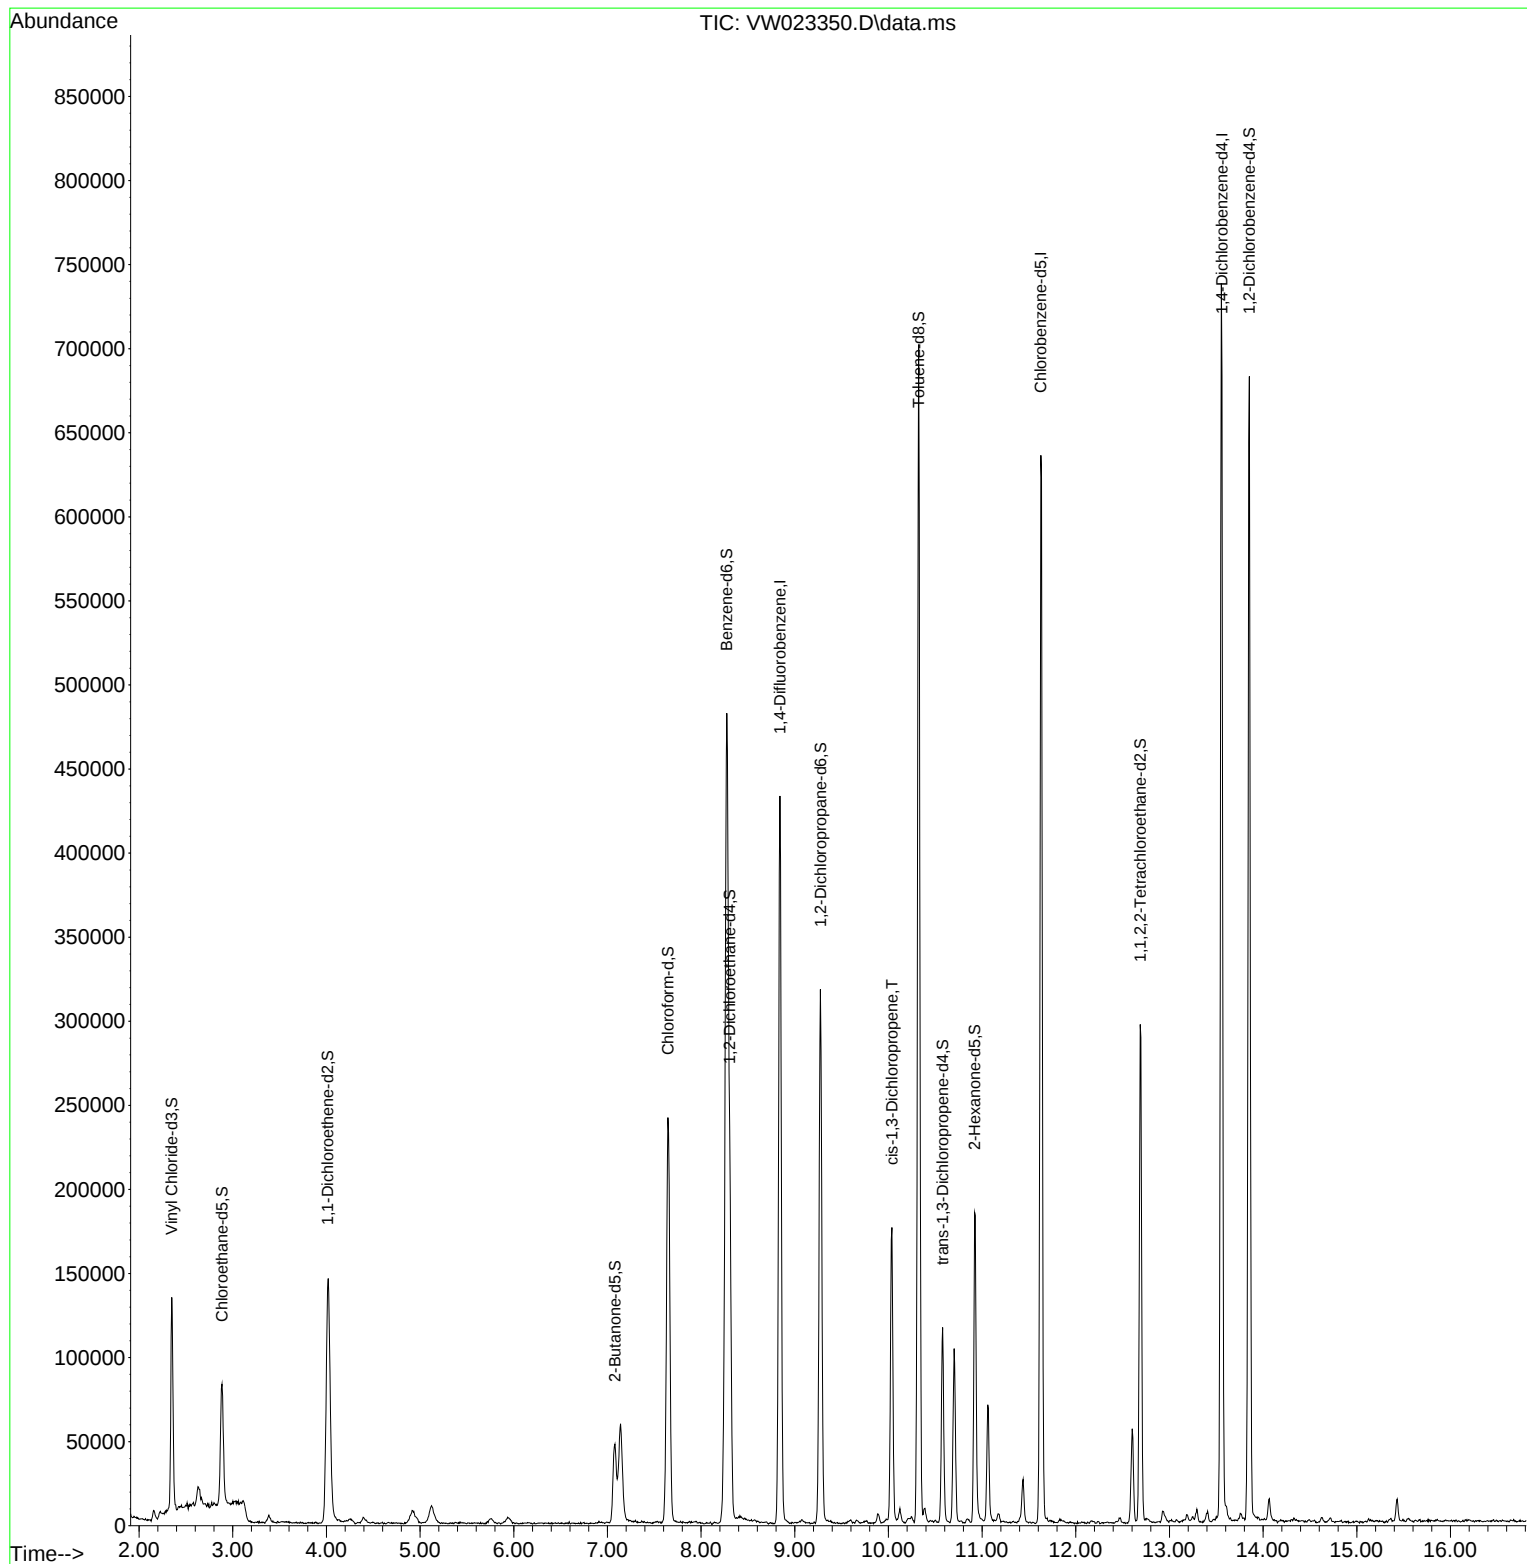

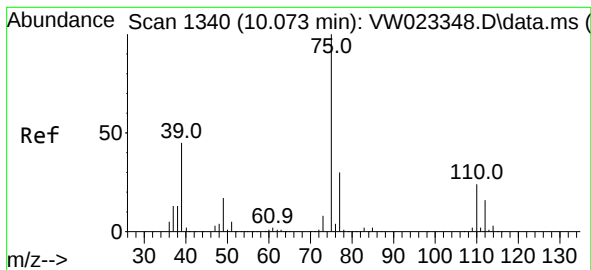

#39
 cis-1,3-Dichloropropene
 Concen: 0.670 ug/L
 RT: 10.036 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW023350.D
 Acq: 26 May 2022 11:02

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 5355
 Ion Ratio Lower Upper
 75 100
 77 47.2 22.1 41.1#

