

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052622\
 Data File : VW023356.D
 Acq On : 26 May 2022 13:27
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: May 27 00:24:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 27 00:22:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	325295	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	325756	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	169986	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	120775	18.097	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	72.400%		
7) Chloroethane-d5	2.879	69	73420	16.910	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	67.640%		
11) 1,1-Dichloroethene-d2	4.019	63	122517	14.207	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	56.840%		
21) 2-Butanone-d5	7.080	46	56204	44.293	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	88.580%		
24) Chloroform-d	7.653	84	216764	22.745	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	90.960%		
26) 1,2-Dichloroethane-d4	8.305	65	119809	22.921	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	91.680%		
32) Benzene-d6	8.275	84	415867	22.148	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.600%		
36) 1,2-Dichloropropane-d6	9.275	67	122115	23.153	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	92.600%		
41) Toluene-d8	10.323	98	394402	21.744	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	86.960%		
43) trans-1,3-Dichloroprop...	10.579	79	50857	20.942	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.760%		
47) 2-Hexanone-d5	10.921	63	46398	46.082	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.160%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	112420	22.868	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	91.480%		
66) 1,2-Dichlorobenzene-d4	13.853	152	145991	24.569	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.280%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.037	75	4551	0.632	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW052622\
Data File : VW023356.D
Acq On : 26 May 2022 13:27
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: May 27 00:24:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 27 00:22:20 2022
Response via : Initial Calibration

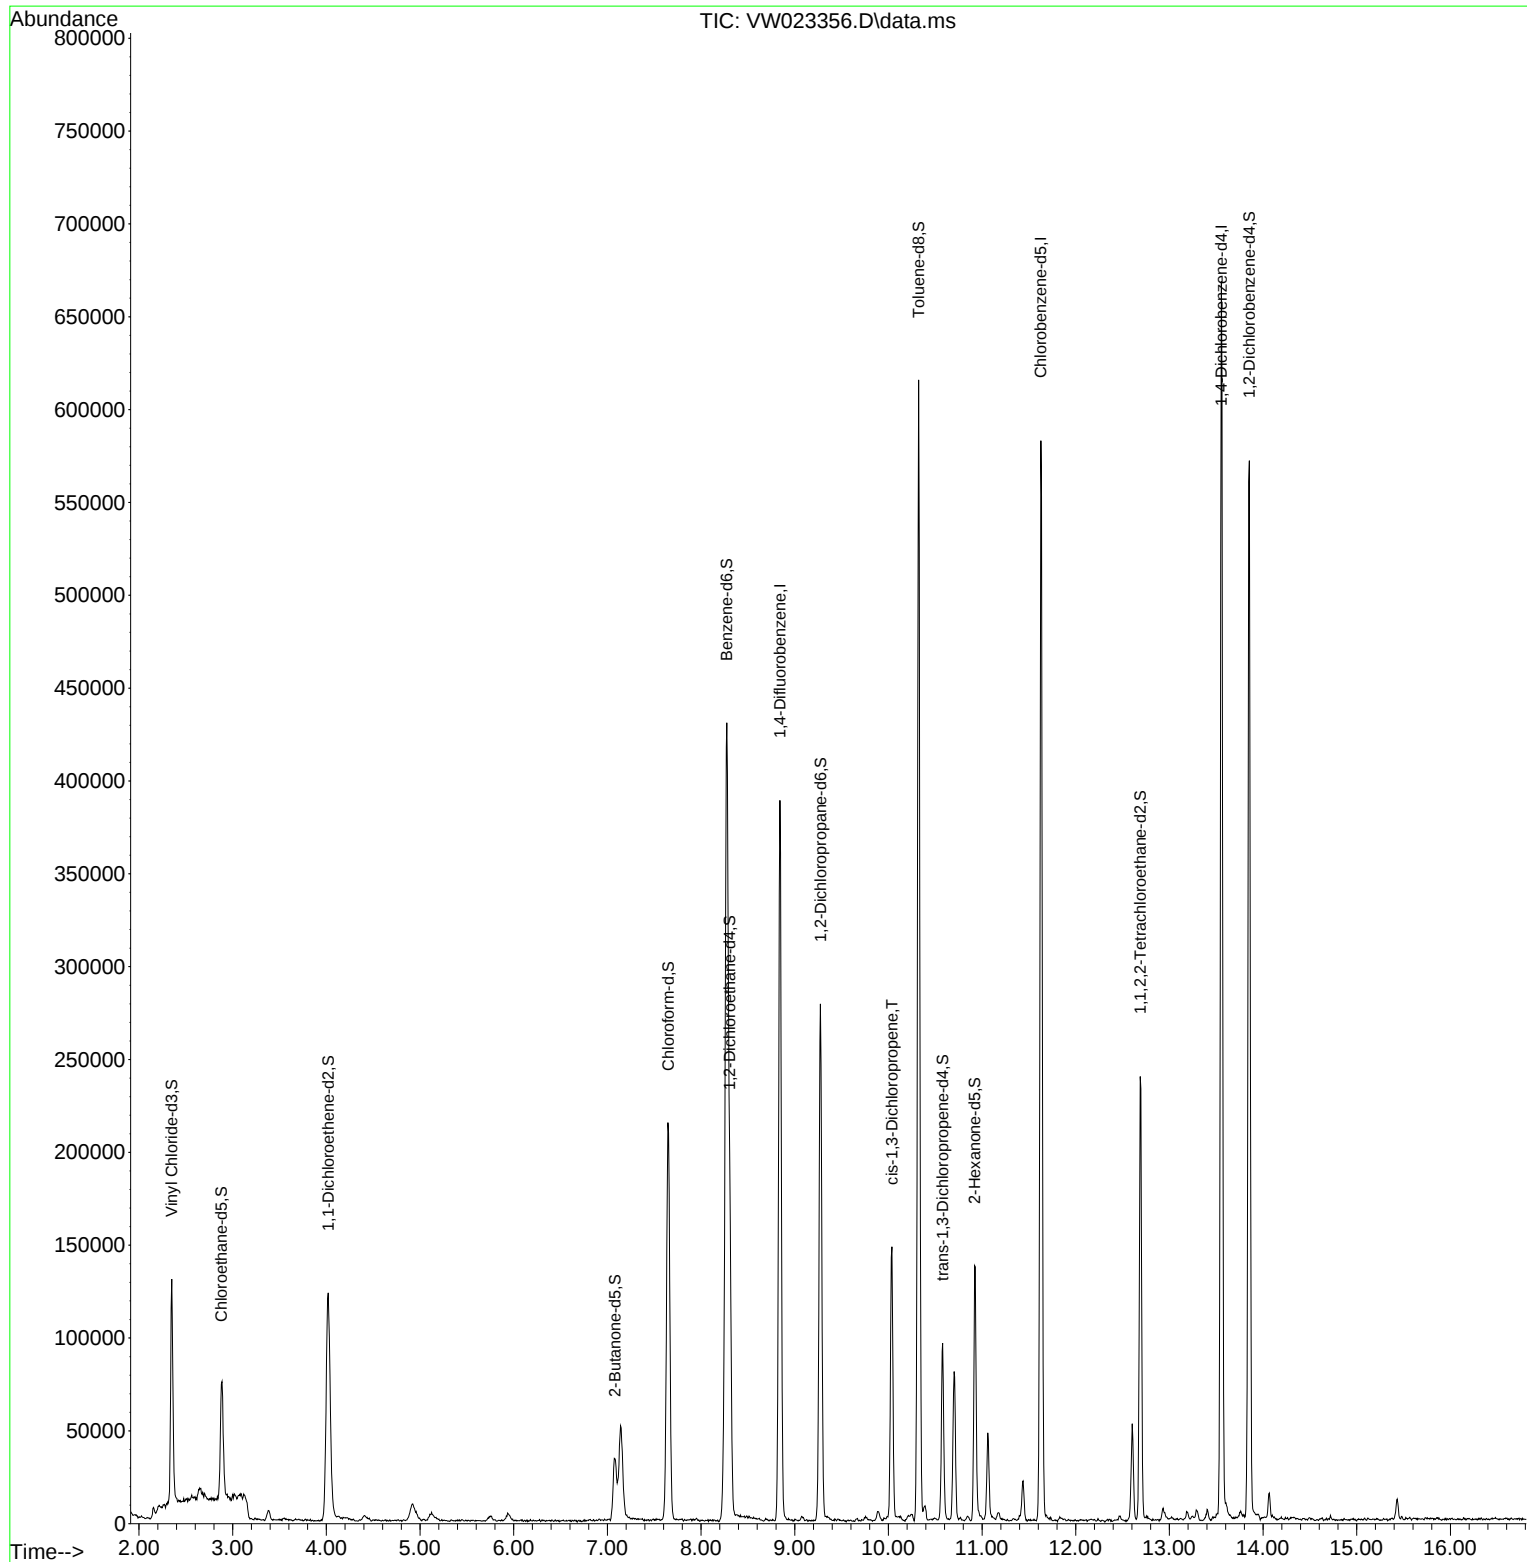

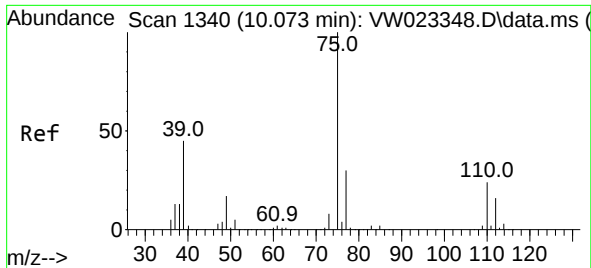

#39

cis-1,3-Dichloropropene

Concen: 0.632 ug/L

RT: 10.037 min Scan# 11

Delta R.T. -0.037 min


Lab File: VW023356.D

Acq: 26 May 2022 13:27

Instrument :

MSVOA_W

ClientSampleId :

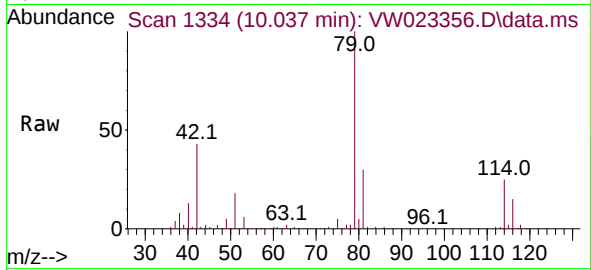

Tgt Ion: 75 Resp: 4551

Ion Ratio Lower Upper

75 100

77 35.2 22.1 41.1

