


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW052820\
 Data File : VW015511.D
 Acq On : 28 May 2020 09:17
 Operator : SY/VA
 Sample : BFB03
 Misc : 5.00G/10.0mL/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB03

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM052620S.M
 Title : VOC Analysis
 Last Update : Fri May 29 03:23:16 2020

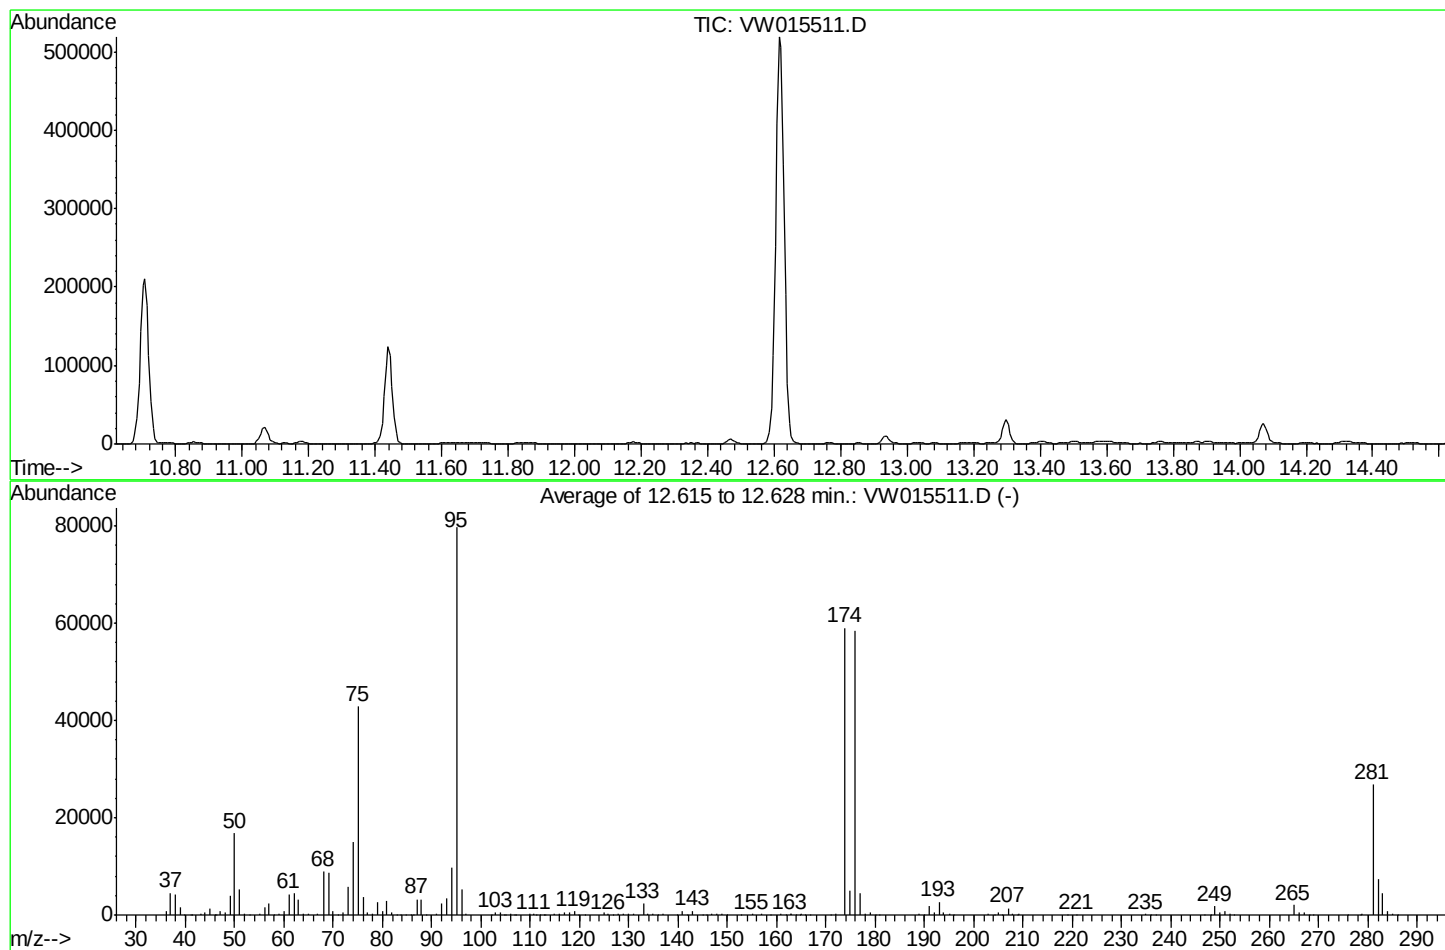

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	16822	PASS
75	95	30	80	53.7	42810	PASS
95	95	100	100	100.0	79717	PASS
96	95	5	9	6.7	5364	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.0	59024	PASS
175	174	5	9	8.3	4891	PASS
176	174	95	101	99.0	58429	PASS
177	176	5	9	7.6	4423	PASS

m/z	Abundance
36.00	1007.0
37.00	4931.0
38.00	4656.0
39.00	1727.0
39.90	176.0
40.90	61.0
41.20	56.0
43.10	277.0
44.00	830.0
45.00	1672.0
46.00	133.0
47.00	933.0
48.00	673.0
49.00	4315.0
50.00	19224.0
51.00	5834.0
52.00	286.0
54.90	315.0
56.00	1584.0
57.00	2796.0
58.00	155.0
59.00	656.0
60.00	962.0
61.00	4857.0
62.00	4907.0
63.00	3695.0
64.00	344.0
64.90	192.0
67.00	247.0
68.00	9773.0
69.00	9370.0
70.00	765.0
70.90	91.0
72.00	554.0
73.00	7834.0
74.00	16584.0
75.00	46664.0
76.00	4137.0
76.90	469.0
77.90	306.0
78.90	3109.0
79.90	1017.0
80.90	3258.0
82.00	666.0
83.10	135.0
83.70	160.0
84.80	96.0
87.00	3526.0
87.90	3586.0
88.90	317.0
90.90	410.0
92.00	2597.0
93.00	3557.0
94.00	10688.0
95.00	85736.0
96.00	5792.0
96.90	226.0
102.00	75.0
102.90	683.0
103.90	568.0
104.80	334.0
106.00	371.0
106.80	118.0
109.90	266.0
110.80	198.0
111.10	215.0
112.10	165.0
112.80	131.0
114.90	294.0
115.80	385.0
116.90	703.0
117.90	735.0
118.90	1060.0
119.70	134.0
121.00	133.0
124.90	1138.0
125.90	259.0
127.90	286.0
128.90	181.0
129.90	337.0
130.90	244.0
132.90	3818.0
134.80	427.0
135.90	79.0
136.90	144.0
139.80	65.0
140.90	830.0
141.80	92.0
142.90	794.0
145.00	100.0
145.80	131.0
146.90	529.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

147.90	289.0
148.90	174.0
149.90	131.0
152.80	58.0
155.00	174.0
156.80	159.0
158.90	151.0
160.80	256.0
161.90	92.0
162.80	670.0
163.90	109.0
165.00	328.0
165.80	122.0
166.90	97.0
171.90	227.0
173.90	55008.0
174.90	4941.0
175.90	57456.0
176.90	4692.0
177.90	427.0
178.90	961.0
180.00	163.0
180.90	90.0
188.90	306.0
189.80	129.0
190.90	3321.0
192.00	763.0
193.00	4317.0
193.90	803.0
195.00	467.0
195.80	53.0
203.00	306.0
204.10	130.0
204.90	873.0
205.80	221.0
207.00	2492.0
208.00	532.0
208.80	263.0
209.00	262.0
219.00	99.0
220.90	159.0
234.90	365.0
235.80	77.0
237.00	64.0
246.80	82.0
248.00	116.0
249.00	2871.0
249.90	837.0
251.00	1428.0
252.00	228.0
252.90	154.0
264.90	3161.0
266.00	759.0
267.00	821.0
268.10	135.0
268.90	78.0
275.90	53.0
278.90	285.0
281.00	39440.0
282.00	11238.0
282.90	7239.0
284.00	1533.0
285.00	552.0
285.90	108.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

m/z	Abundance
36.00	959.0
37.00	5336.0
38.00	4553.0
39.00	1763.0
40.00	128.0
41.00	95.0
43.00	145.0
44.00	882.0
45.00	1255.0
46.00	90.0
46.90	1015.0
48.00	675.0
49.00	4331.0
50.00	18384.0
51.00	5794.0
52.00	294.0
53.00	77.0
55.00	306.0
56.00	1720.0
57.00	2596.0
58.00	125.0
59.00	296.0
60.00	991.0
61.00	4669.0
62.00	4790.0
63.00	3587.0
64.00	389.0
65.00	110.0
66.90	278.0
68.00	9900.0
69.00	9881.0
70.00	744.0
71.00	126.0
71.90	621.0
73.00	6069.0
74.00	16872.0
75.00	47832.0
76.00	3996.0
77.00	568.0
77.90	270.0
78.90	3110.0
79.90	903.0
80.90	3336.0
81.90	697.0
82.90	131.0
83.70	67.0
85.80	99.0
86.90	3470.0
87.90	3171.0
90.90	372.0
92.00	2561.0
93.00	3924.0
94.00	11066.0
95.00	89248.0
96.00	6176.0
97.00	230.0
102.90	468.0
103.90	454.0
105.00	230.0
105.90	479.0
107.00	100.0
109.80	152.0
110.80	209.0
111.90	132.0
112.70	71.0
115.00	222.0
115.90	422.0
116.90	789.0
118.00	495.0
118.90	739.0
119.80	109.0
124.90	549.0
125.80	215.0
126.70	55.0
127.80	291.0
128.90	159.0
129.90	337.0
131.00	147.0
133.00	2231.0
133.80	537.0
134.90	320.0
135.90	65.0
136.90	184.0
139.80	93.0
140.90	933.0
141.80	120.0
142.90	941.0
144.90	106.0
145.80	140.0
146.90	273.0
147.80	278.0
148.90	220.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

149.80	129.0
155.00	165.0
156.80	116.0
156.90	116.0
158.80	110.0
160.80	224.0
161.90	80.0
163.00	379.0
164.00	79.0
164.90	240.0
171.00	90.0
171.80	266.0
173.90	68320.0
174.90	5156.0
175.90	64840.0
176.90	4838.0
177.90	320.0
179.00	548.0
179.90	86.0
180.70	81.0
188.90	206.0
190.90	1695.0
192.00	501.0
193.00	2566.0
193.90	536.0
195.00	268.0
202.90	210.0
204.10	60.0
204.90	446.0
205.90	108.0
207.00	1216.0
207.90	349.0
209.00	165.0
218.80	64.0
220.90	93.0
235.00	256.0
235.80	66.0
246.80	53.0
248.10	84.0
248.90	1425.0
249.90	459.0
250.90	790.0
252.00	197.0
252.80	78.0
265.00	1910.0
266.00	449.0
266.90	378.0
267.90	138.0
278.80	181.0
281.00	27584.0
282.00	7387.0
283.00	4357.0
284.00	733.0
284.90	315.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

m/z	Abundance
36.00	666.0
37.00	3519.0
38.00	3164.0
39.10	1380.0
39.90	217.0
40.90	61.0
43.00	103.0
44.00	647.0
44.90	752.0
46.20	65.0
46.90	791.0
48.00	449.0
49.00	2976.0
50.00	12858.0
51.00	3815.0
51.90	165.0
53.00	58.0
55.10	281.0
56.00	1103.0
57.00	2054.0
58.00	87.0
59.00	157.0
60.00	655.0
61.00	3278.0
62.00	3370.0
63.00	2400.0
64.00	179.0
64.90	144.0
66.80	212.0
68.00	7078.0
69.00	6813.0
70.00	599.0
71.00	60.0
72.10	354.0
73.00	3797.0
74.00	11781.0
75.00	33936.0
76.00	2670.0
77.00	392.0
77.90	308.0
78.90	2089.0
79.90	596.0
80.90	2326.0
81.90	573.0
83.10	69.0
86.20	101.0
86.90	2755.0
87.90	2567.0
90.90	272.0
92.00	1796.0
93.00	2923.0
94.00	7798.0
95.00	64168.0
96.00	4124.0
96.90	128.0
103.00	244.0
103.80	371.0
104.90	113.0
105.80	291.0
106.90	88.0
109.90	117.0
110.80	99.0
112.00	95.0
113.00	58.0
114.80	140.0
116.00	320.0
116.90	467.0
117.90	436.0
118.90	542.0
124.90	273.0
125.90	73.0
127.90	249.0
128.90	130.0
130.00	273.0
130.80	133.0
133.00	737.0
134.90	224.0
136.90	155.0
140.90	631.0
141.90	120.0
142.90	710.0
144.80	56.0
145.10	55.0
145.90	92.0
146.80	143.0
148.00	202.0
148.80	119.0
149.70	60.0
152.80	53.0
155.00	156.0
156.90	101.0
158.80	101.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

160.80	119.0
162.90	166.0
164.70	108.0
170.90	60.0
172.00	236.0
173.90	53744.0
174.90	4577.0
175.90	52992.0
176.90	3739.0
177.90	180.0
179.00	208.0
189.00	100.0
190.90	779.0
192.00	315.0
192.90	1119.0
194.00	188.0
195.00	160.0
203.00	98.0
204.90	201.0
207.00	794.0
207.90	152.0
208.80	72.0
234.80	113.0
248.90	881.0
250.90	246.0
251.90	91.0
252.80	59.0
264.90	951.0
265.90	297.0
267.00	204.0
278.40	78.0
281.00	13337.0
282.00	3427.0
283.00	2090.0
284.10	402.0
285.00	233.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03

Scan 1749 (12.567 min): VW015511.D
BFB03

m/z	Abundance
39.80	115.0
41.00	68.0
43.90	308.0
57.00	97.0
207.00	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB03