

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW053019\
 Data File : VW010607.D
 Acq On : 30 May 2019 11:21
 Operator : SY/VA
 Sample : VW0530SBL01
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0530SBL01

Quant Time: May 31 07:56:41 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 21 06:38:43 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	116092	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	203195	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	176067	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	76884	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	61111	51.00	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.00%	
35) Dibromofluoromethane	7.88	113	59220	48.03	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.06%	
50) Toluene-d8	10.32	98	244706	51.95	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.90%	
62) 4-Bromofluorobenzene	12.62	95	87302	46.53	ug/l	0.00
Spiked Amount	50.000		Recovery	=	93.06%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW053019\
Data File : VW010607.D
Acq On : 30 May 2019 11:21
Operator : SY/VA
Sample : VW0530SBL01
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0530SBL01

Quant Time: May 31 07:56:41 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
Quant Title : SW846 8260
QLast Update : Tue May 21 06:38:43 2019
Response via : Initial Calibration

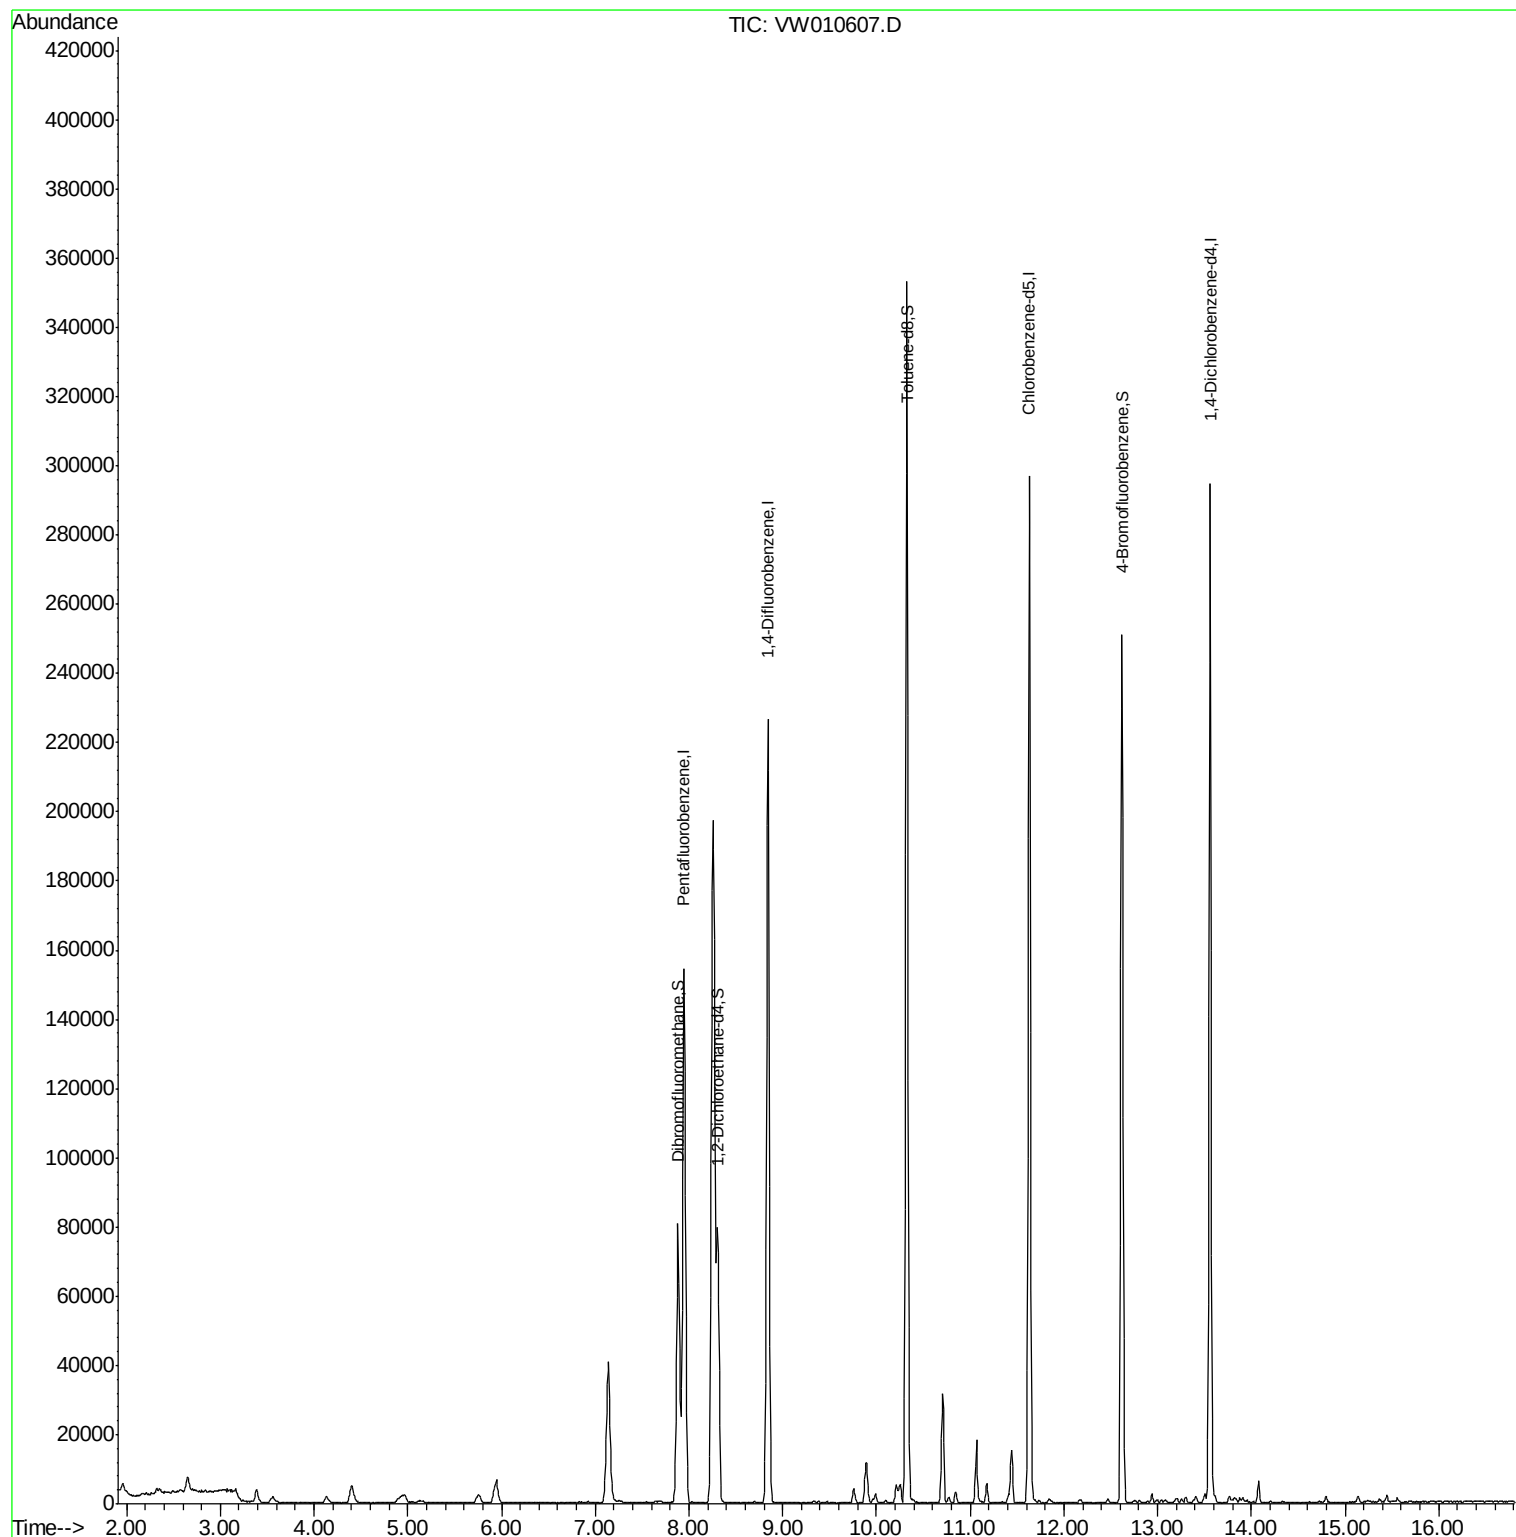

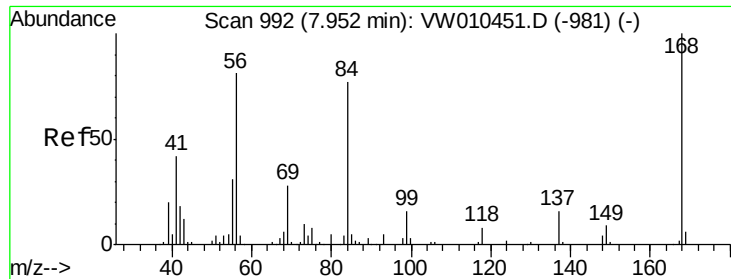

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.01 min

Lab File: VW010607.D

Acq: 30 May 2019 11:21

Instrument :

MSVOA_W

ClientSampleId :


VW0530SBL01

Tot Ion:168 Resp: 116092

Ion Ratio Lower Upper

168 100

99 59.2 46.1 69.1

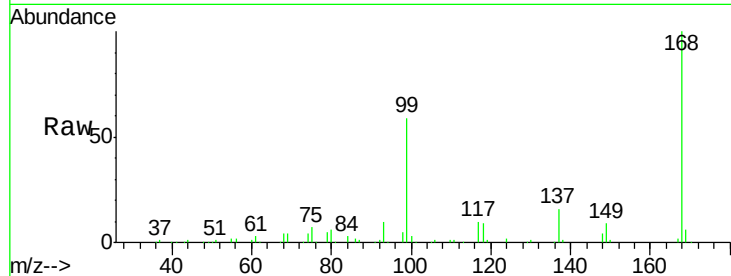

Abundance Ion 167.90 (167.60 to 168.60): VW

Ion 98.90 (98.60 to 99.60): VW

7.95

60000

50000

40000

30000



20000

10000

0

7.90 8.00 8.10

Time-->

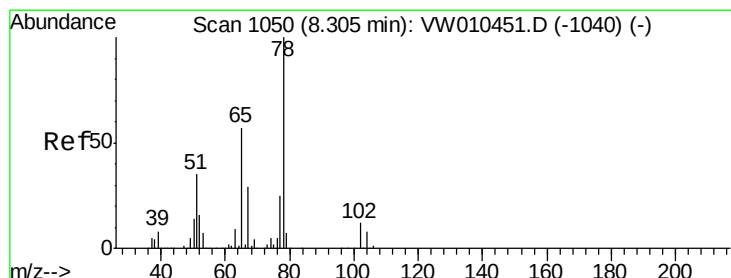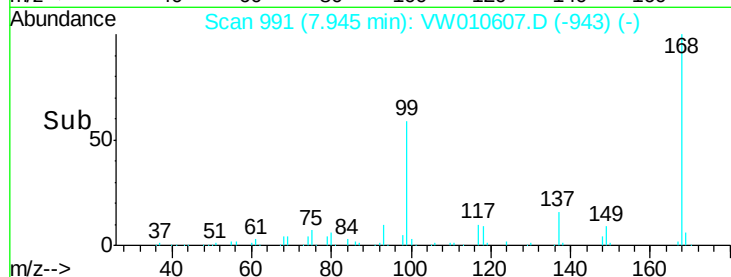

#33

1,2-Dichloroethane-d4

Concen: 50.999 ug/l

RT: 8.30 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW010607.D


Acq: 30 May 2019 11:21

Tgt Ion: 65 Resp: 61111

Ion Ratio Lower Upper

65 100

67 52.3 0.0 103.6

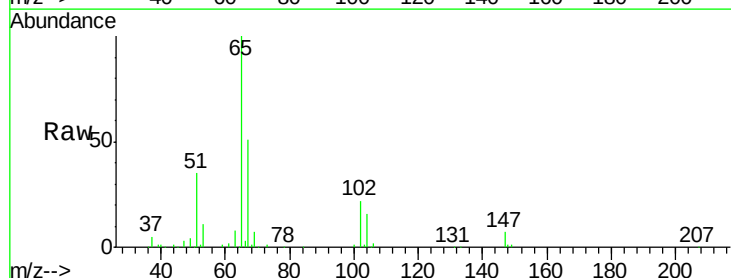

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.30

30000

25000

20000

15000


10000


5000

0

8.20 8.30 8.40

Time-->

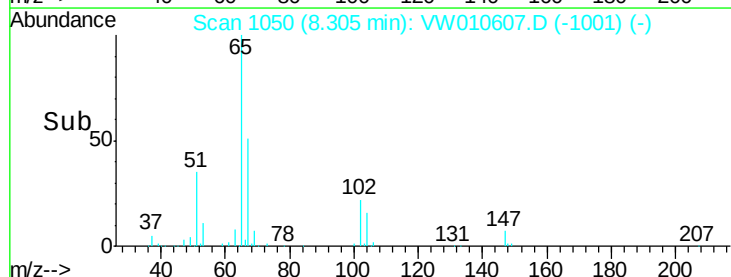

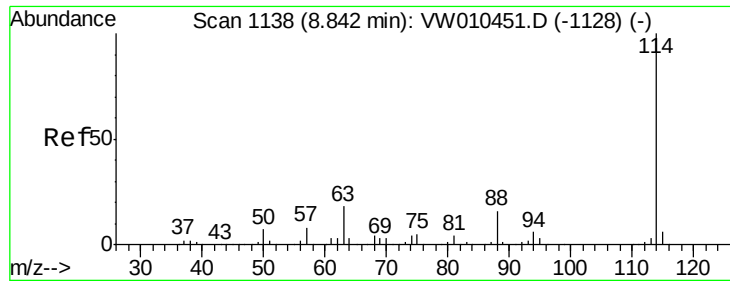

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. -0.00 min

Lab File: VW010607.D

Acq: 30 May 2019 11:21

Instrument :

MSVOA_W

ClientSampleId :

VW0530SBL01


Tot Ion:114 Resp: 203195

Ion Ratio Lower Upper

114 100

63 18.2 0.0 36.0




88 15.5 0.0 32.0

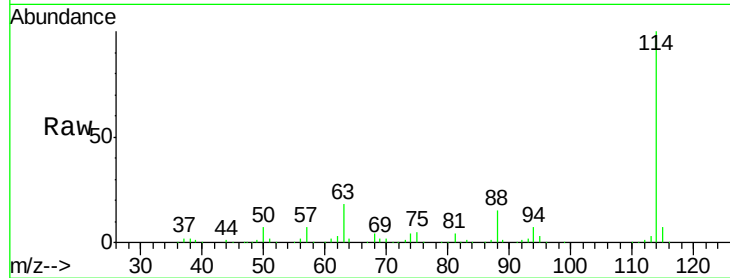

Abundance Ion 113.90 (113.60 to 114.60): V

Ion 63.00 (62.70 to 63.70): VW

Ion 87.90 (87.60 to 88.60): VW

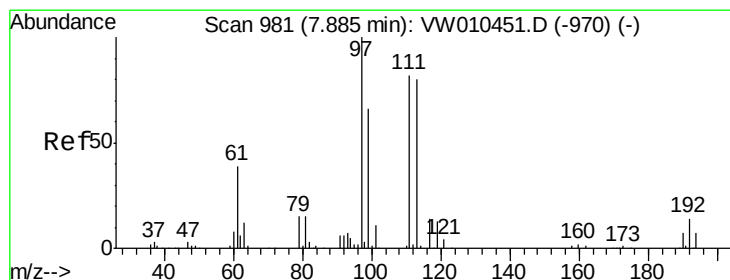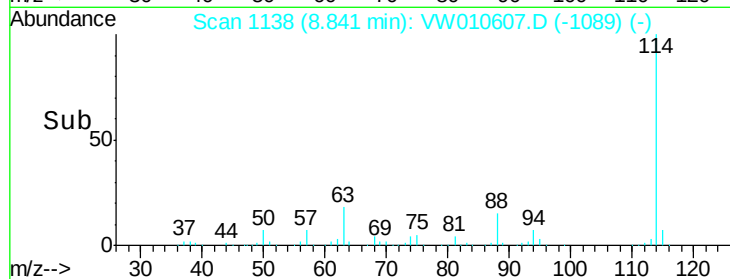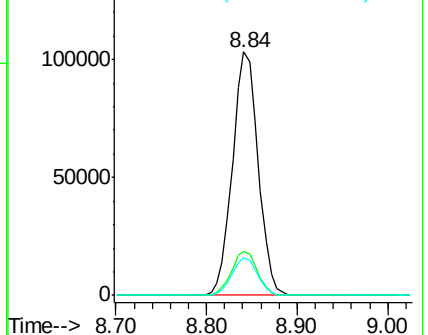

#35

Dibromofluoromethane

Concen: 48.031 ug/l

RT: 7.88 min Scan# 981

Delta R.T. -0.00 min

Lab File: VW010607.D

Acq: 30 May 2019 11:21


Tgt Ion:113 Resp: 59220

Ion Ratio Lower Upper

113 100

111 104.7 82.2 123.4



192 18.4 14.3 21.5

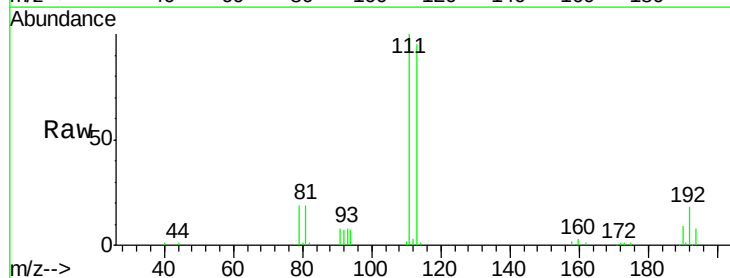


Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

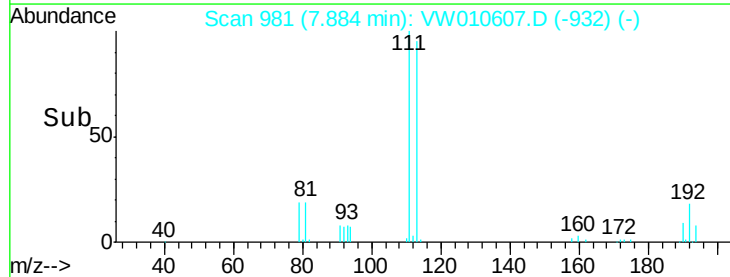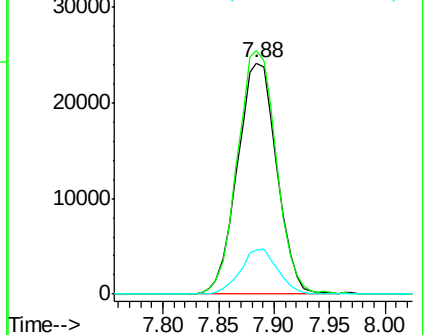

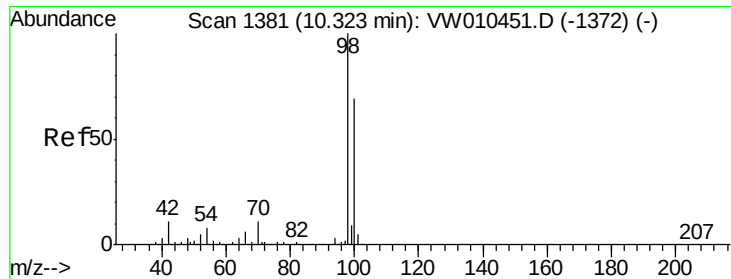

#50

Toluene-d8

Concen: 51.953 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW010607.D

Acq: 30 May 2019 11:21

Instrument :

MSVOA_W

ClientSampleId :





VW0530SBL01

Tot Ion: 98 Resp: 244706

Ion Ratio Lower Upper

98 100

100 67.5 53.7 80.5

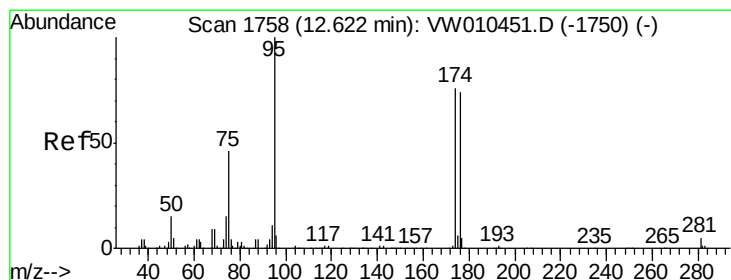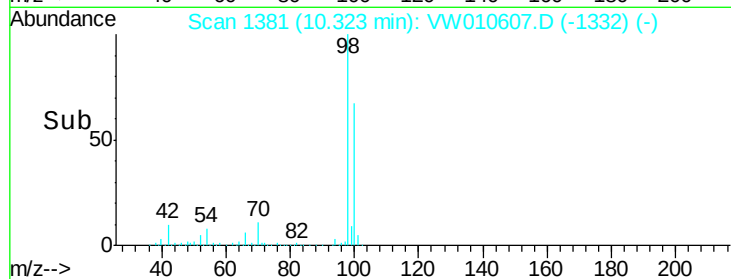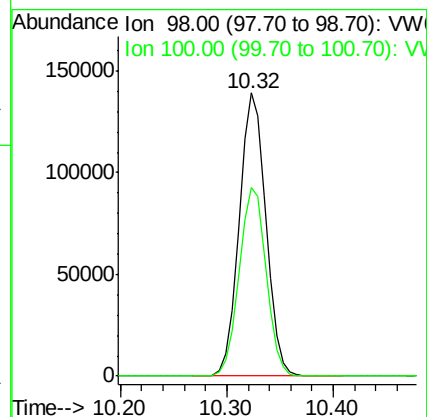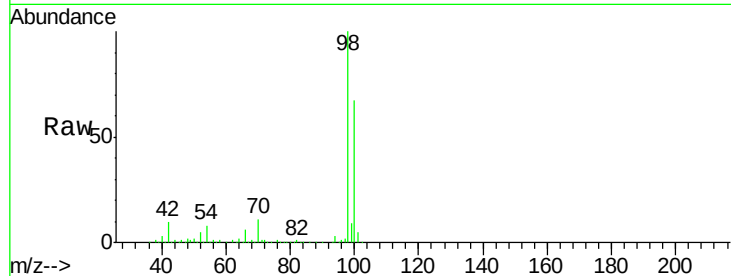

#62

4-Bromofluorobenzene

Concen: 46.533 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. -0.00 min

Lab File: VW010607.D

Acq: 30 May 2019 11:21




Tgt Ion: 95 Resp: 87302


Ion Ratio Lower Upper

95 100

174 72.4 0.0 148.6

176 70.6 0.0 144.2

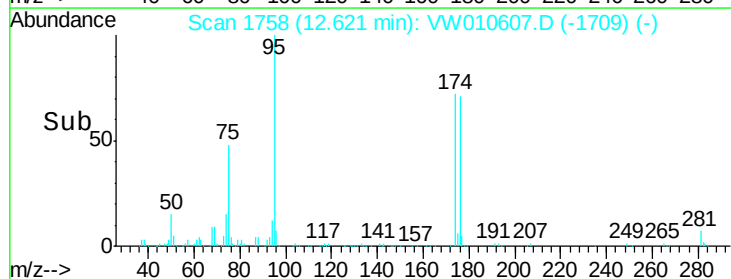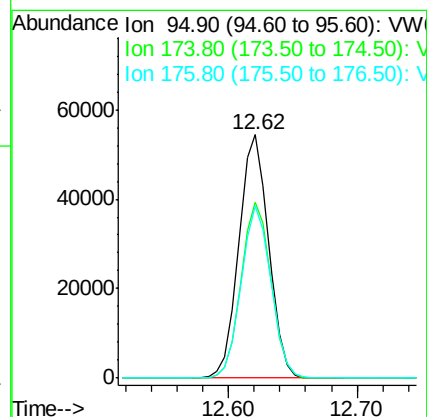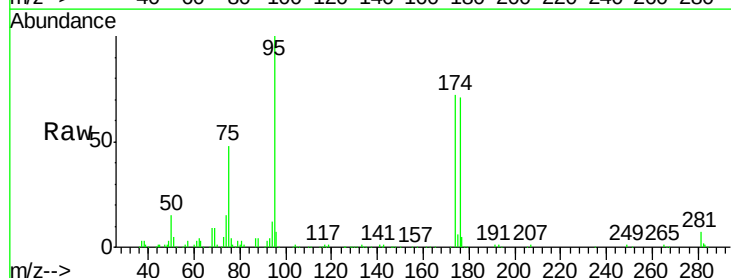


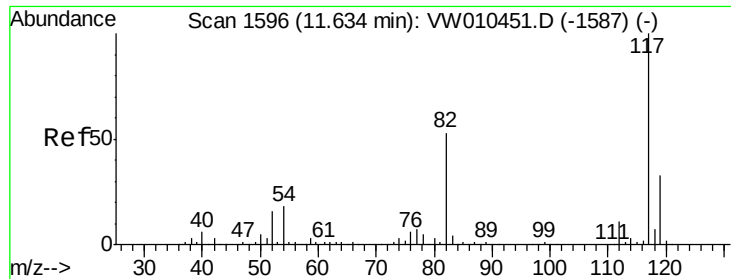




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW010607.D
Acq: 30 May 2019 11:21

Instrument :
MSVOA_W
ClientSampleId :
VW0530SBL01

Tot Ion:117 Resp: 176067
Ion Ratio Lower Upper
117 100
82 51.8 42.8 64.2
119 32.3 26.3 39.5

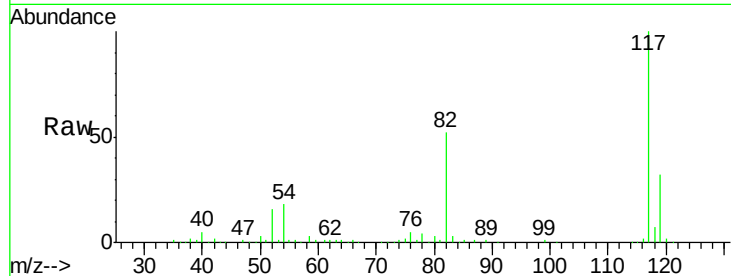


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

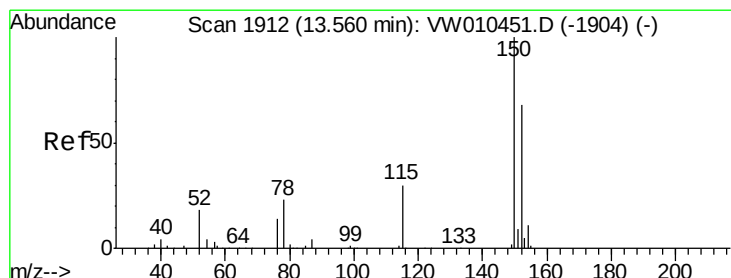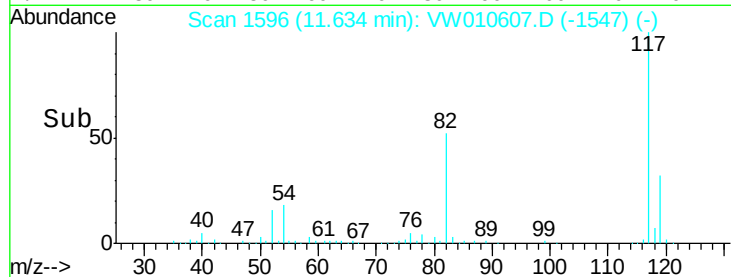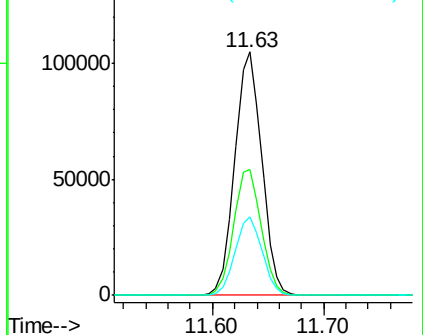

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW010607.D
Acq: 30 May 2019 11:21

Tgt Ion:152 Resp: 76884
Ion Ratio Lower Upper
152 100
115 61.6 30.3 91.0
150 157.2 0.0 349.8

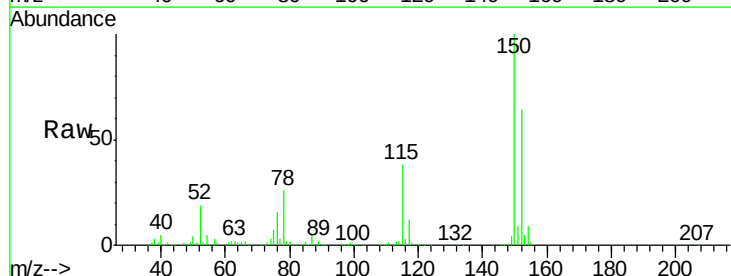

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

