


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW053019\
Data File : VW010605.D
Acq On : 30 May 2019 09:27
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
Title : SW846 8260
Last Update : Tue May 21 06:38:43 2019

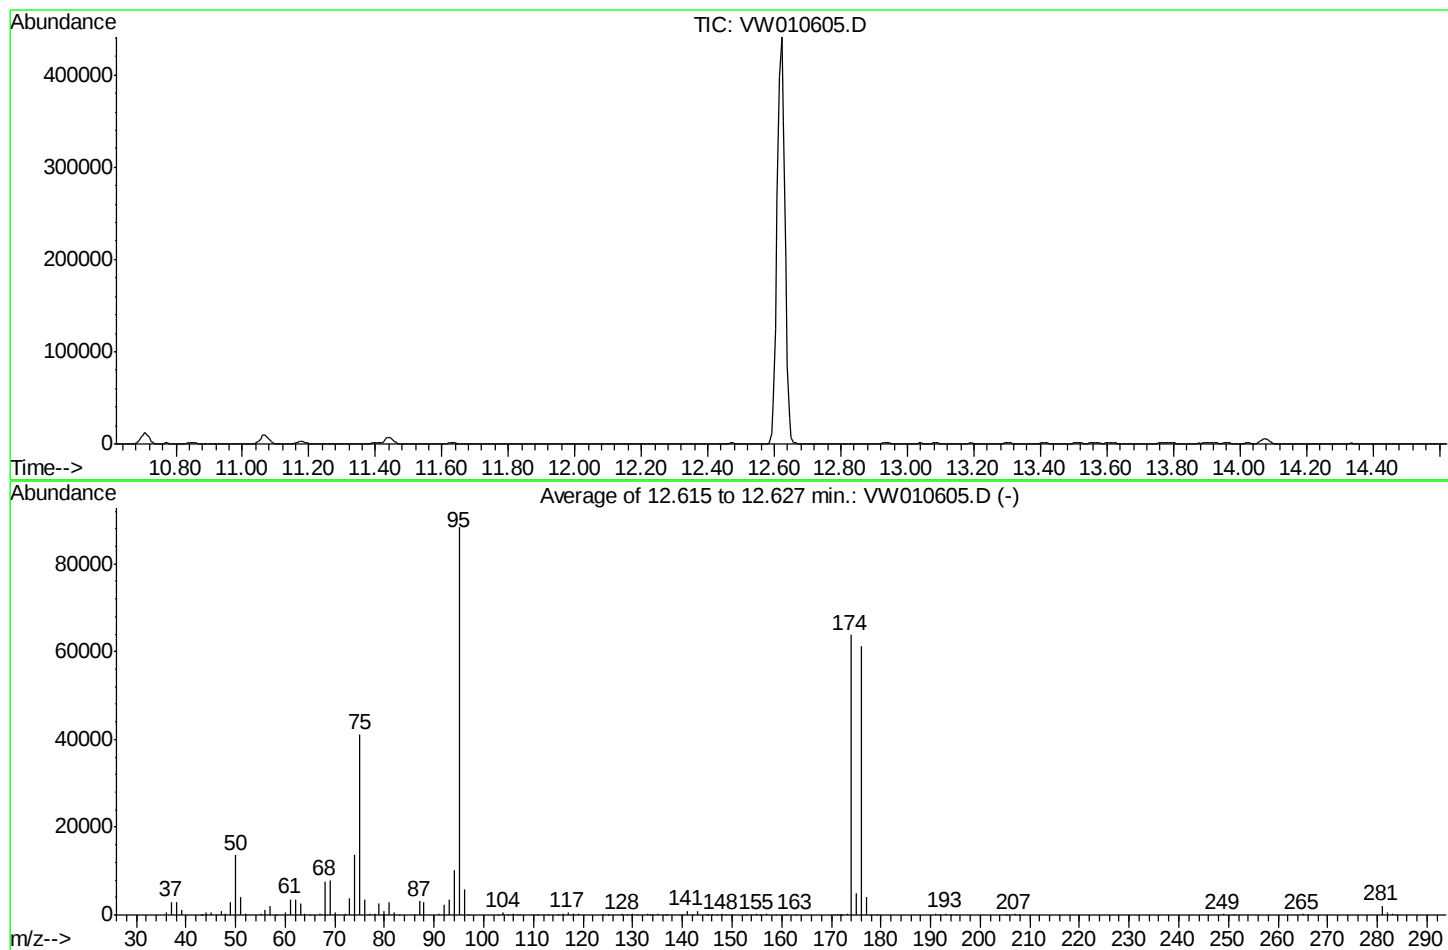

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.4	13634	PASS
75	95	30	60	46.5	41096	PASS
95	95	100	100	100.0	88330	PASS
96	95	5	9	6.7	5938	PASS
173	174	0.00	2	0.5	323	PASS
174	95	50	100	72.2	63778	PASS
175	174	5	9	7.9	5063	PASS
176	174	95	101	96.2	61378	PASS
177	176	5	9	6.5	4003	PASS