


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW053119\
 Data File : VW010628.D
 Acq On : 31 May 2019 10:12
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W052019S.M
 Title : SW846 8260
 Last Update : Tue May 21 06:38:43 2019

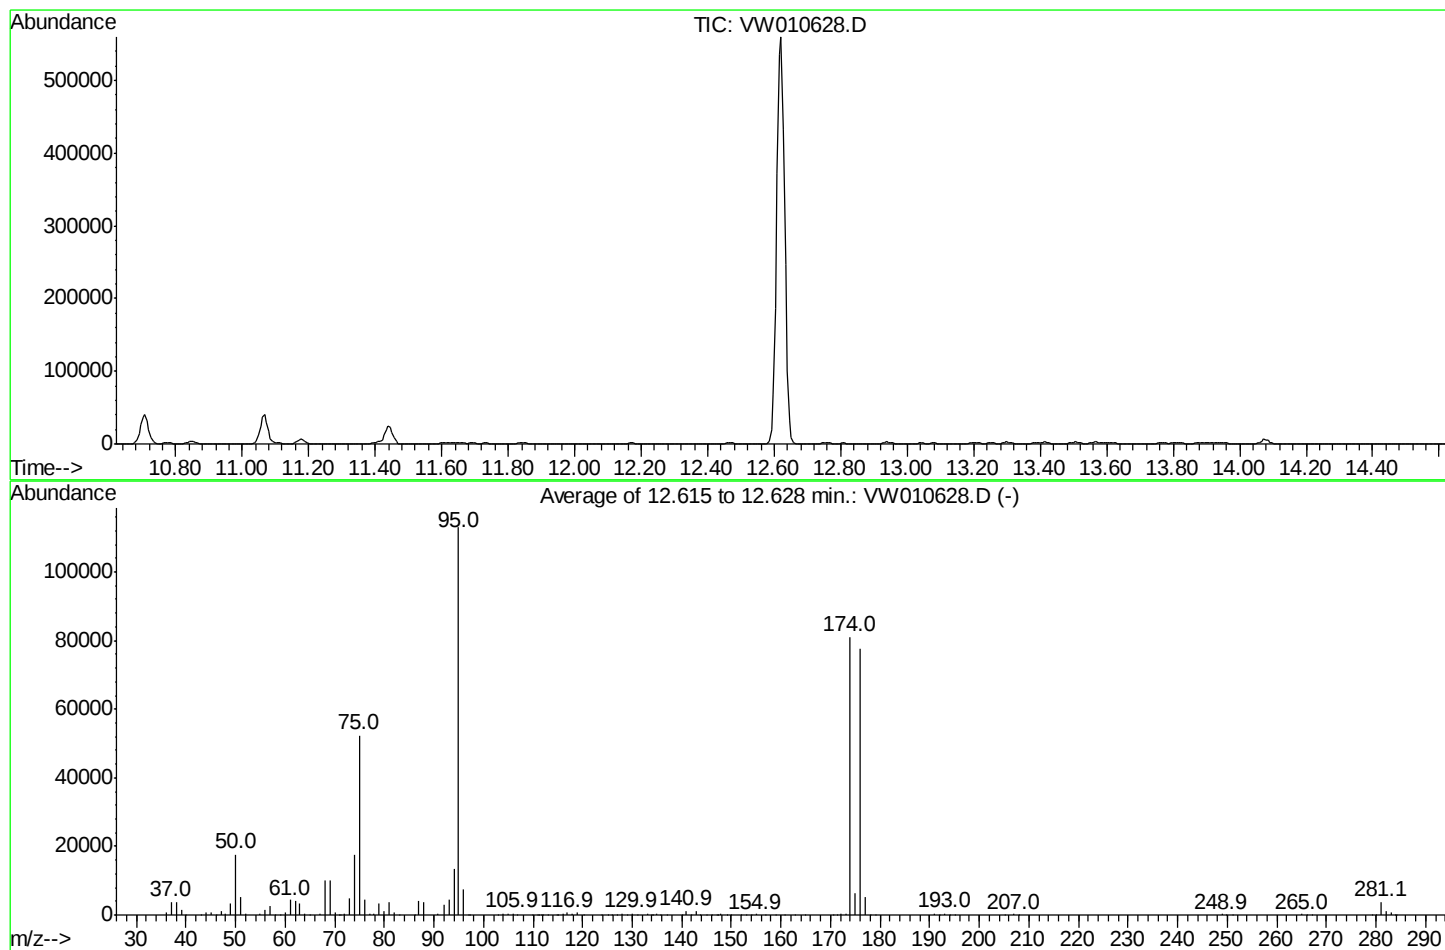

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	17739	PASS
75	95	30	60	46.4	52397	PASS
95	95	100	100	100.0	113018	PASS
96	95	5	9	6.6	7504	PASS
173	174	0.00	2	0.5	417	PASS
174	95	50	100	71.8	81117	PASS
175	174	5	9	7.9	6379	PASS
176	174	95	101	95.9	77784	PASS
177	176	5	9	6.9	5395	PASS